

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
 Data File : BF136195.D
 Acq On : 25 Nov 2023 00:06
 Operator : CG\JU
 Sample : PB157124TB
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157124TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.440	394	400	408	rBV	69163	87247	1.16%	0.200%
2	5.063	498	506	517	rVB	401921	618041	8.20%	1.417%
3	5.451	566	572	575	rBV	5556109	5966575	79.18%	13.684%
4	6.445	734	741	744	rBV	4962147	5814389	77.16%	13.335%
5	6.804	799	802	806	rVB	1277672	1059311	14.06%	2.429%
6	7.369	892	898	901	rBV	3605398	3663709	48.62%	8.403%
7	8.081	1015	1019	1023	rBV	1728461	1546982	20.53%	3.548%
8	9.163	1197	1203	1206	rBV	7704213	7535829	100.00%	17.283%
9	9.839	1312	1318	1321	rBV	2339998	1812701	24.05%	4.157%
10	10.633	1448	1453	1456	rBV	4725962	4253332	56.44%	9.755%
11	11.328	1567	1571	1575	rBV	2224516	1854786	24.61%	4.254%
12	12.933	1839	1844	1847	rBV	7793524	7219735	95.81%	16.558%
13	13.980	2018	2022	2025	rBV	1279703	1125973	14.94%	2.582%
14	15.463	2268	2274	2281	rBV	803688	1043810	13.85%	2.394%




Sum of corrected areas: 43602420

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136195.D
Acq On : 25 Nov 2023 00:06
Operator : CG\JU
Sample : PB157124TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157124TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

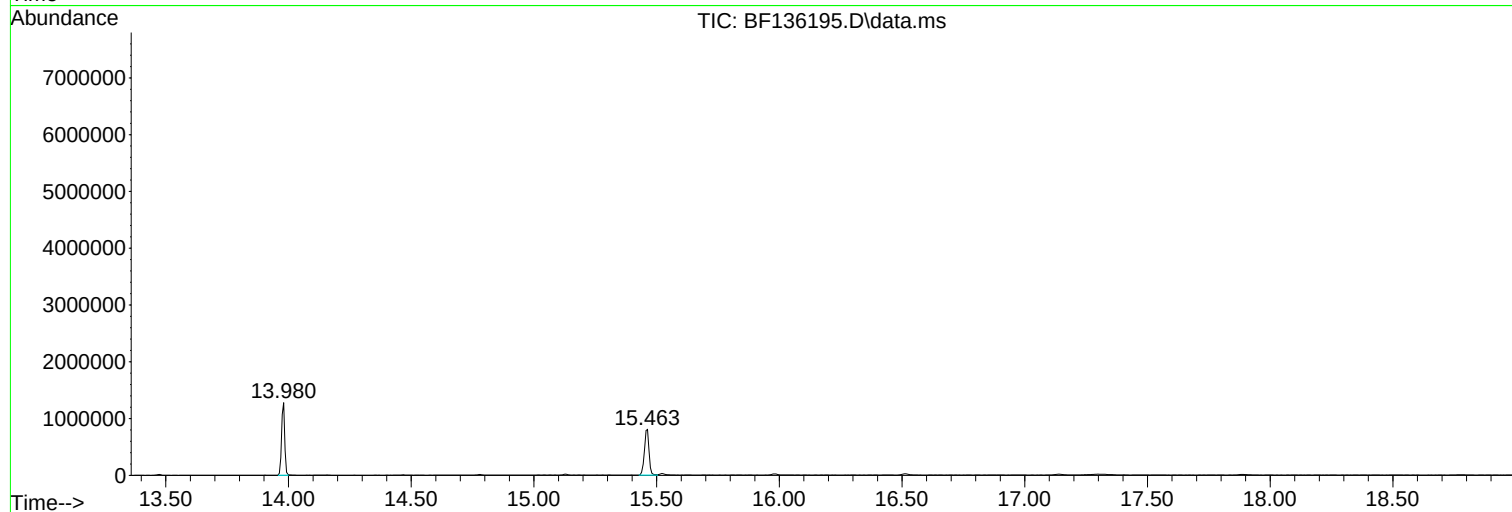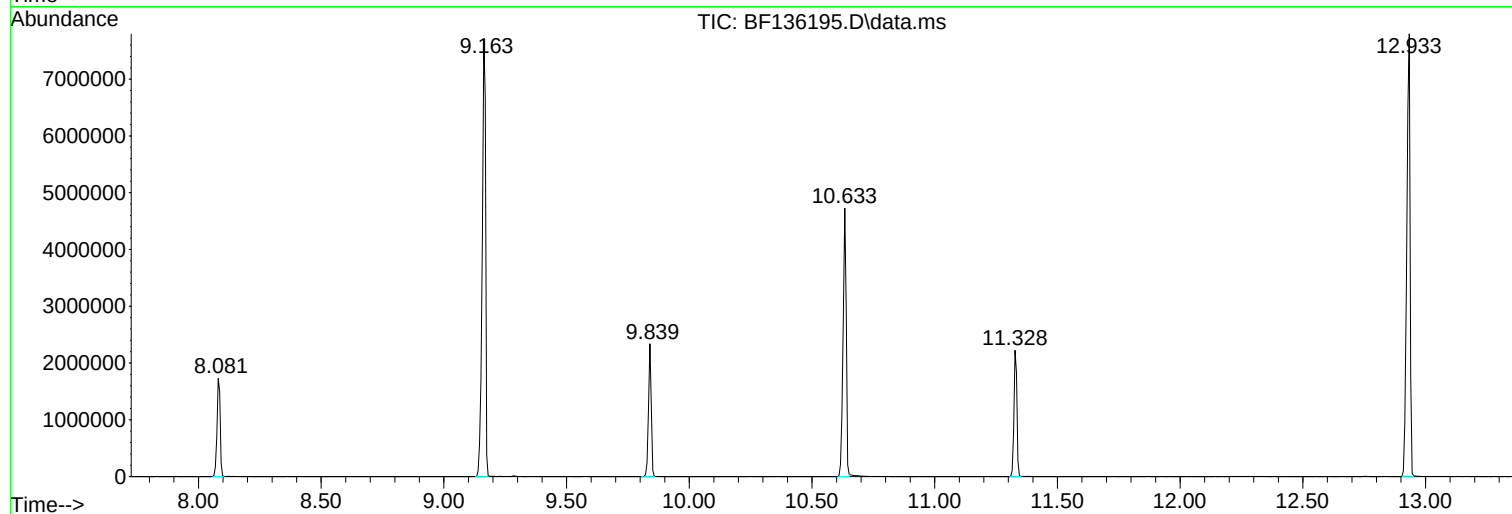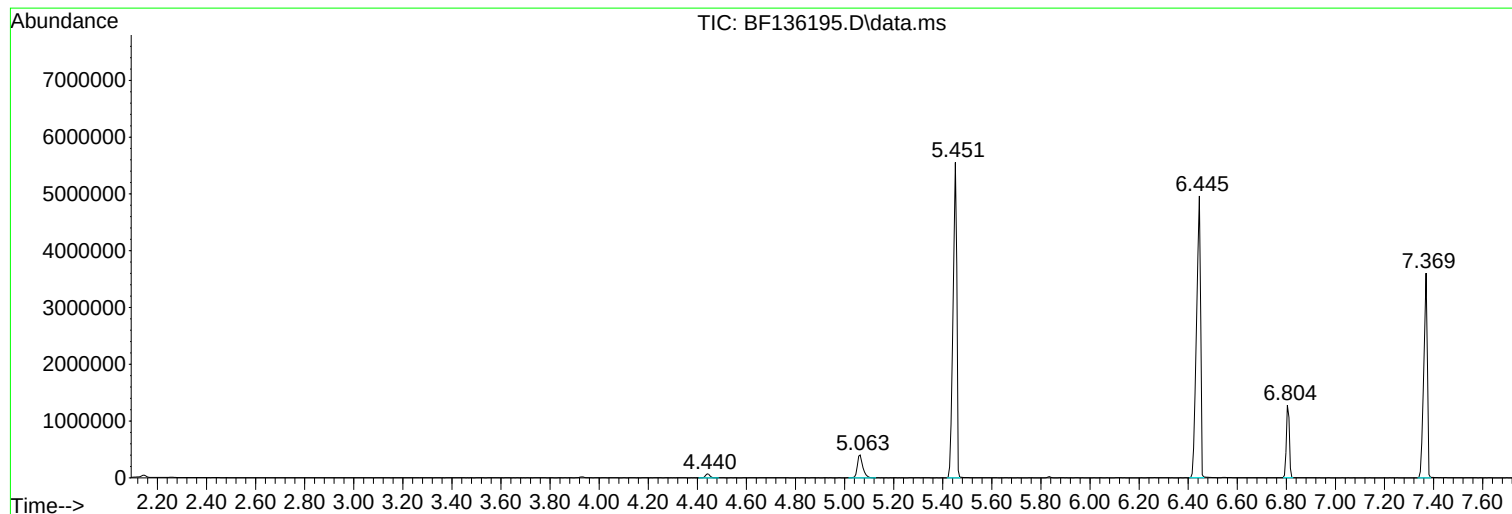

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136195.D
Acq On : 25 Nov 2023 00:06
Operator : CG\JU
Sample : PB157124TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157124TB










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.063	11.67 ng	618041	1,4-Dichlorobenzene-d4	6.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	37		
3	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		

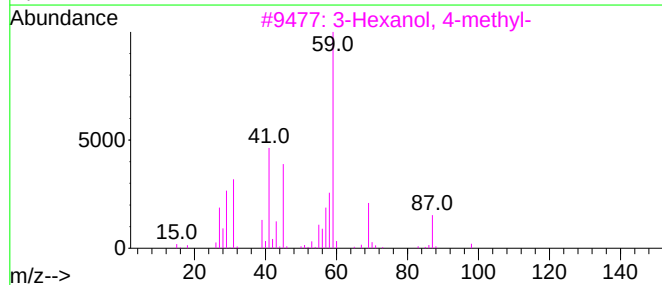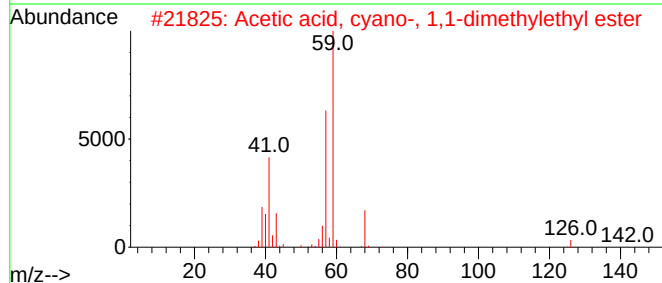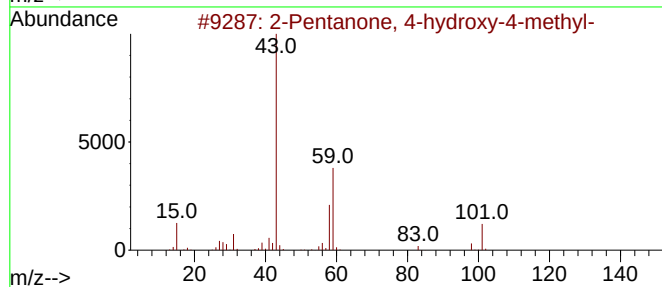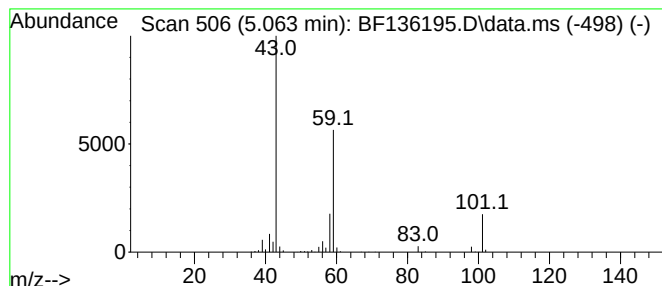

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136195.D
Acq On : 25 Nov 2023 00:06
Operator : CG\JU
Sample : PB157124TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157124TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.063	11.7	ng	618041	1	6.804	1059310	20.0