

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
 Data File : BF136196.D
 Acq On : 25 Nov 2023 00:39
 Operator : CG\JU
 Sample : PB157264BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157264BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	565	570	573	rBV	3456105	3519771	76.19%	13.275%
2	6.439	734	740	743	rBV	3543345	3394354	73.47%	12.802%
3	6.804	799	802	806	rBV	957644	753303	16.31%	2.841%
4	7.369	892	898	900	rBV	2252873	2185964	47.32%	8.245%
5	8.081	1015	1019	1023	rBV	1338764	1057802	22.90%	3.990%
6	9.163	1198	1203	1206	rBV	5714149	4619995	100.00%	17.425%
7	9.839	1314	1318	1321	rBV	1611757	1225886	26.53%	4.624%
8	10.627	1448	1452	1456	rBV	2713906	2433504	52.67%	9.178%
9	11.327	1568	1571	1575	rBV	1548276	1225604	26.53%	4.623%
10	12.927	1839	1843	1846	rBV	5308866	4603168	99.64%	17.361%
11	13.980	2018	2022	2031	rBV	823080	772737	16.73%	2.914%
12	15.457	2268	2273	2281	rBV	597096	721613	15.62%	2.722%




Sum of corrected areas: 26513701

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136196.D
Acq On : 25 Nov 2023 00:39
Operator : CG\JU
Sample : PB157264BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157264BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

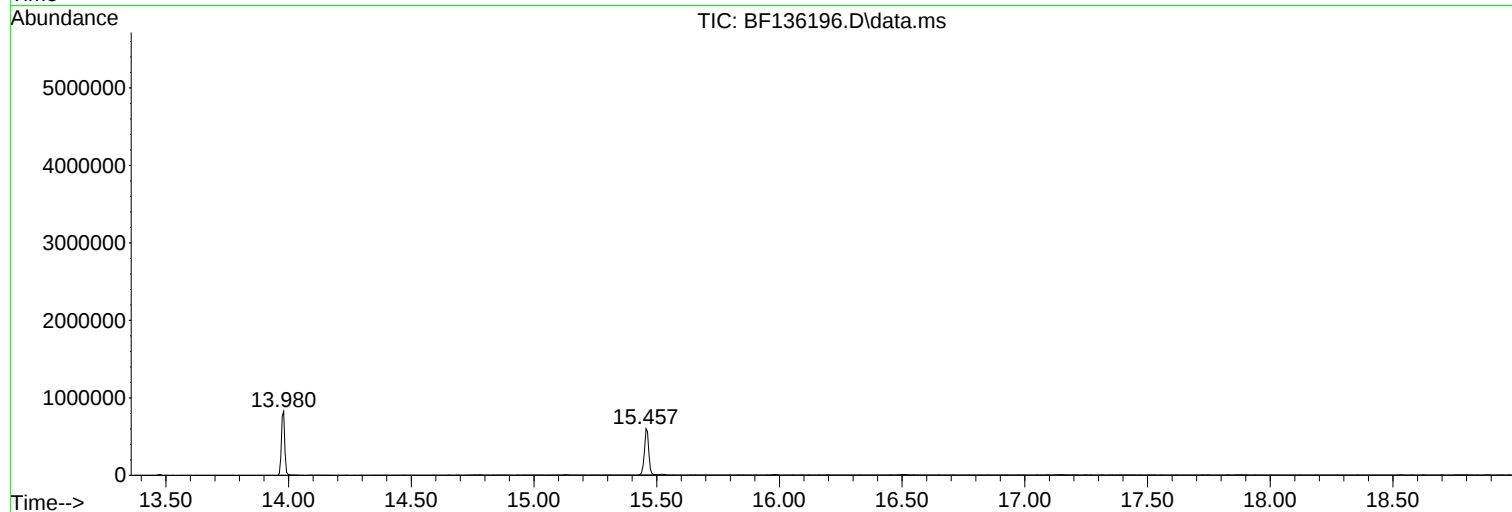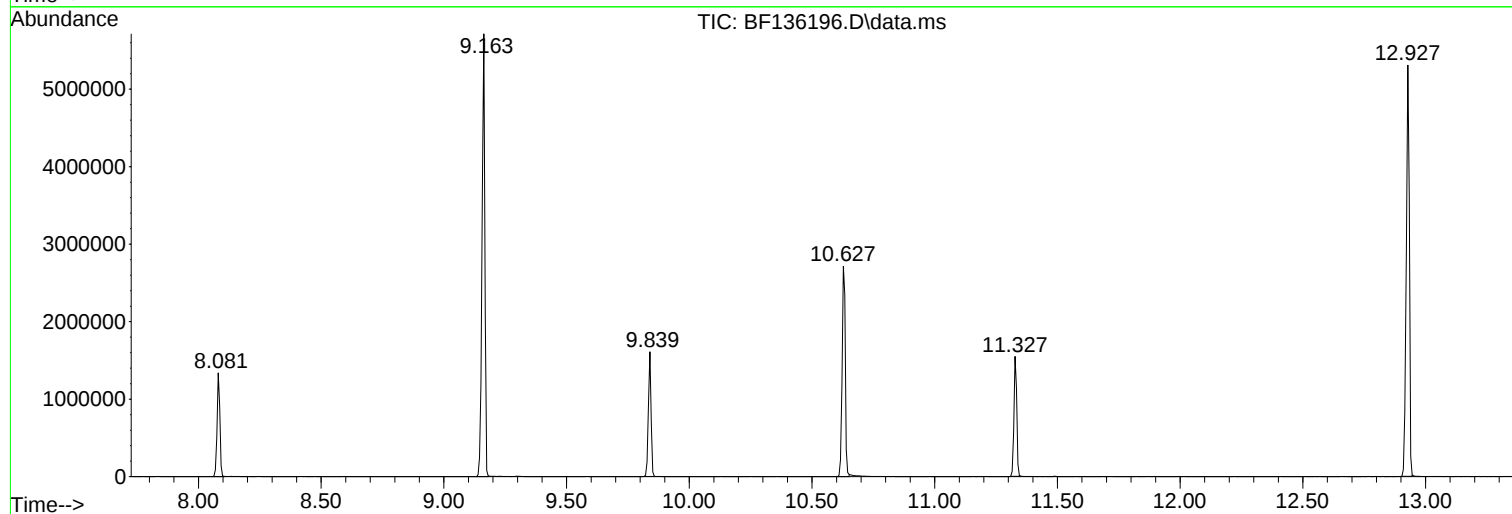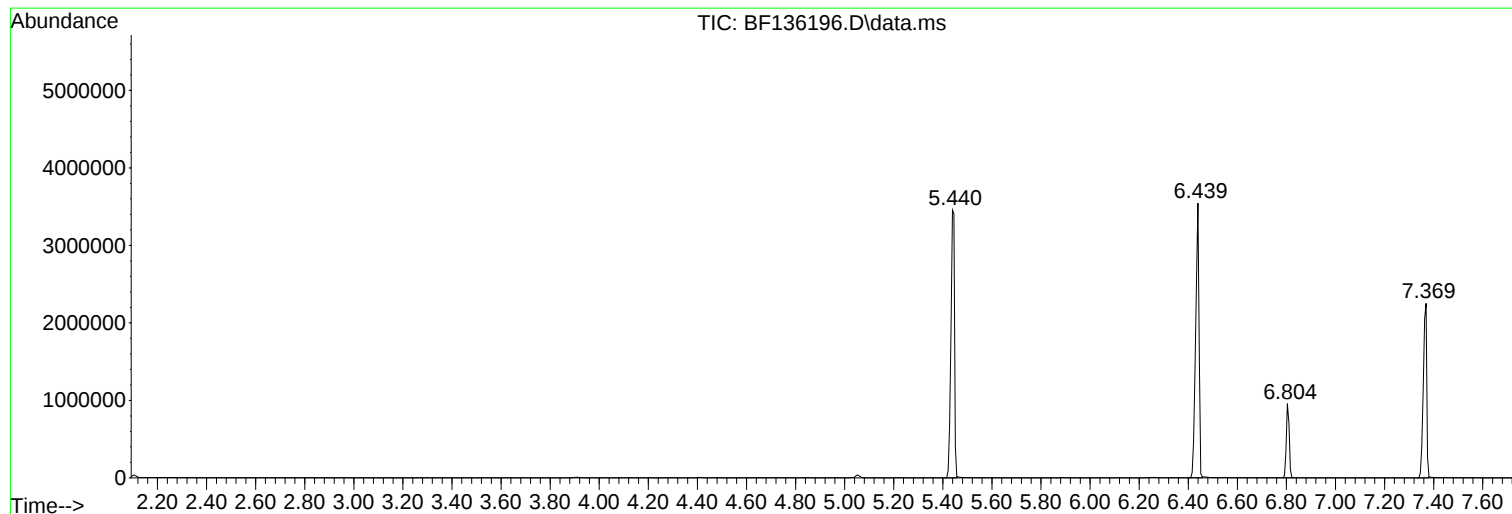

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136196.D
Acq On : 25 Nov 2023 00:39
Operator : CG\JU
Sample : PB157264BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157264BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136196.D
Acq On : 25 Nov 2023 00:39
Operator : CG\JU
Sample : PB157264BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157264BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------