

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
 Data File : BF136201.D
 Acq On : 25 Nov 2023 03:24
 Operator : CG\JU
 Sample : PB157233BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157233BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.445	566	571	574	rBV	4050813	4336403	76.03%	13.589%
2	6.440	734	740	743	rBV	3860744	4221007	74.00%	13.227%
3	6.804	799	802	806	rVB	1102598	840275	14.73%	2.633%
4	7.369	892	898	901	rBV	2766861	2711062	47.53%	8.496%
5	8.081	1014	1019	1023	rBV	1312733	1173905	20.58%	3.679%
6	9.163	1197	1203	1206	rBV	6686107	5703902	100.00%	17.874%
7	9.839	1312	1318	1321	rBV	1774553	1357442	23.80%	4.254%
8	10.633	1448	1453	1456	rBV	3260023	2988978	52.40%	9.367%
9	11.327	1567	1571	1575	rBV	1691391	1375555	24.12%	4.311%
10	12.927	1838	1843	1846	rBV	5874291	5581261	97.85%	17.490%
11	13.980	2018	2022	2025	rBV	923486	850536	14.91%	2.665%
12	15.457	2267	2273	2281	rBV	624604	770829	13.51%	2.416%




Sum of corrected areas: 31911155

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136201.D
Acq On : 25 Nov 2023 03:24
Operator : CG\JU
Sample : PB157233BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157233BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

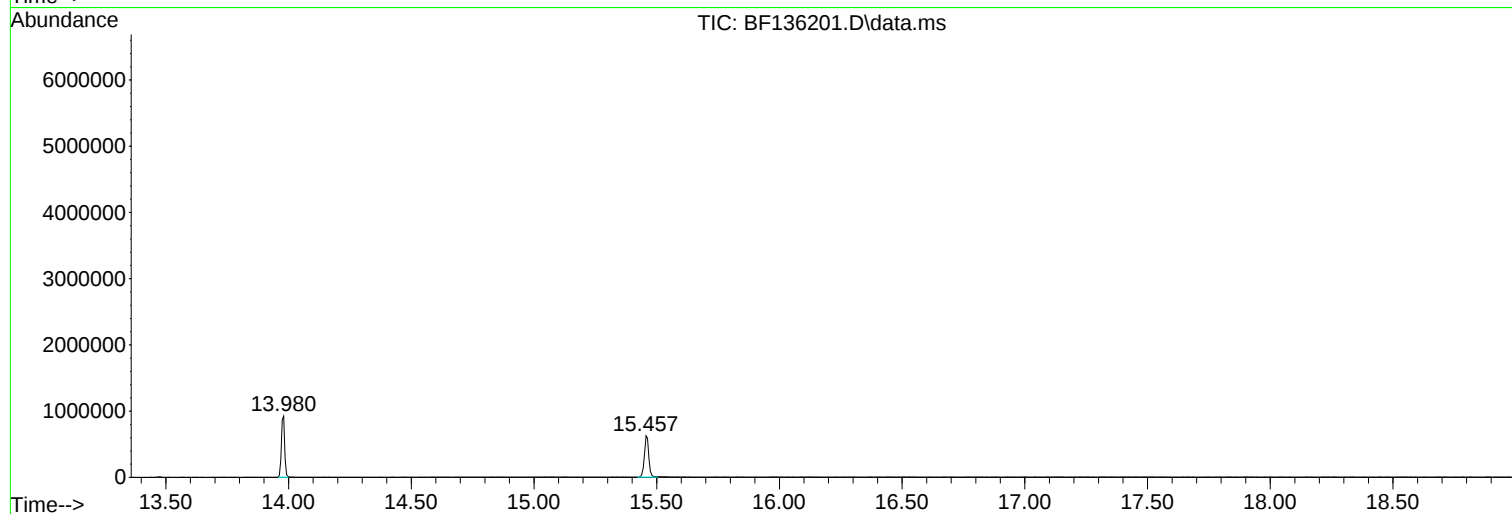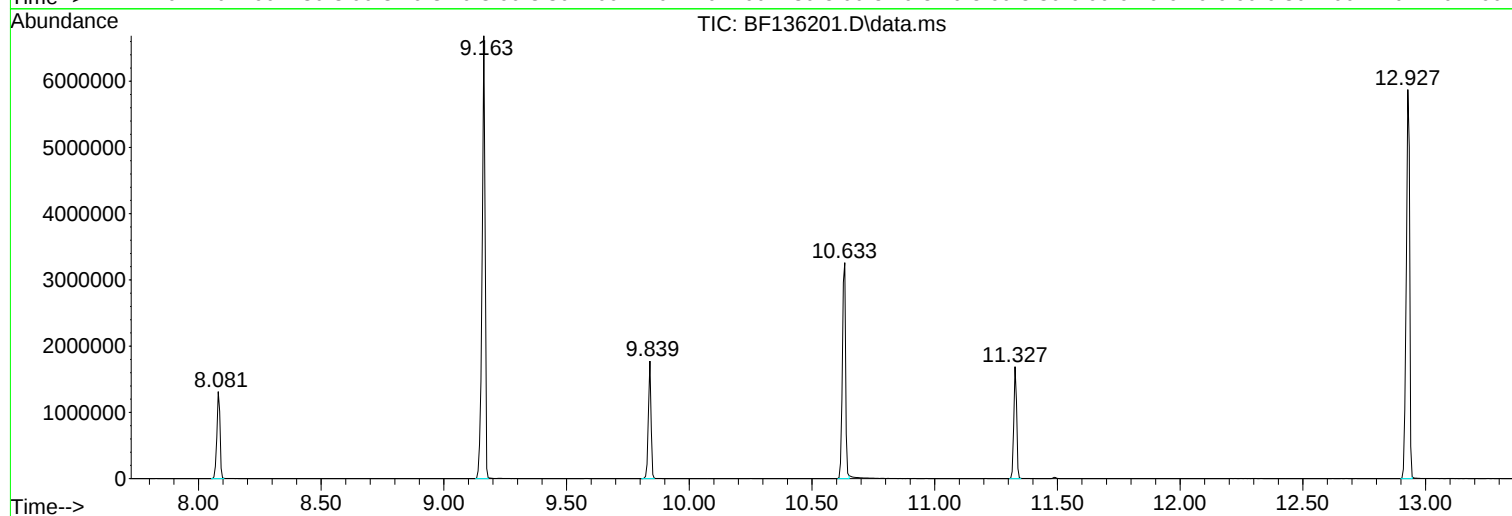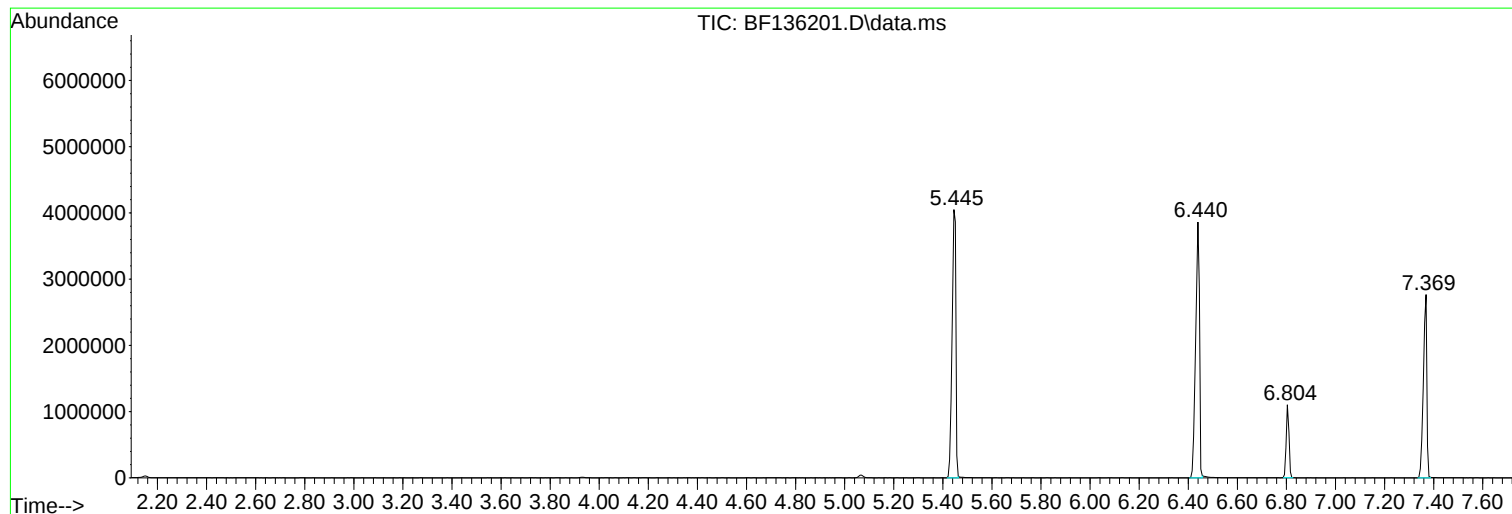

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136201.D
Acq On : 25 Nov 2023 03:24
Operator : CG\JU
Sample : PB157233BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157233BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136201.D
Acq On : 25 Nov 2023 03:24
Operator : CG\JU
Sample : PB157233BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157233BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------