

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
 Data File : BF136206.D
 Acq On : 25 Nov 2023 06:07
 Operator : CG\JU
 Sample : 05418-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 STONE-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.852	124	130	137	rVB	294957	386833	7.57%	1.343%
2	4.646	431	435	440	rVB	144104	137235	2.69%	0.476%
3	4.710	440	446	454	rBV	107826	106940	2.09%	0.371%
4	5.057	500	505	507	rBV	269950	377422	7.39%	1.310%
5	5.075	507	508	512	rVB	247907	190009	3.72%	0.660%
6	5.451	567	572	575	rBV	3851618	3526466	69.02%	12.240%
7	6.440	735	740	743	rBV	3109247	3062042	59.93%	10.628%
8	6.804	799	802	806	rVB	948920	801981	15.70%	2.784%
9	7.369	892	898	901	rBV	2832189	2536290	49.64%	8.803%
10	8.081	1015	1019	1023	rBV	1349582	1107700	21.68%	3.845%
11	9.163	1198	1203	1206	rBV	6309342	5109570	100.00%	17.735%
12	9.839	1314	1318	1321	rBV	1646416	1279272	25.04%	4.440%
13	10.633	1448	1453	1456	rBV	2711519	2617441	51.23%	9.085%
14	11.327	1568	1571	1575	rBV	1545520	1255693	24.58%	4.358%
15	12.927	1838	1843	1846	rBV	5065733	4838866	94.70%	16.795%
16	13.980	2018	2022	2032	rBV	864779	767416	15.02%	2.664%
17	15.462	2268	2274	2282	rBV	574290	709640	13.89%	2.463%




Sum of corrected areas: 28810816

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136206.D
Acq On : 25 Nov 2023 06:07
Operator : CG\JU
Sample : 05418-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
STONE-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

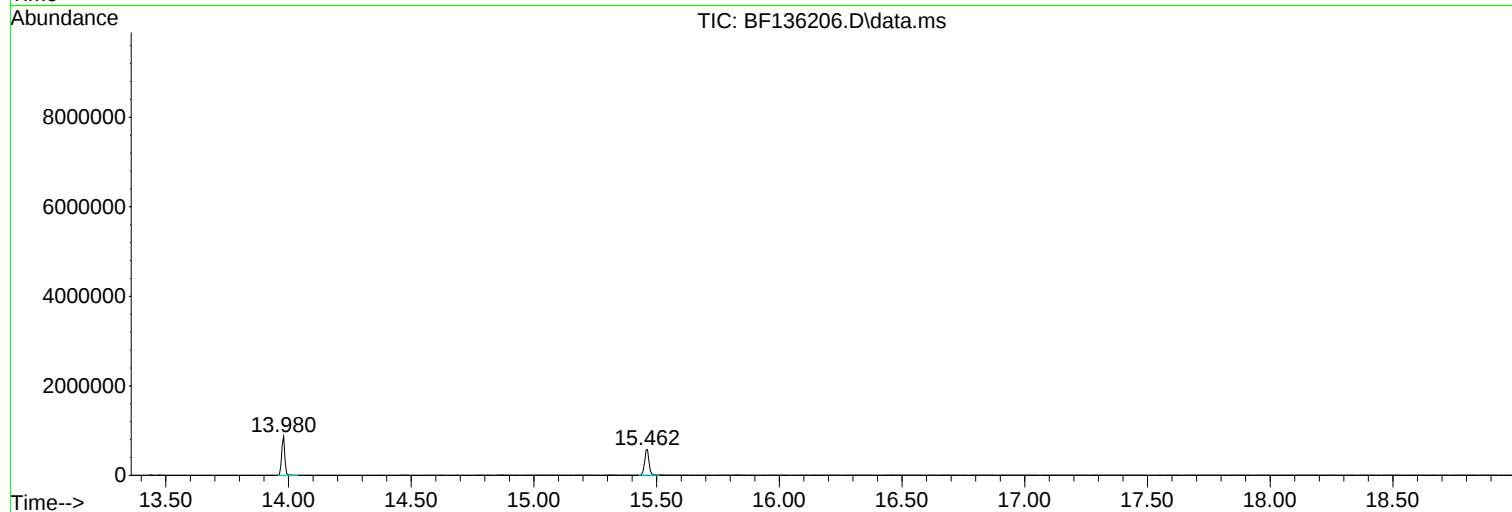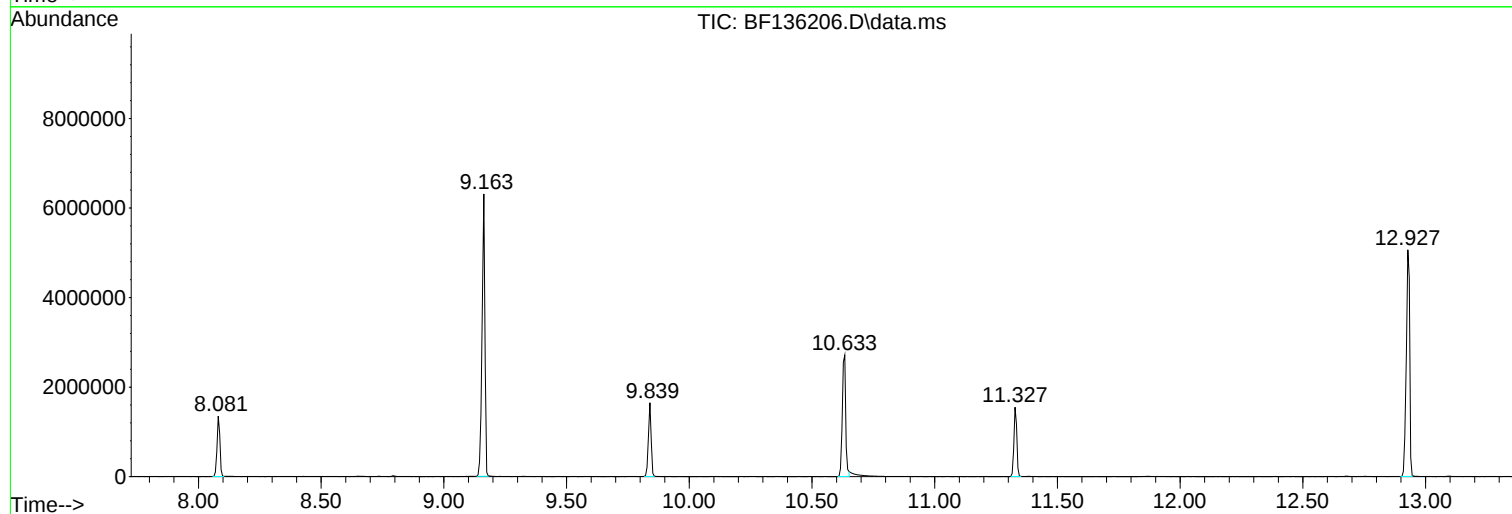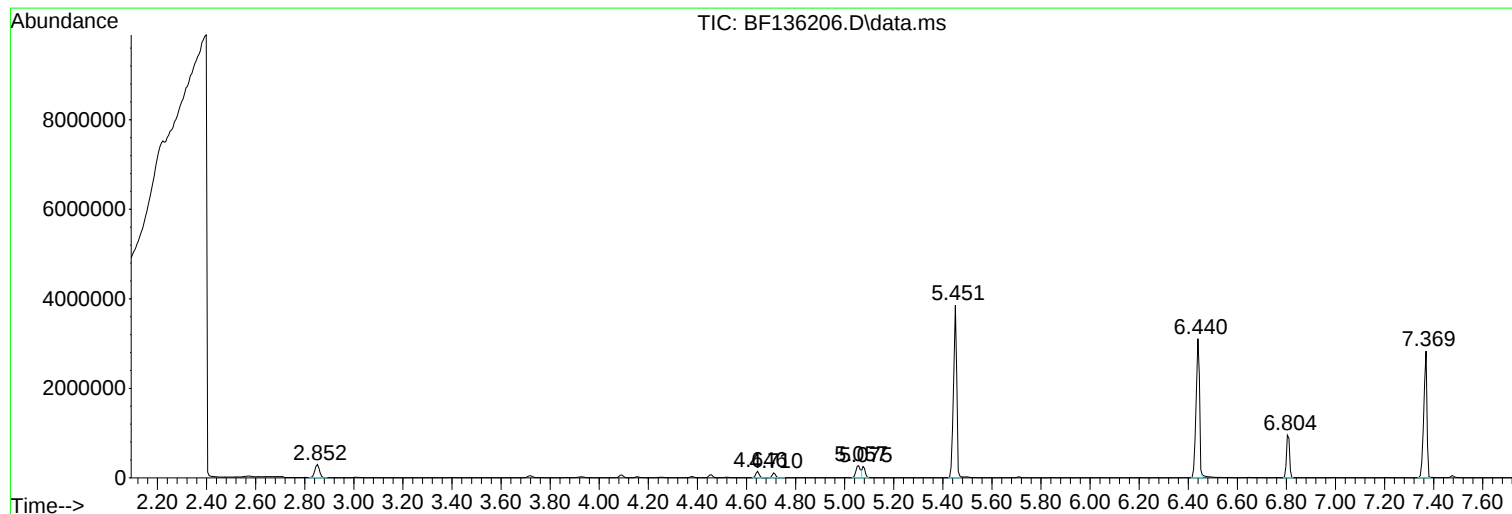

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136206.D
Acq On : 25 Nov 2023 06:07
Operator : CG\JU
Sample : 05418-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
STONE-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136206.D
Acq On : 25 Nov 2023 06:07
Operator : CG\JU
Sample : 05418-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
STONE-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------