

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
 Data File : BF136207.D
 Acq On : 25 Nov 2023 06:39
 Operator : CG\JU
 Sample : 05418-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 STONE-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136207.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.863	127	132	139	rVB	238525	314367	5.91%	1.047%
2	4.646	430	435	440	rBV	102352	110004	2.07%	0.366%
3	5.057	500	505	507	rBV	271399	335320	6.30%	1.116%
4	5.075	507	508	513	rVB2	202558	179995	3.38%	0.599%
5	5.451	567	572	575	rBV	3717478	3795601	71.31%	12.637%
6	6.440	735	740	743	rBV	3154078	3325724	62.48%	11.072%
7	6.804	799	802	806	rBV	1027609	859851	16.15%	2.863%
8	7.369	892	898	901	rBV	2944941	2644740	49.69%	8.805%
9	8.081	1015	1019	1023	rBV	1434634	1170256	21.99%	3.896%
10	9.163	1197	1203	1206	rBV	6427589	5322871	100.00%	17.721%
11	9.839	1313	1318	1321	rBV	1717049	1360162	25.55%	4.528%
12	10.633	1448	1453	1456	rBV	2907579	2774515	52.12%	9.237%
13	11.327	1567	1571	1575	rBV	1629883	1334412	25.07%	4.443%
14	12.927	1839	1843	1846	rBV	5362020	4948944	92.98%	16.476%
15	13.980	2018	2022	2033	rBV	924311	814187	15.30%	2.711%
16	15.462	2268	2274	2281	rBV	604267	745652	14.01%	2.482%




Sum of corrected areas: 30036601

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136207.D
Acq On : 25 Nov 2023 06:39
Operator : CG\JU
Sample : 05418-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
STONE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

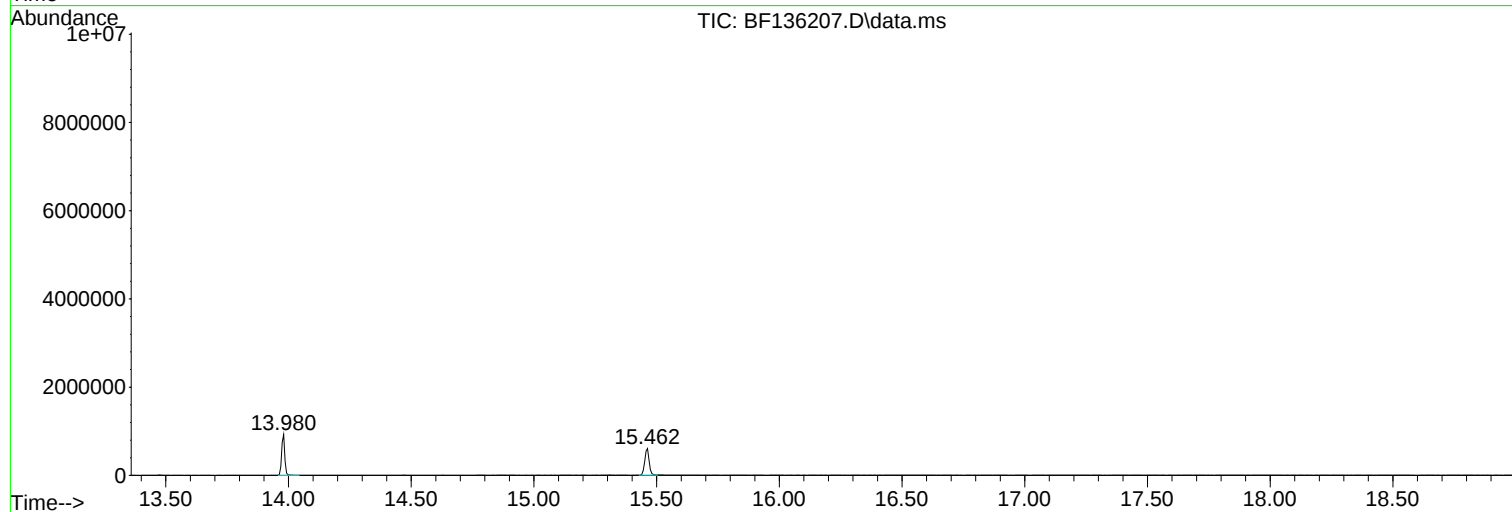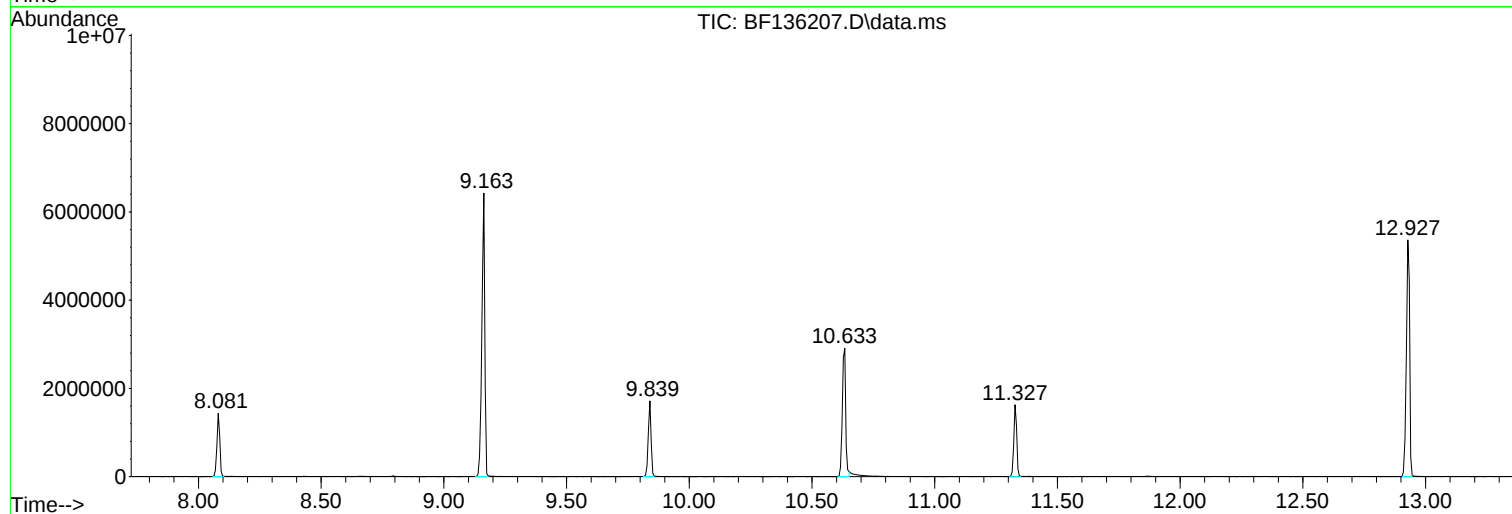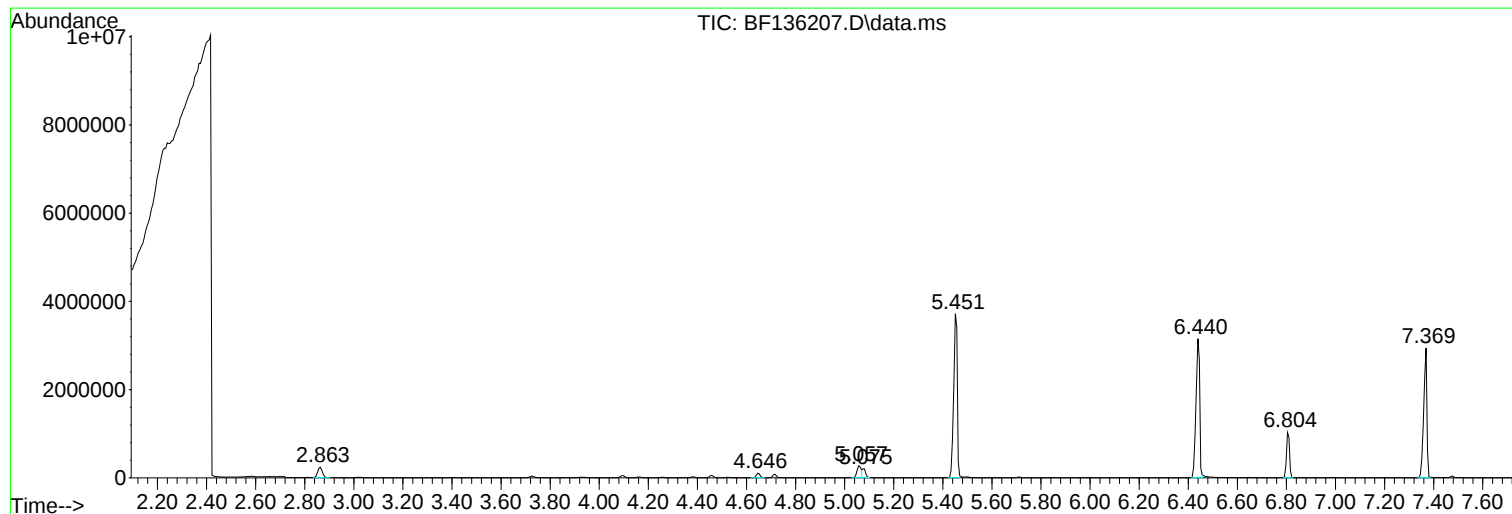

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136207.D
Acq On : 25 Nov 2023 06:39
Operator : CG\JU
Sample : 05418-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
STONE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136207.D
Acq On : 25 Nov 2023 06:39
Operator : CG\JU
Sample : 05418-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
STONE-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------