


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136179.D
Acq On : 24 Nov 2023 11:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 24 23:44:28 2023

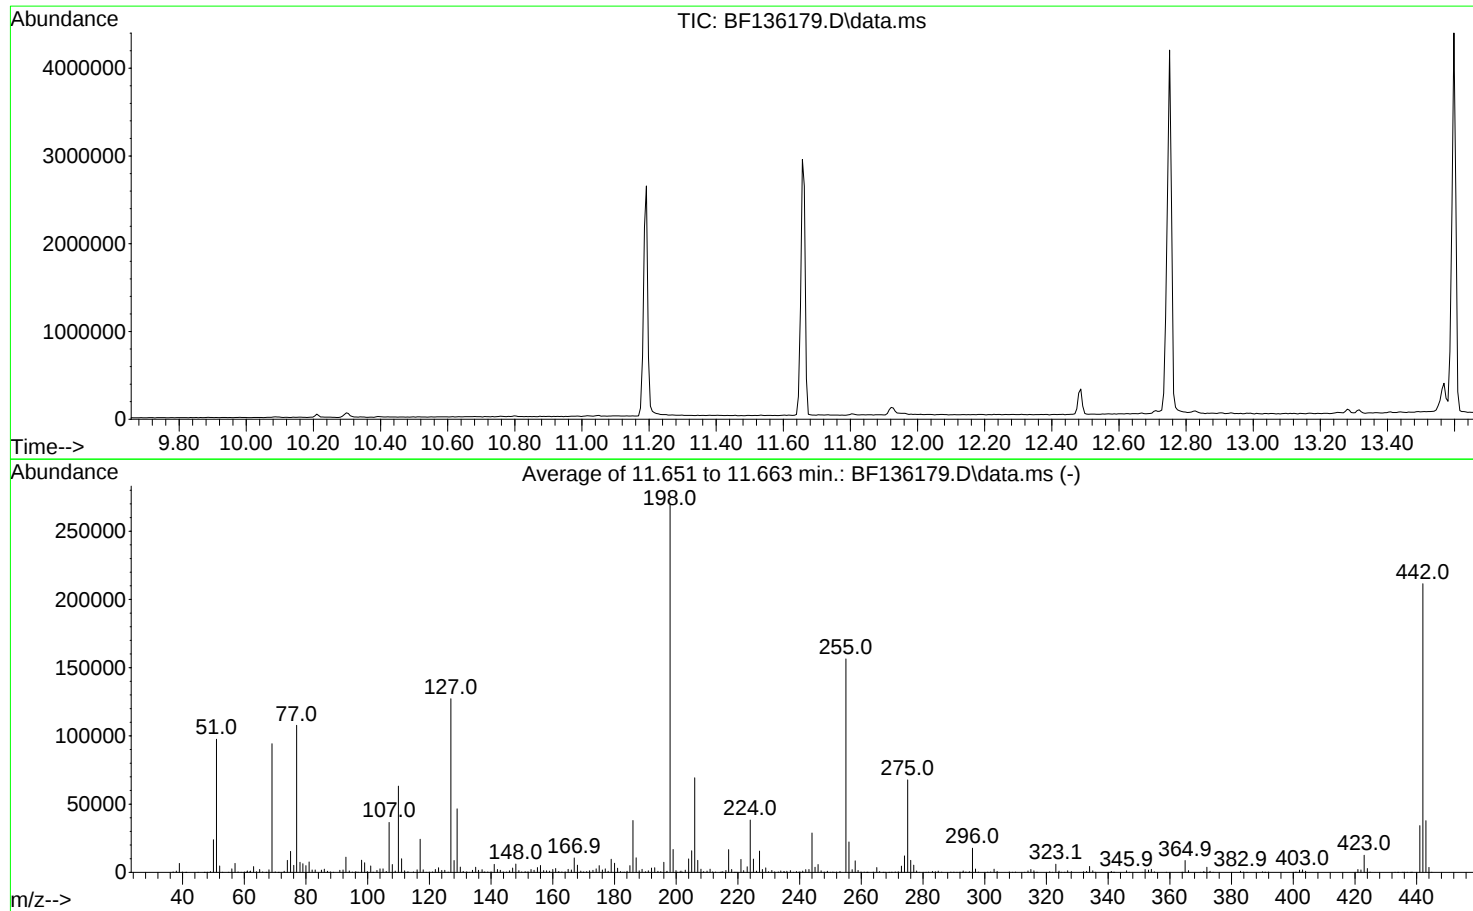




AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	97587	PASS
68	69	0.00	2	2.0	1844	PASS
69	198	0.00	100	35.0	94347	PASS
70	69	0.00	2	0.4	395	PASS
127	198	10	80	47.2	127221	PASS
197	198	0.00	2	0.3	817	PASS
198	198	100	100	100.0	269589	PASS
199	198	5	9	6.2	16812	PASS
275	198	10	60	25.1	67787	PASS
365	198	1	100	3.2	8730	PASS
441	198	0.01	100	12.7	34204	PASS
442	442	50	100	100.0	211571	PASS
443	442	15	24	17.9	37919	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136179.D
Acq On : 24 Nov 2023 11:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 24 23:42:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 23:42:24 2023
Response via : Initial Calibration

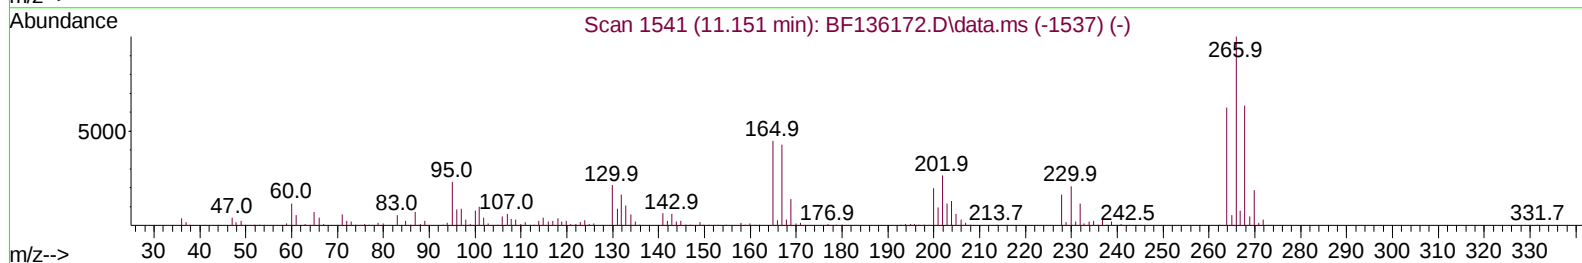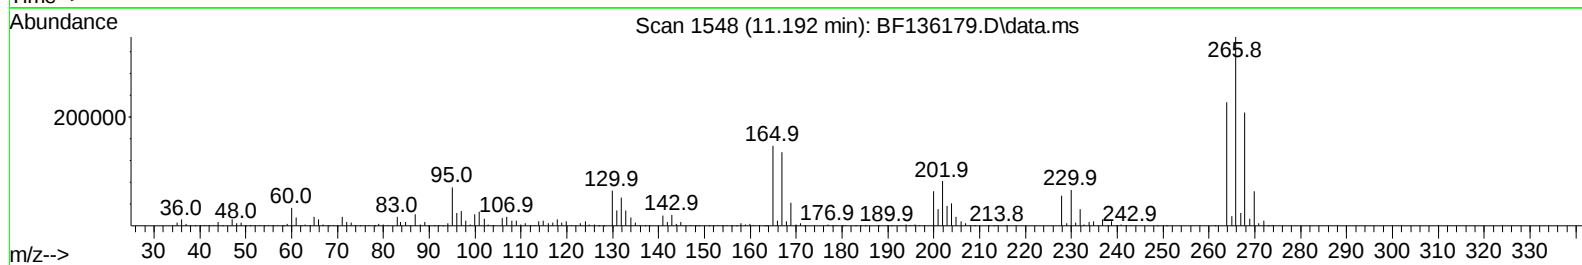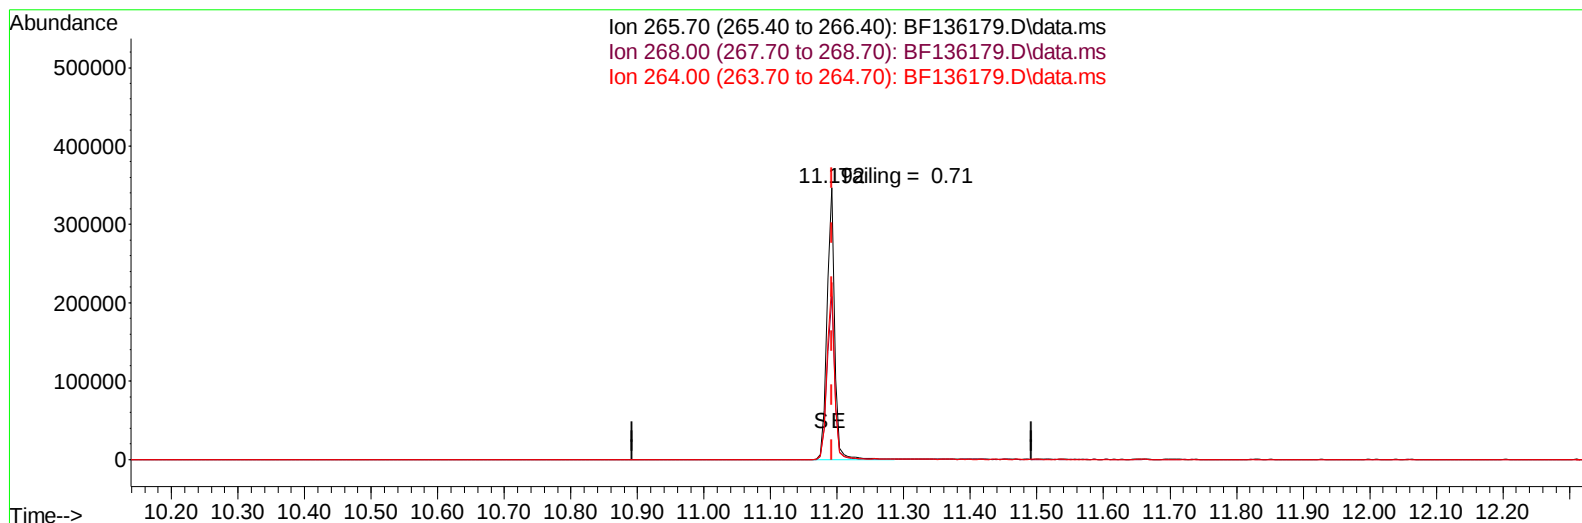

TIC: BF136179.D\data.ms

(70) Pentachlorophenol (C)

11.192min (0.000) 56831.47 ng




response 280373

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	60.07
264.00	62.50	65.30
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\  
Data File : BF136179.D  
Acq On    : 24 Nov 2023  11:50  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 24 23:42:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 23:42:24 2023
Response via : Initial Calibration

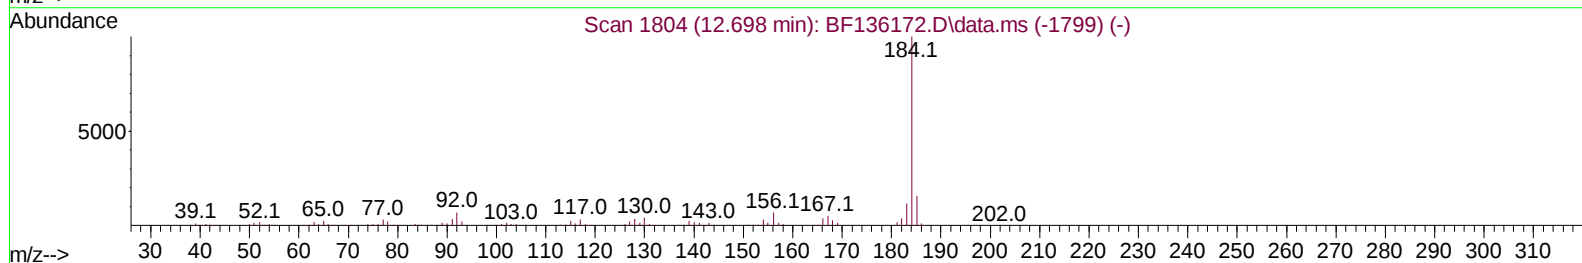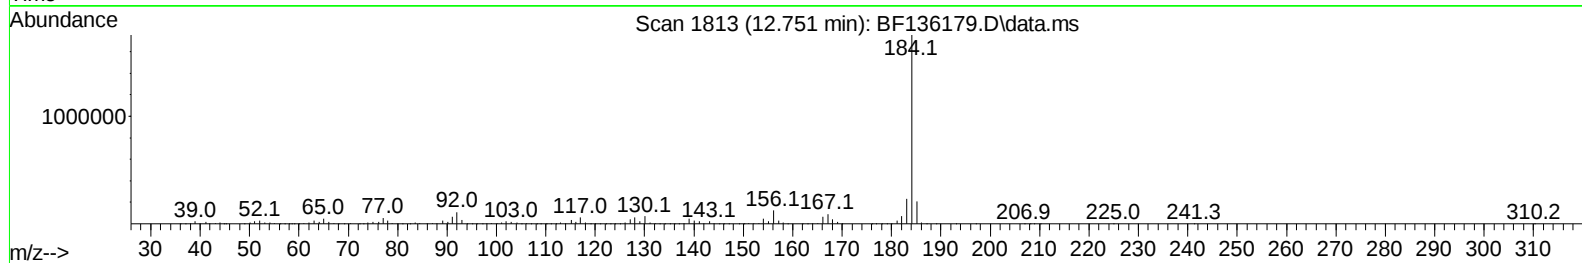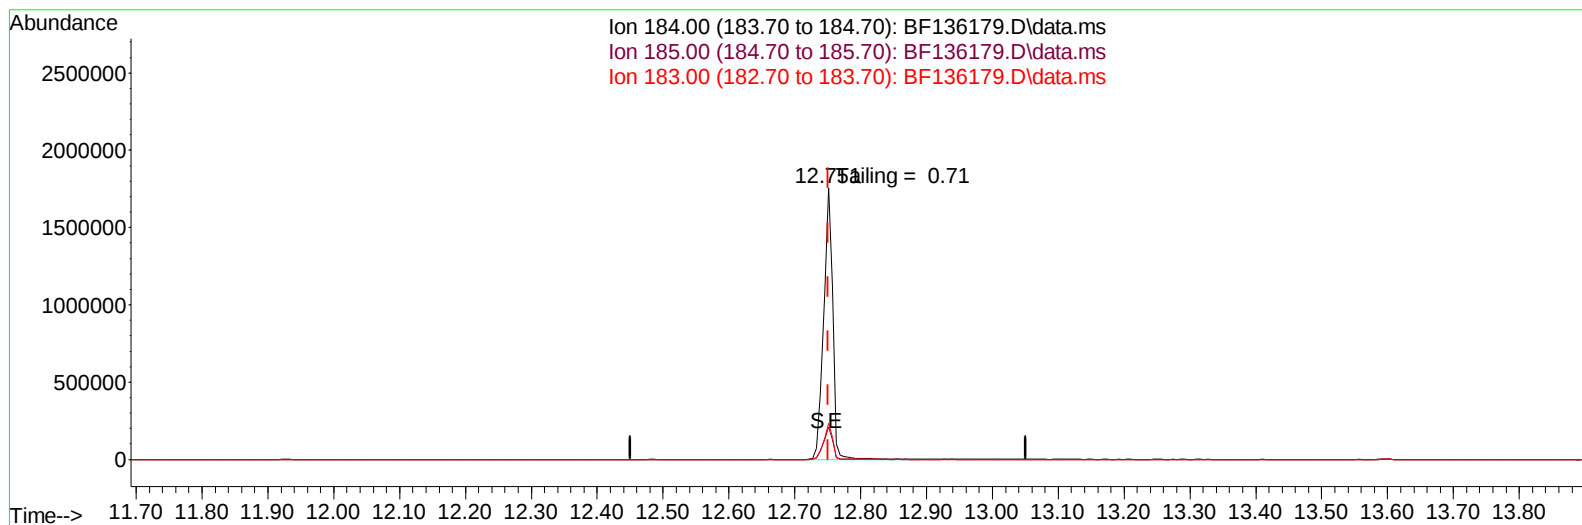

TIC: BF136179.D\data.ms

(77) Benzidine

12.751min (0.000) 133645.04 ng

response **1659250**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	11.96#
183.00	11.50	13.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/24/2023	BNA_F	<u>BF136179.D</u>
Compound Name	Response	Retention Time
DDT	746035	13.598
DDD	13195	13.28
DDE	615	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13810	759845	1.82

Instrument :
BNA_F
ClientSampleId :
DFTPP