


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136193.D
Acq On : 24 Nov 2023 23:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Nov 24 23:44:28 2023

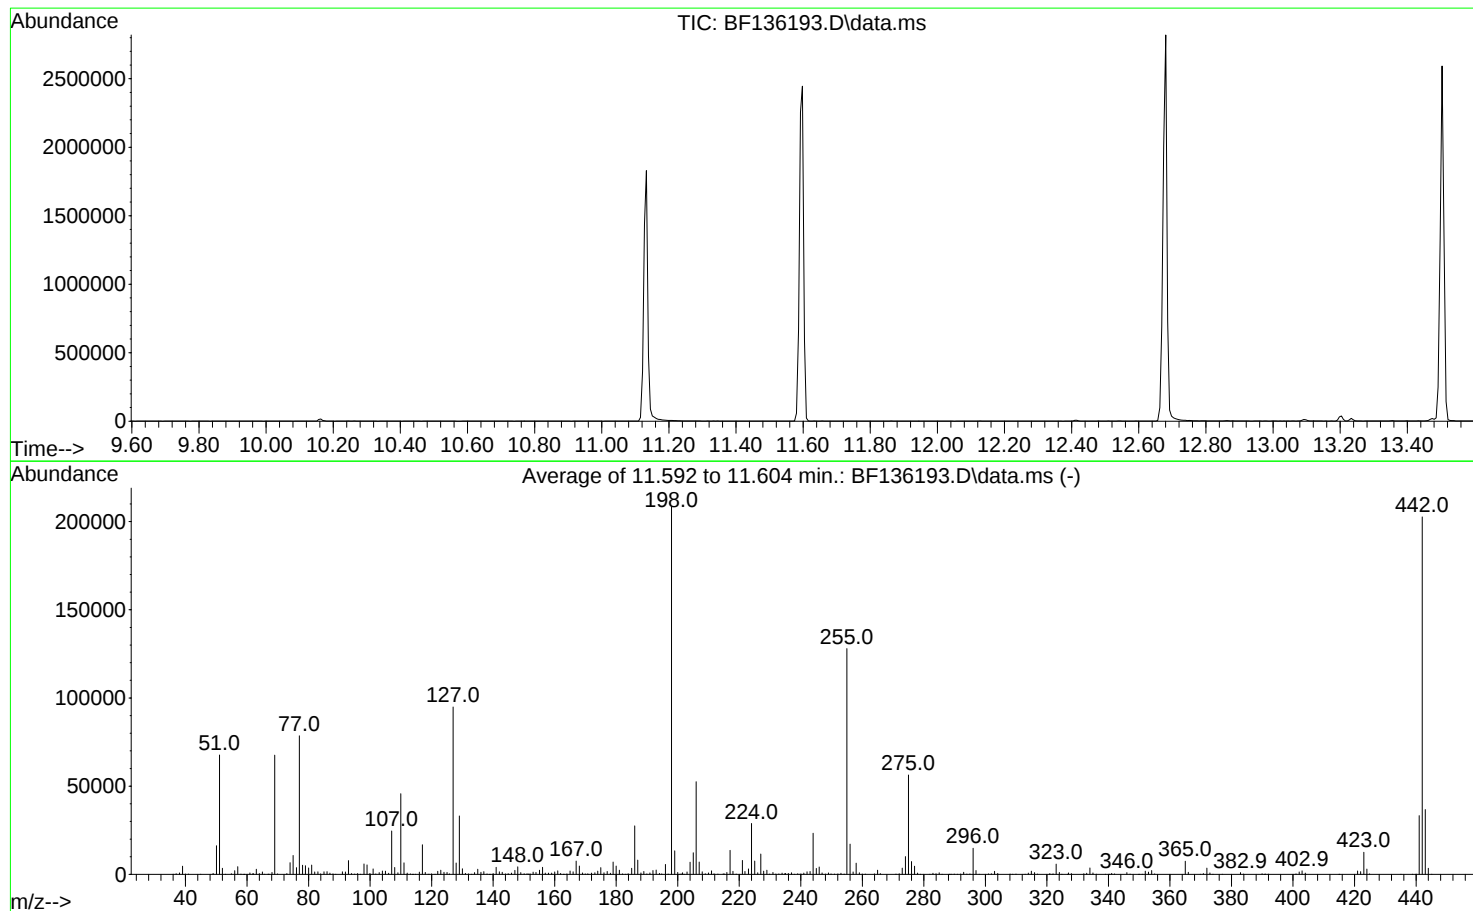




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	67683	PASS
68	69	0.00	2	1.6	1111	PASS
69	198	0.00	100	32.4	67583	PASS
70	69	0.00	2	0.4	292	PASS
127	198	10	80	45.5	94899	PASS
197	198	0.00	2	0.1	185	PASS
198	198	100	100	100.0	208560	PASS
199	198	5	9	6.4	13321	PASS
275	198	10	60	27.0	56349	PASS
365	198	1	100	3.6	7465	PASS
441	198	0.01	100	16.0	33267	PASS
442	442	50	100	100.0	202645	PASS
443	442	15	24	18.1	36747	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
 Data File : BF136193.D
 Acq On : 24 Nov 2023 23:00
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 24 23:44:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 24 23:44:28 2023
 Response via : Initial Calibration

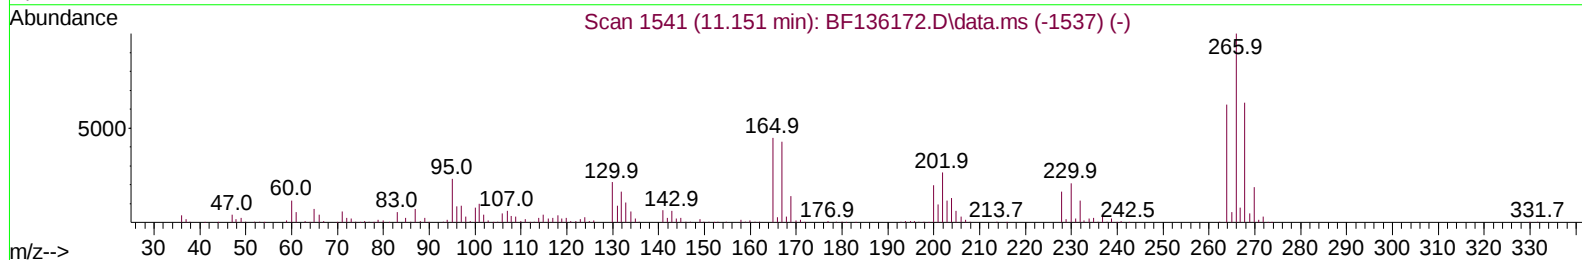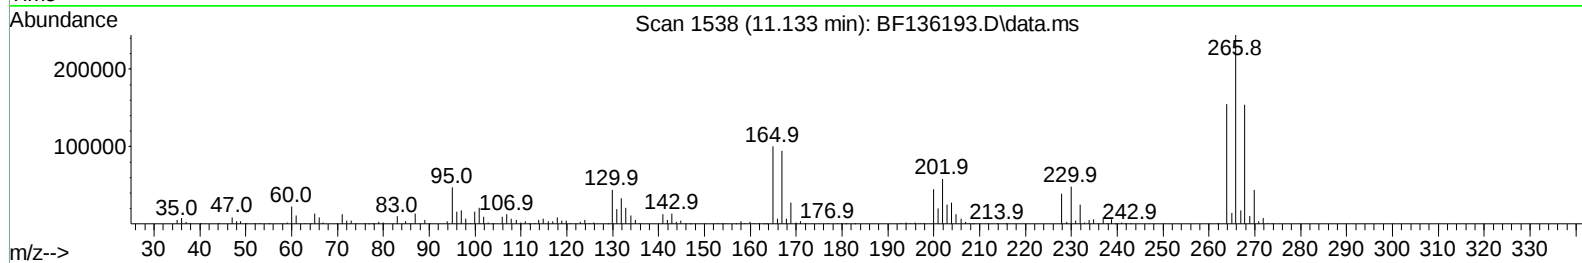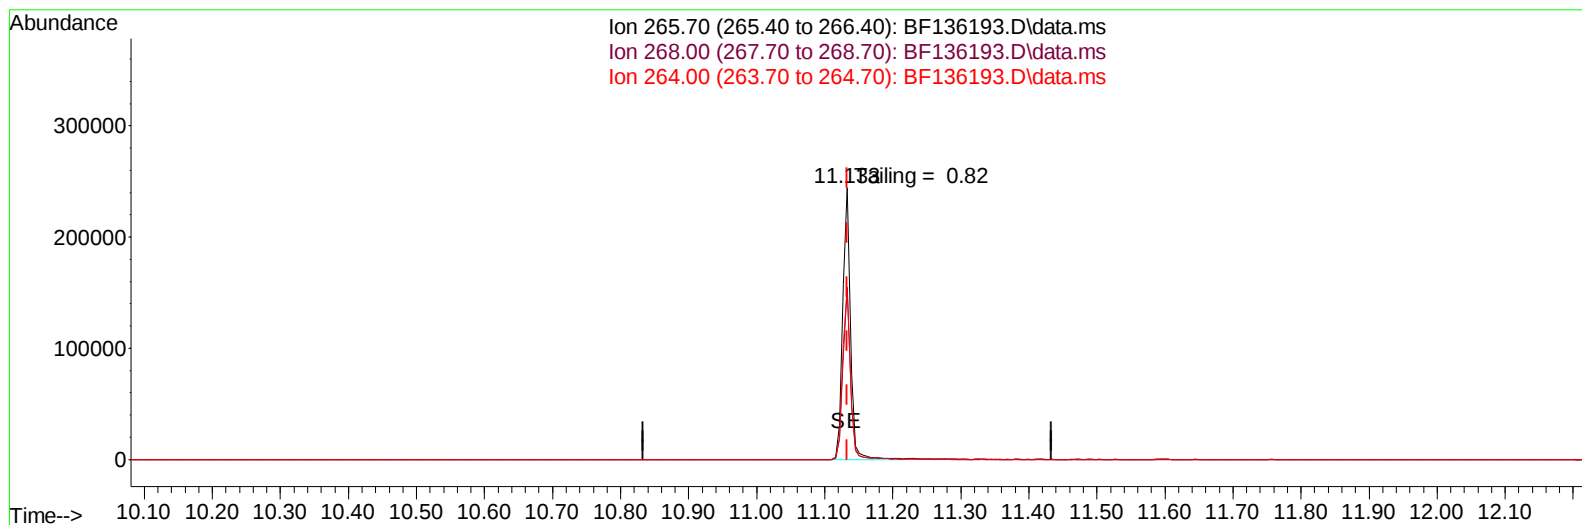

TIC: BF136193.D\data.ms

(70) Pentachlorophenol (C)

11.133min (0.000) 492949.43 ng




response 192337

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.09
264.00	62.50	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112423\
Data File : BF136193.D
Acq On : 24 Nov 2023 23:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 24 23:44:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 24 23:44:28 2023
Response via : Initial Calibration

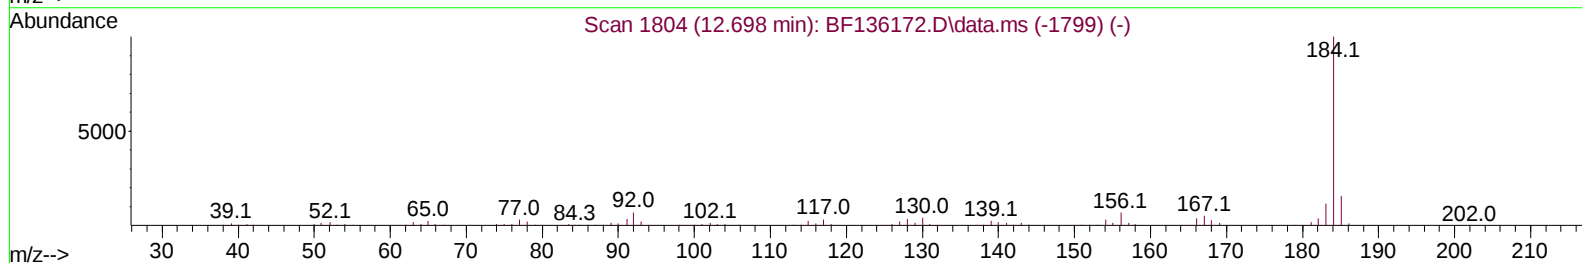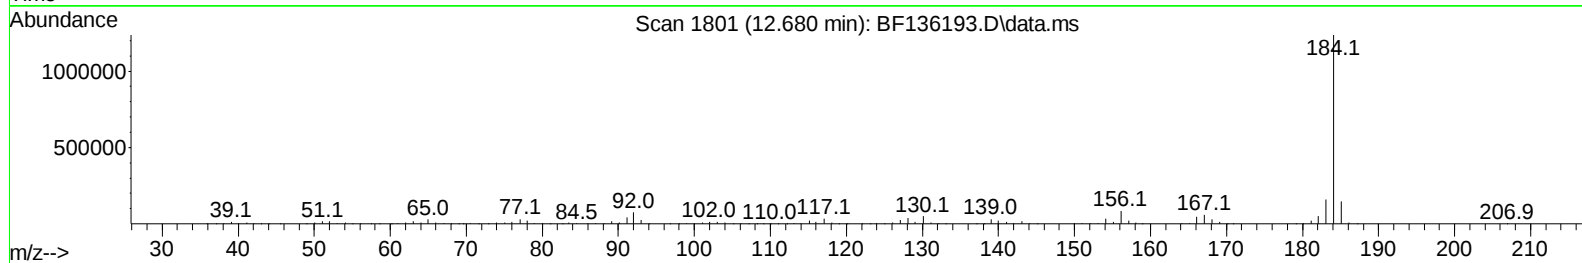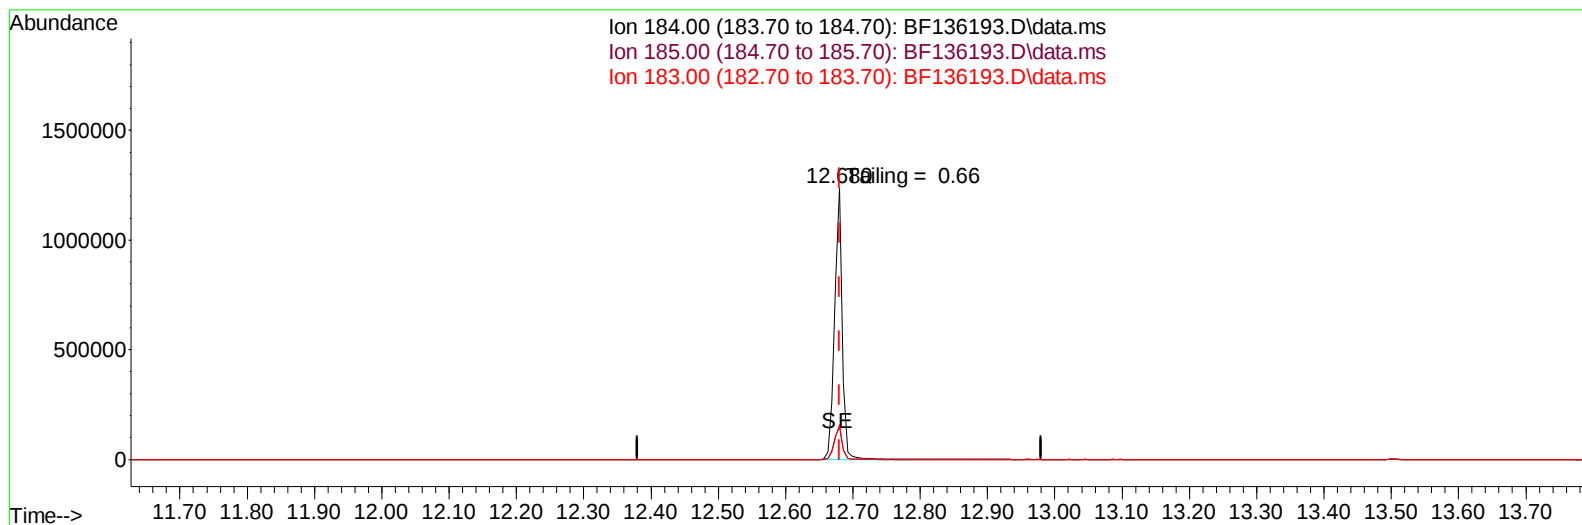

TIC: BF136193.D\data.ms

(77) Benzidine

12.680min (0.000) 0.00 ng

response 988426

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	11.84#
183.00	11.50	12.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/24/2023	BNA_F	<u>BF136193.D</u>
Compound Name	Response	Retention Time
DDT	424405	13.504
DDD	9564	13.204
DDE	548	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10112	434517	2.33

Instrument :
BNA_F
ClientSampleId :
DFTPP