


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112425\
Data File : BF144320.D
Acq On : 24 Nov 2025 12:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

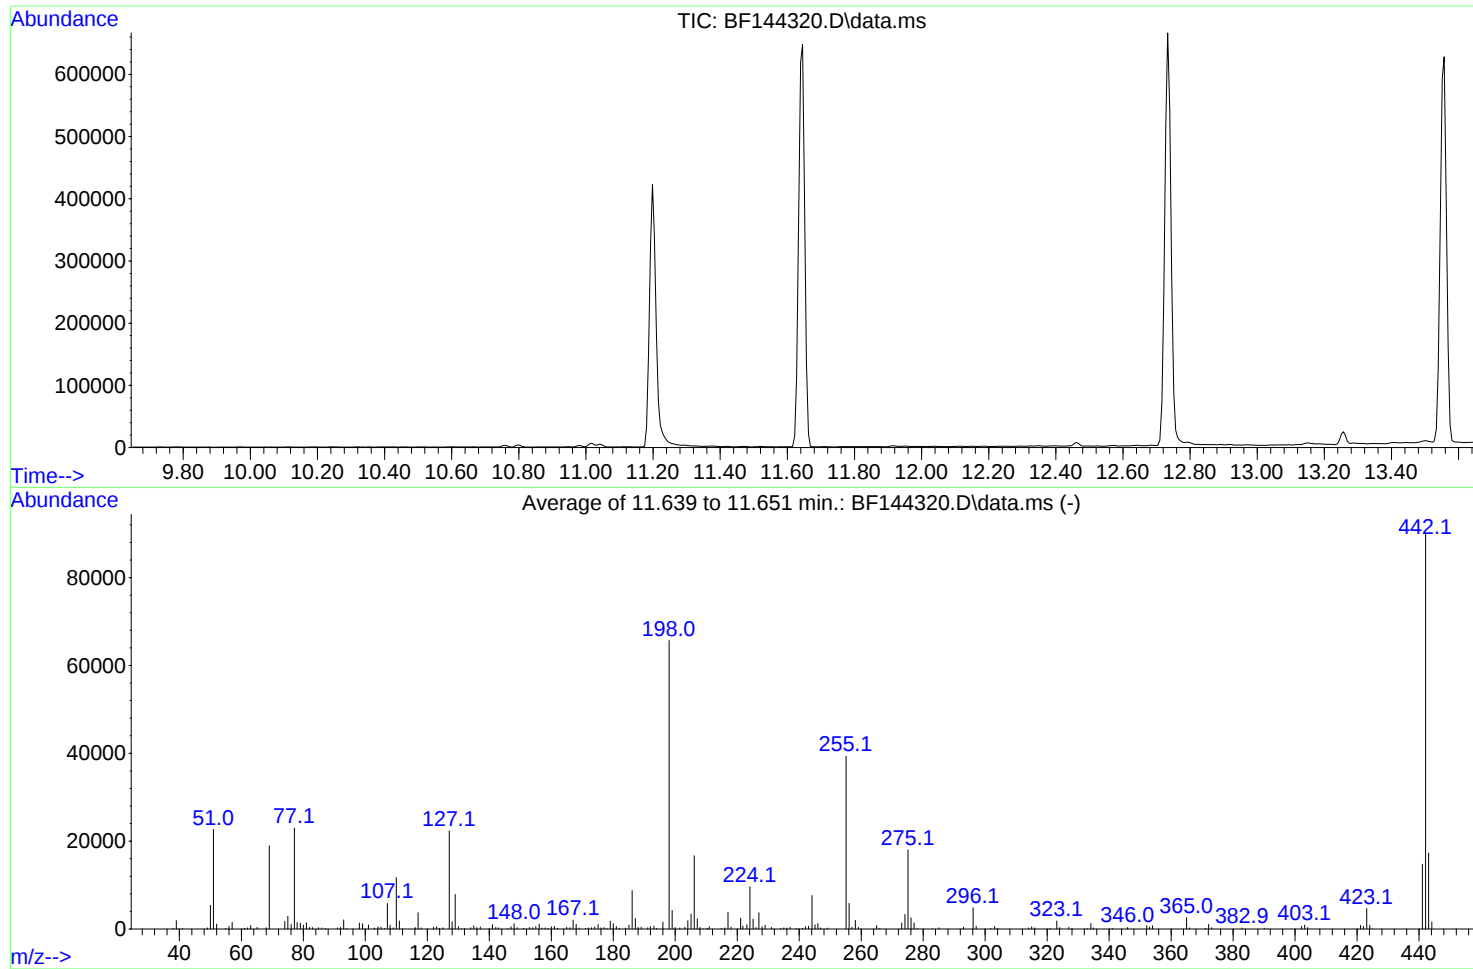

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.5	293	PASS
69	69	100	100	100.0	18942	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65680	PASS
199	198	5	9	6.4	4217	PASS
365	198	1	100	3.9	2584	PASS
441	443	0.01	150	85.3	14768	PASS
442	442	100	100	100.0	89885	PASS
443	442	15	24	19.3	17307	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/24/2025	BNA_F	<u>BF144320.D</u>
Compound Name	Response	Retention Time
DDT	176935	13.557
DDD	8069	13.257
DDE	373	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8442	185377	4.55

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112425\
Data File : BF144320.D
Acq On : 24 Nov 2025 12:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 09:45:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

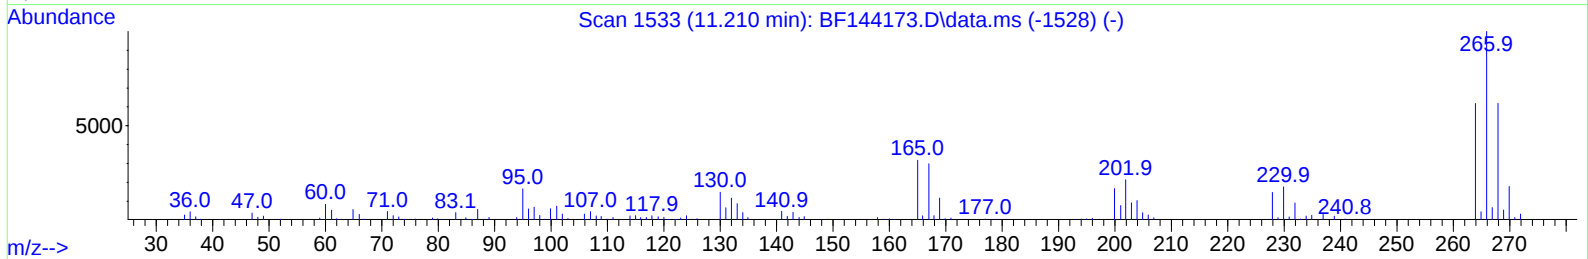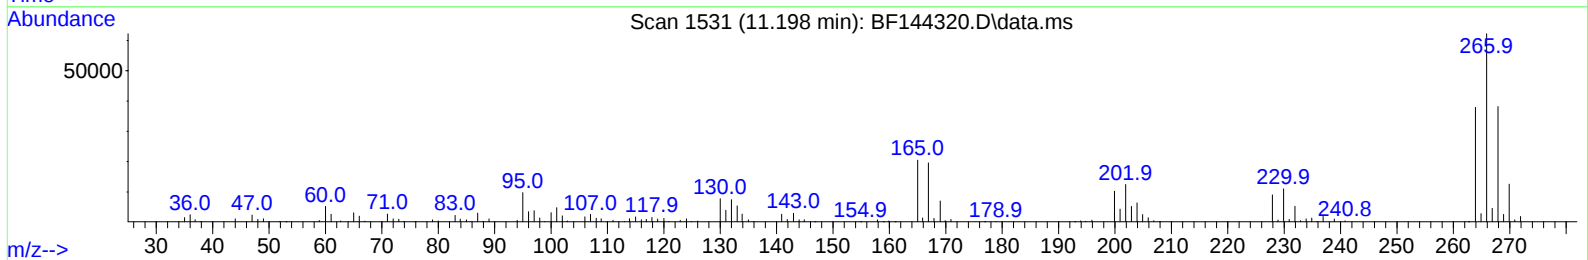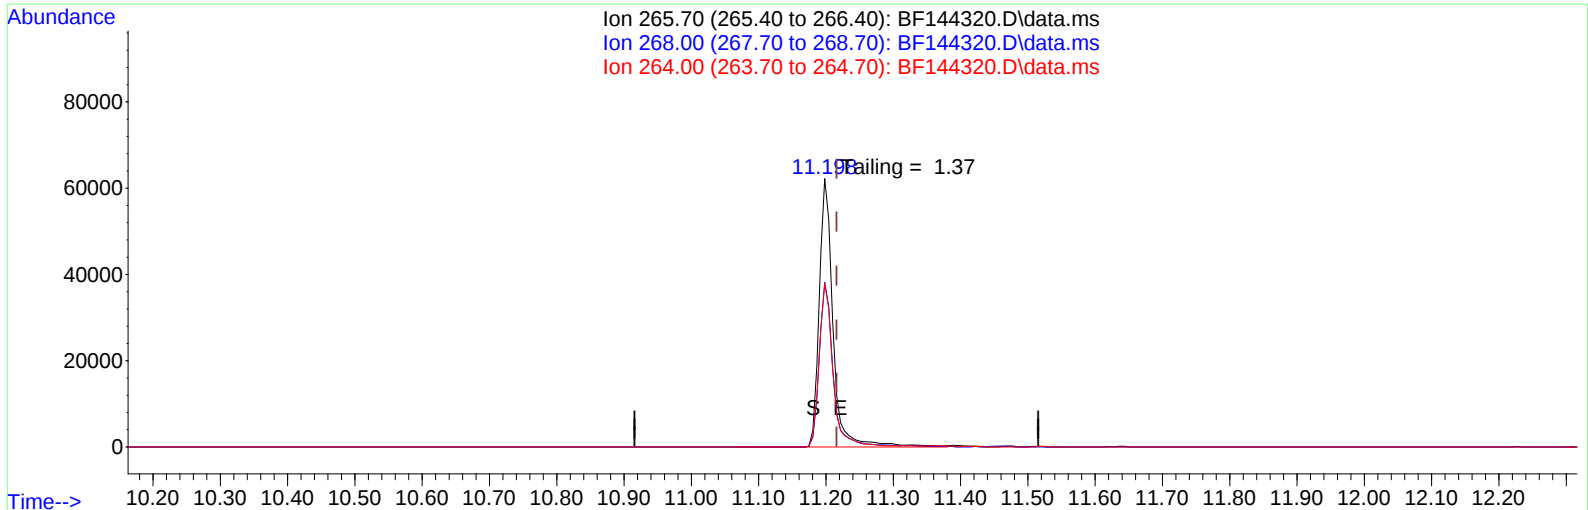

TIC: BF144320.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.018) 25697.51 ng




response 88305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	61.37
264.00	61.80	60.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112425\
Data File : BF144320.D
Acq On : 24 Nov 2025 12:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 09:45:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

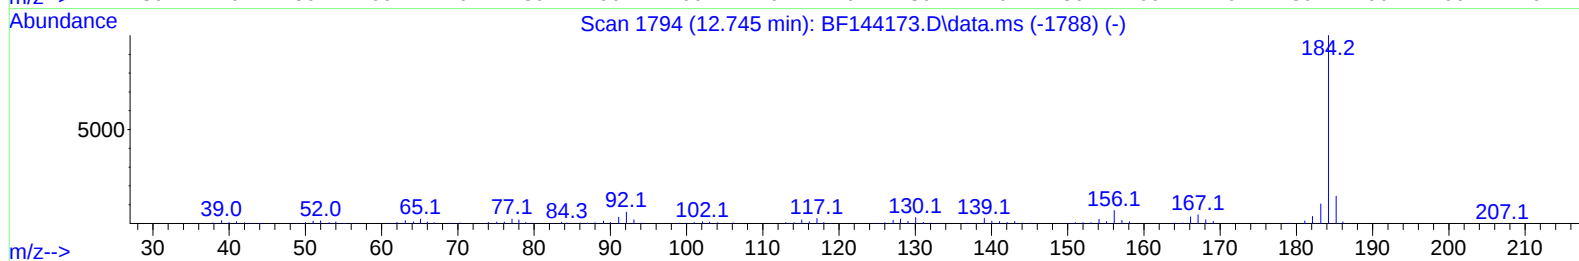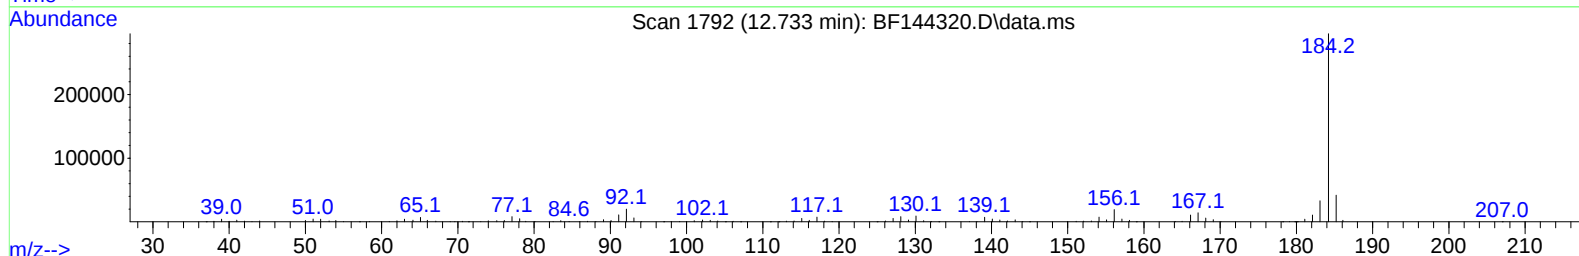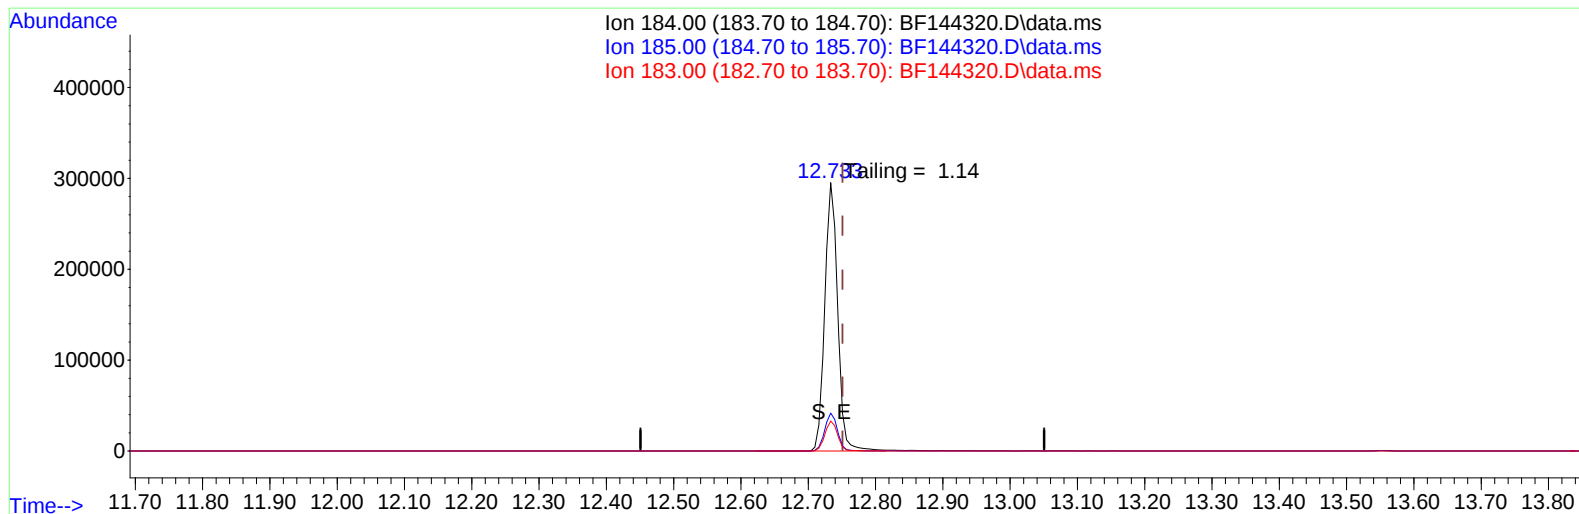

TIC: BF144320.D\data.ms

(77) Benzidine

12.733min (-0.017) 0.00 ng

response 393480

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.17
183.00	10.40	11.19
0.00	0.00	0.00