

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112519\
 Data File : BF117979.D
 Acq On : 25 Nov 2019 21:26
 Operator : JU
 Sample : PB125061BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 26 03:52:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 18:36:07 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	156799	20.00	ng	-0.04
21) Naphthalene-d8	8.17	136	624794	20.00	ng	-0.04
39) Acenaphthene-d10	9.93	164	348983	20.00	ng	-0.04
64) Phenanthrene-d10	11.43	188	693154	20.00	ng	-0.04
76) Chrysene-d12	14.08	240	559729	20.00	ng	-0.04
87) Perylene-d12	15.57	264	498563	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	1013721	114.44	ng	-0.02
7) Phenol-d6	6.52	99	1293964	121.11	ng	-0.03
23) Nitrobenzene-d5	7.45	82	809395	77.01	ng	-0.04
42) 2,4,6-Tribromophenol	10.73	330	473433	128.14	ng	-0.04
45) 2-Fluorobiphenyl	9.26	172	1660261	85.35	ng	-0.04
79) Terphenyl-d14	13.03	244	2239165	73.11	ng	-0.03
Target Compounds						
9) Benzaldehyde	6.52	77	2119	Below Cal	Qvalue	# 1
19) n-Nitroso-di-n-propylamine	7.45	70	110417	16.752 ng	#	74
25) Isophorone	7.45	82	791917	41.109 ng	#	62
51) 2,6-Dinitrotoluene	9.93	165	43965	8.220 ng	#	24
57) 2,4-Dinitrotoluene	9.93	165	43965	6.462 ng	#	25
67) 4-Bromophenyl-phenylether	10.73	248	29627	3.961 ng	#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112519\
Data File : BF117979.D
Acq On : 25 Nov 2019 21:26
Operator : JU
Sample : PB125061BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 26 03:52:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

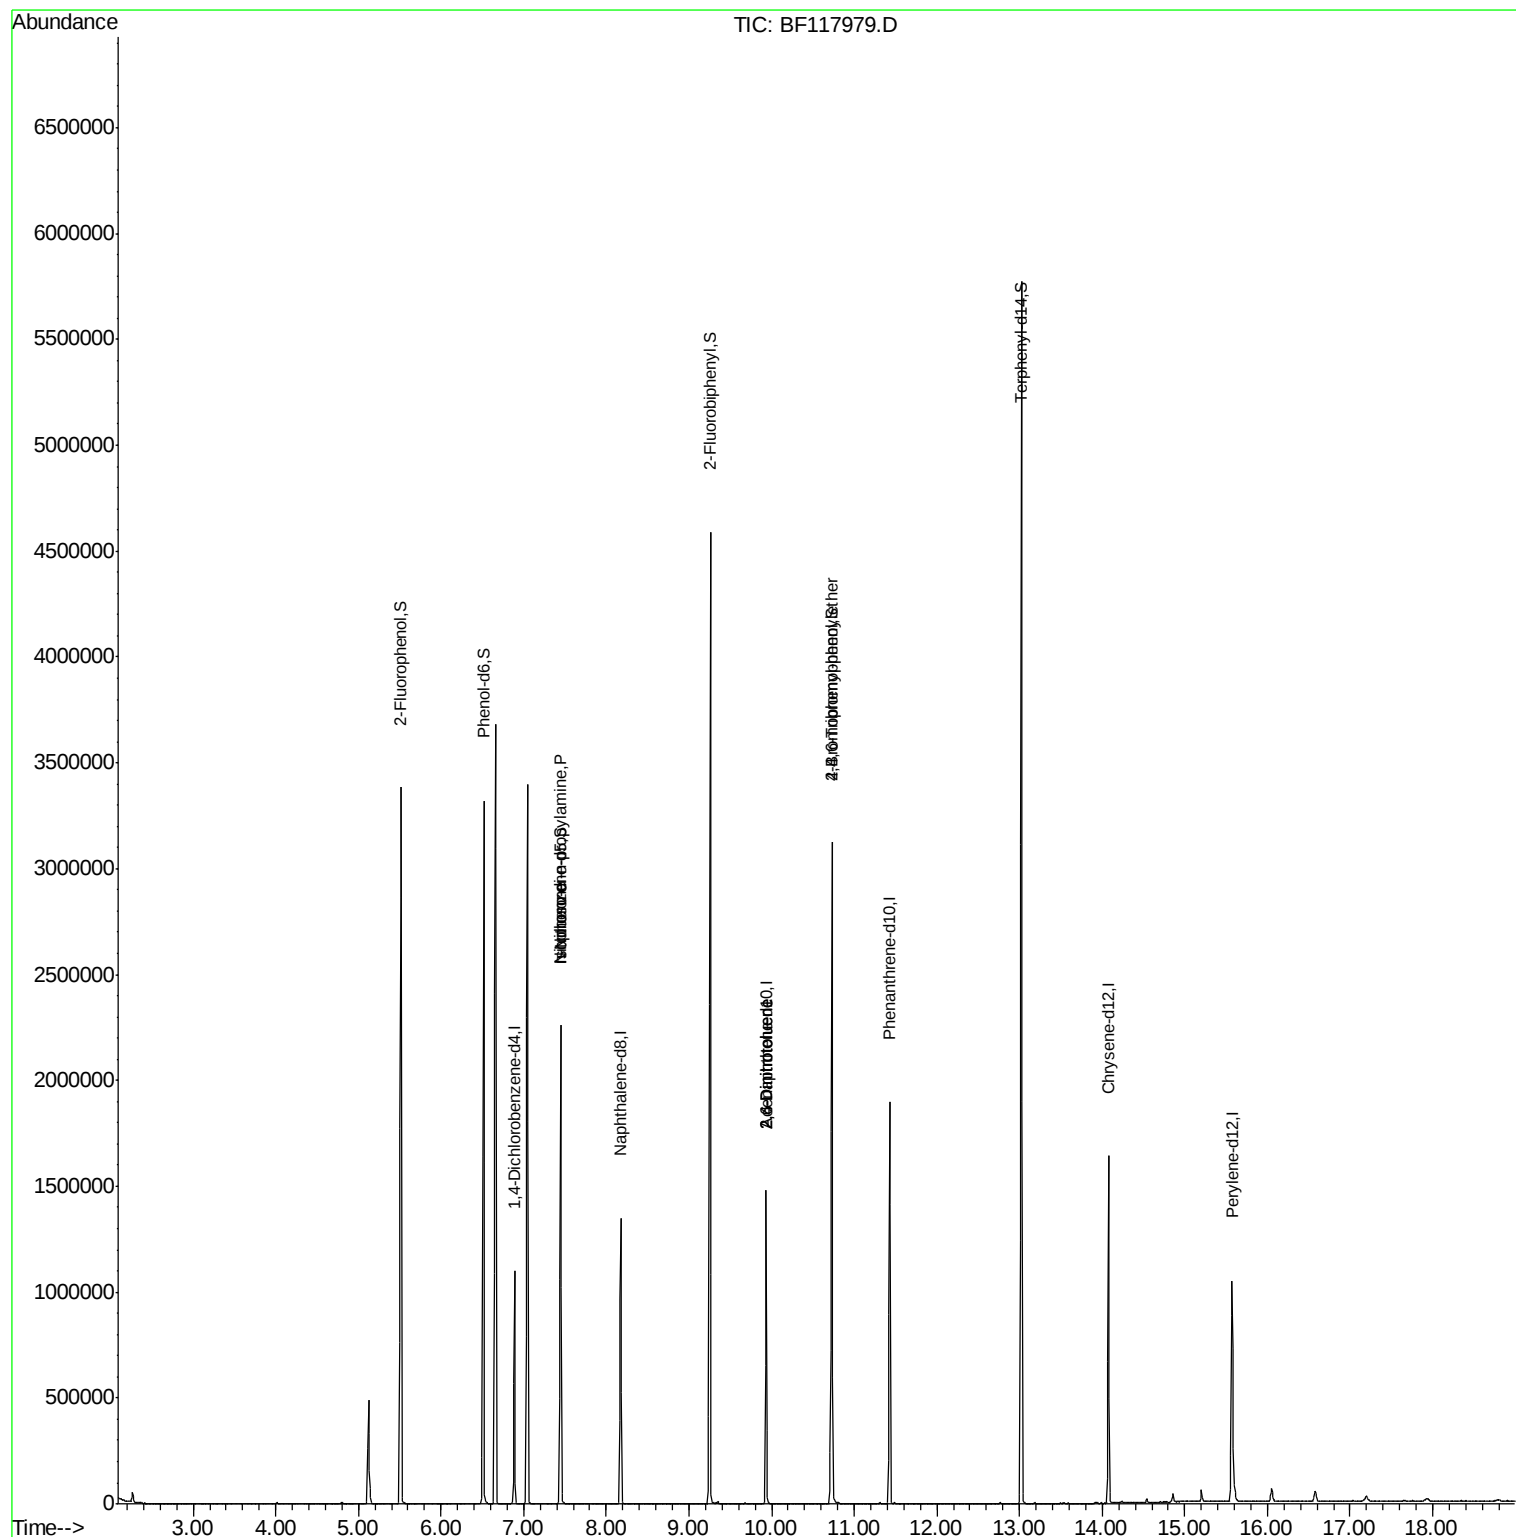

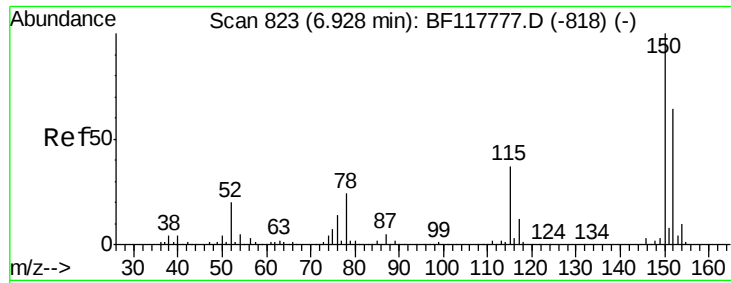


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.89 min Scan# 816
Delta R.T. -0.04 min
Lab File: BF117979.D
Acq: 25 Nov 2019 21:26

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 156799
Ion Ratio Lower Upper
152 100
150 154.0 125.3 187.9
115 63.0 47.0 70.4

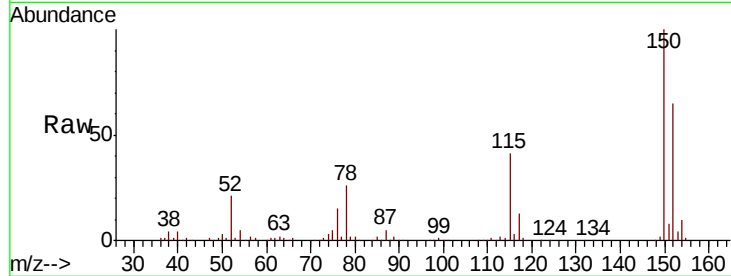


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

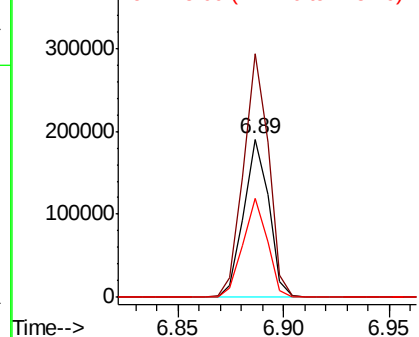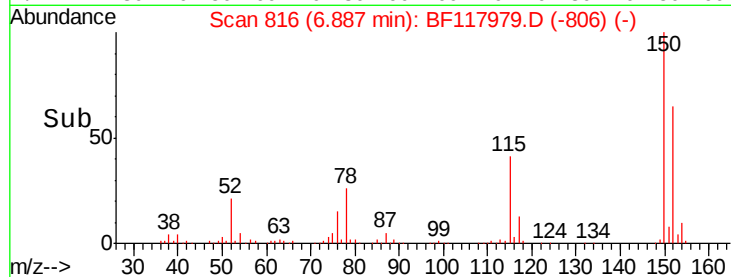



#5


2-Fluorophenol
Concen: 114.439 ng
RT: 5.52 min Scan# 583
Delta R.T. -0.02 min
Lab File: BF117979.D
Acq: 25 Nov 2019 21:26

Tgt Ion:112 Resp: 1013721
Ion Ratio Lower Upper
112 100
64 54.6 45.6 68.4
63 30.0 24.1 36.1

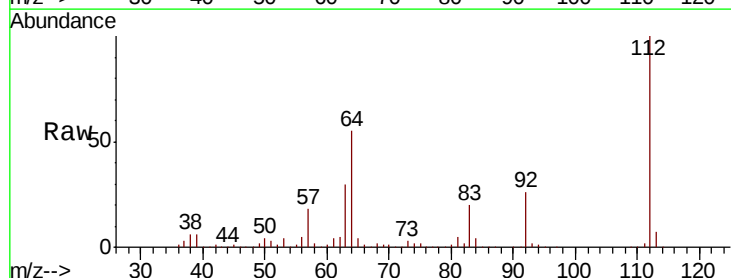

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

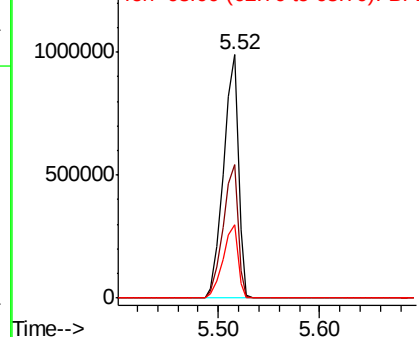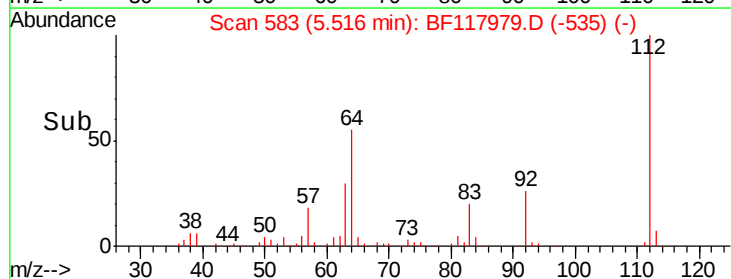



#7

Phenol-d6

Concen: 121.108 ng

RT: 6.52 min Scan# 753

Delta R.T. -0.03 min

Lab File: BF117979.D

Acq: 25 Nov 2019 21:26

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 1293964

Ion Ratio Lower Upper

99 100

42 18.5 14.9 22.3




71 37.5 28.6 43.0

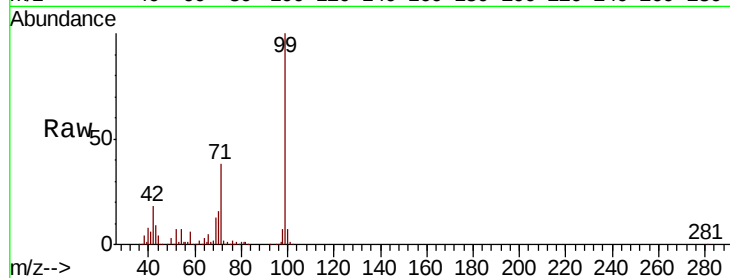

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

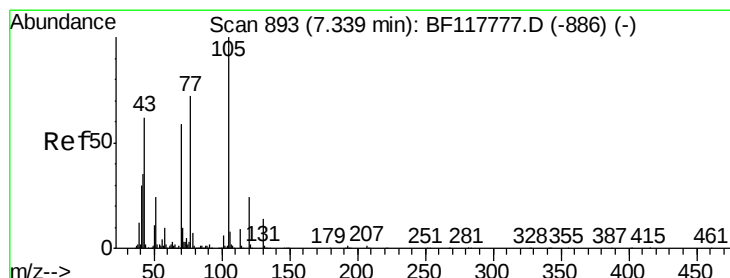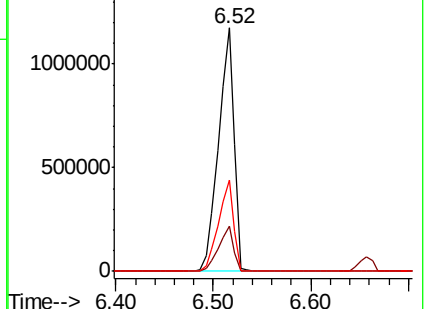

#19

n-Nitroso-di-n-propylamine

Concen: 16.752 ng

RT: 7.45 min Scan# 912

Delta R.T. 0.11 min

Lab File: BF117979.D

Acq: 25 Nov 2019 21:26

Tgt Ion: 70 Resp: 110417


Ion Ratio Lower Upper

70 100

42 45.5 47.4 71.2#

101 0.0 8.4 12.6#

130 2.1 18.8 28.2#


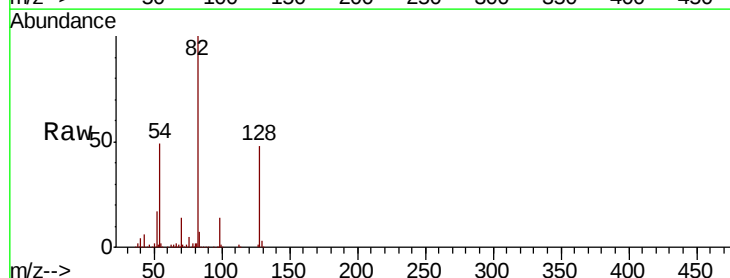


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1



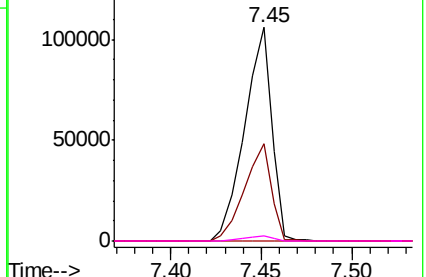





#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.17 min Scan# 1035
Delta R.T. -0.04 min
Lab File: BF117979.D
Acq: 25 Nov 2019 21:26




Instrument :
BNA_F
ClientSampleId :


Tot Ion:136	Resp:	624794
Ion	Ratio	Lower Upper
136	100	
137	11.0	9.0 13.4
54	6.5	5.4 8.2
68	4.5	4.3 6.5

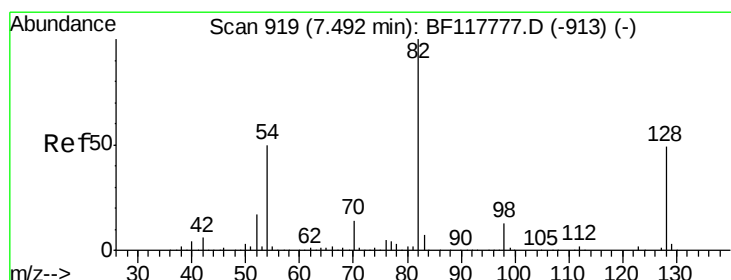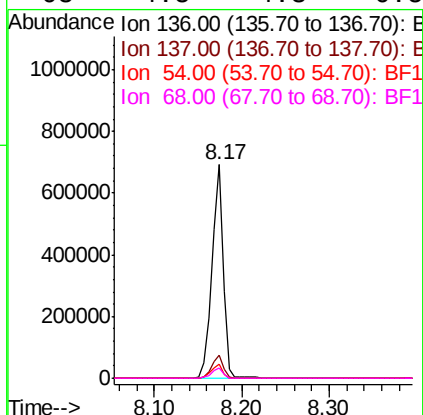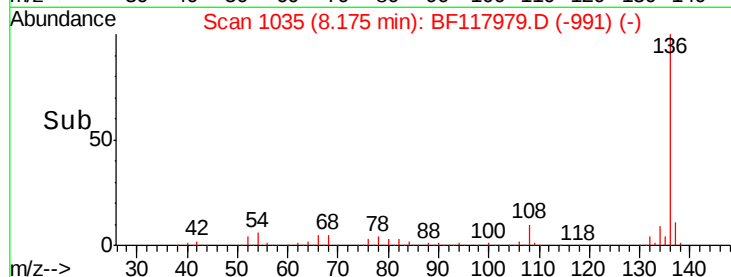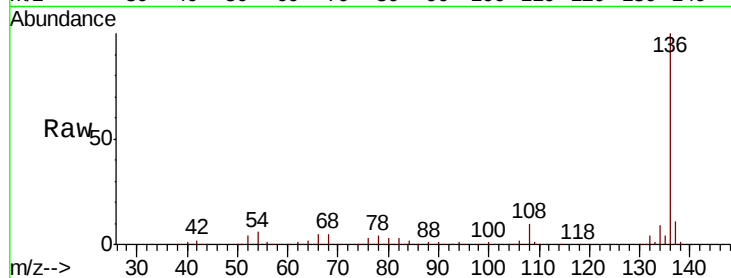

#23
Nitrobenzene-d5
Concen: 77.010 ng
RT: 7.45 min Scan# 912
Delta R.T. -0.04 min
Lab File: BF117979.D
Acq: 25 Nov 2019 21:26

Tgt Ion: 82	Resp:	809395
Ion	Ratio	Lower Upper
82	100	
128	48.1	38.9 58.3
54	48.7	39.8 59.6

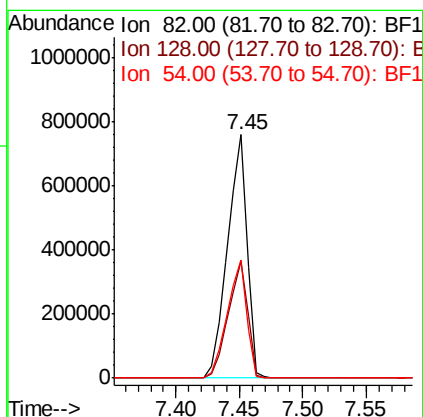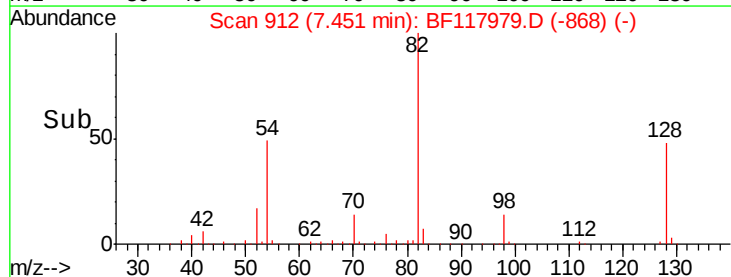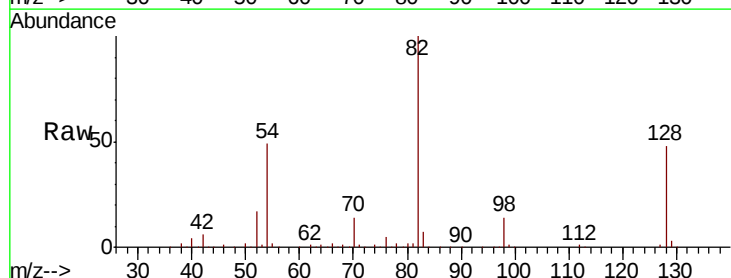

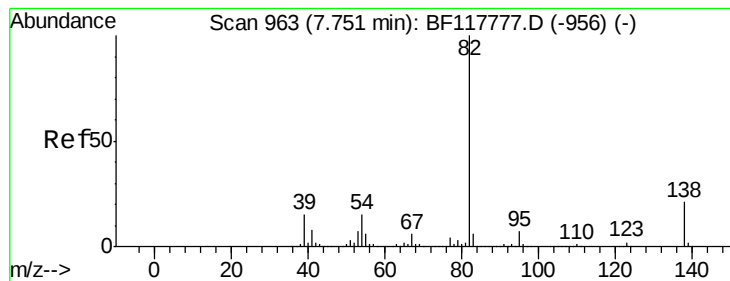

#25

Isophorone

Concen: 41.109 ng

RT: 7.45 min Scan# 912

Delta R.T. -0.30 min

Lab File: BF117979.D

Acq: 25 Nov 2019 21:26

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 791917

Ion Ratio Lower Upper

82 100

95 0.0 5.8 8.8#




138 0.0 16.5 24.7#

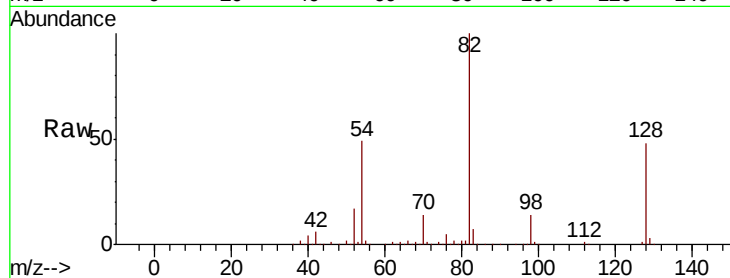

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

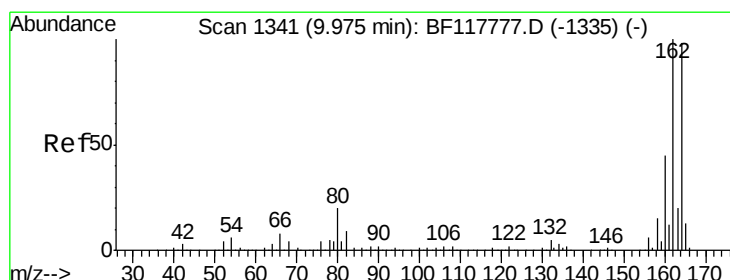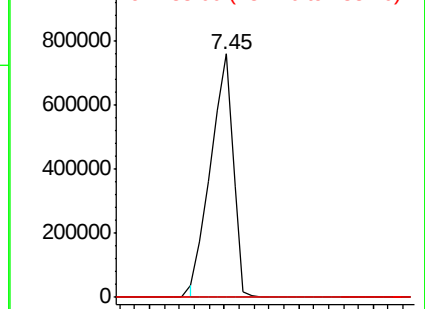

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.93 min Scan# 1334

Delta R.T. -0.04 min

Lab File: BF117979.D

Acq: 25 Nov 2019 21:26


Tgt Ion:164 Resp: 348983

Ion Ratio Lower Upper

164 100

162 101.8 81.3 121.9



160 45.0 36.6 55.0

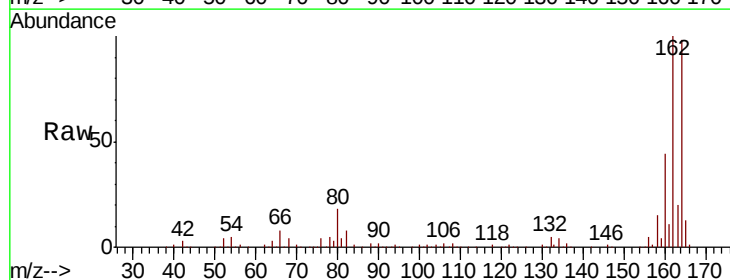

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

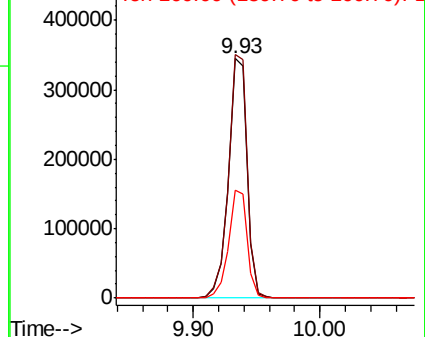



#42

2,4,6-Tribromophenol

Concen: 128.140 ng

RT: 10.73 min Scan# 1470

Delta R.T. -0.04 min

Lab File: BF117979.D

Acq: 25 Nov 2019 21:26

Instrument :

BNA_F

ClientSampleId :


Tot Ion:330 Resp: 473433

Ion Ratio Lower Upper




330 100

332 96.7 76.7 115.1

141 33.0 27.7 41.5

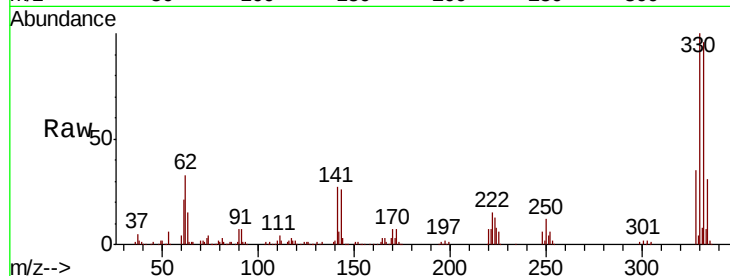

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

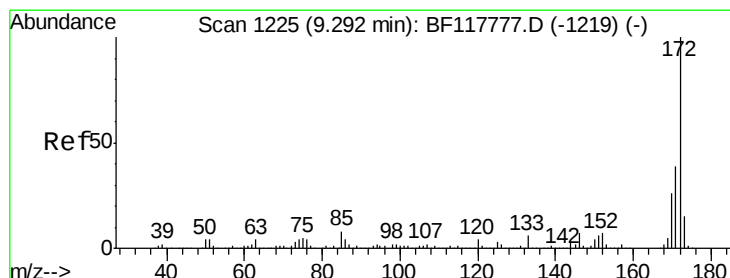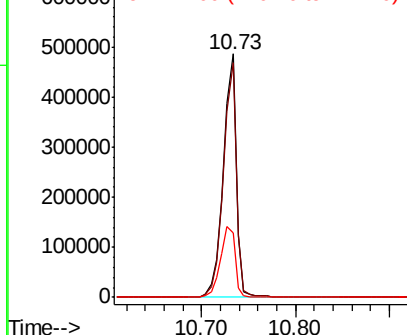

#45

2-Fluorobiphenyl

Concen: 85.350 ng

RT: 9.26 min Scan# 1219

Delta R.T. -0.04 min

Lab File: BF117979.D

Acq: 25 Nov 2019 21:26


Tgt Ion:172 Resp: 1660261

Ion Ratio Lower Upper



172 100


171 36.3 30.9 46.3

170 24.3 21.0 31.4

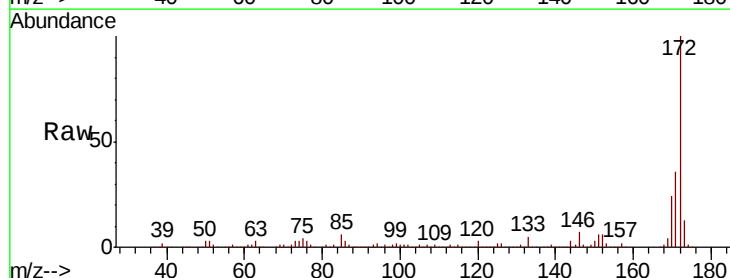

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

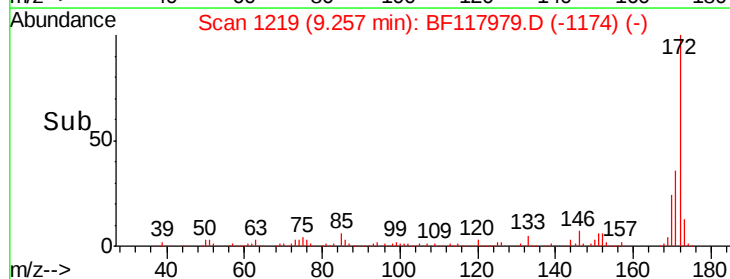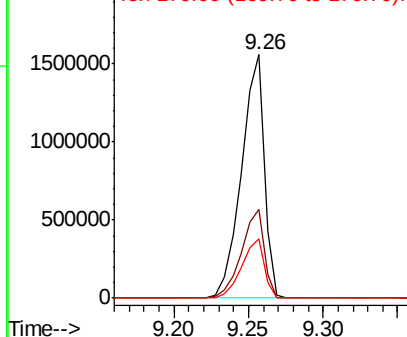







#51
 2,6-Dinitrotoluene
 Concen: 8.220 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. 0.18 min
 Lab File: BF117979.D
 Acq: 25 Nov 2019 21:26

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.5	46.0	69.0#
89	1.4	47.7	71.5#

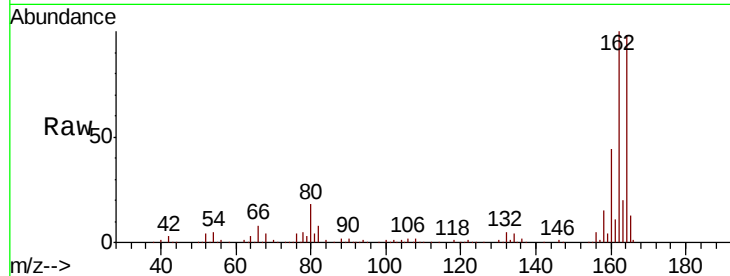




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

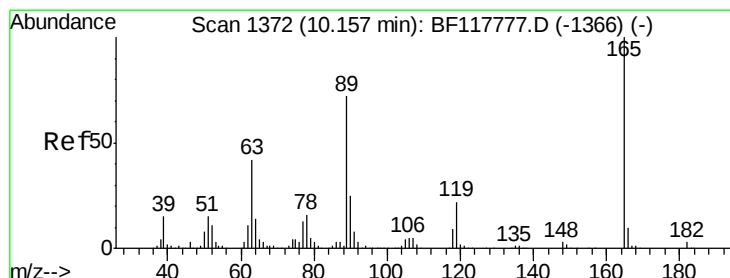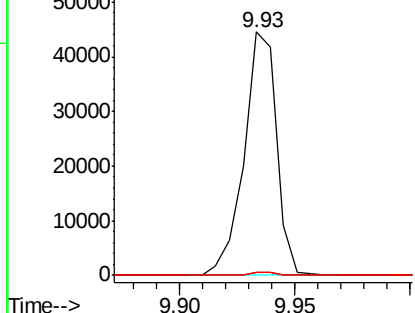


#57
 2,4-Dinitrotoluene
 Concen: 6.462 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. -0.22 min
 Lab File: BF117979.D
 Acq: 25 Nov 2019 21:26

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	33.7	50.5#
89	1.4	57.3	85.9#
182	0.0	2.3	3.5#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E

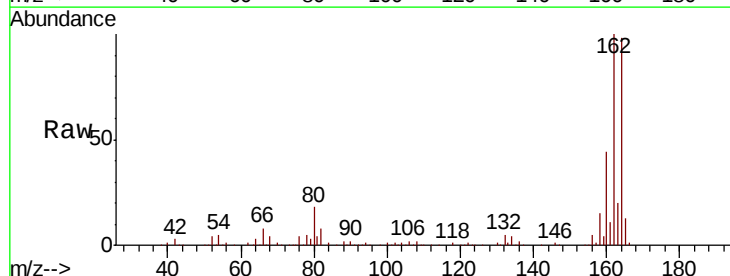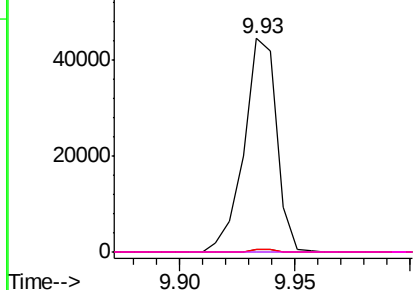







#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.43 min Scan# 1588
 Delta R.T. -0.04 min
 Lab File: BF117979.D
 Acq: 25 Nov 2019 21:26

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:188 Resp: 693154
 Ion Ratio Lower Upper
 188 100
 94 9.2 6.6 10.0
 80 10.1 7.2 10.8

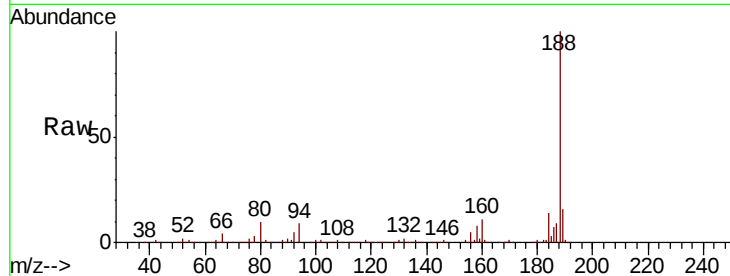


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

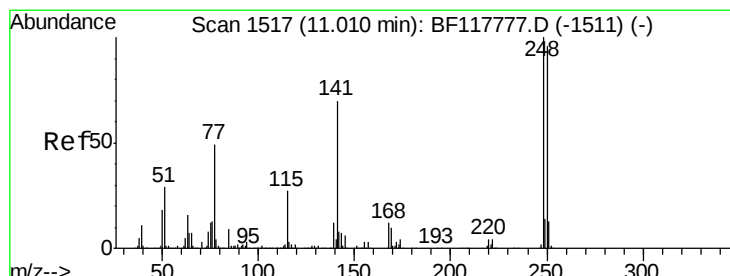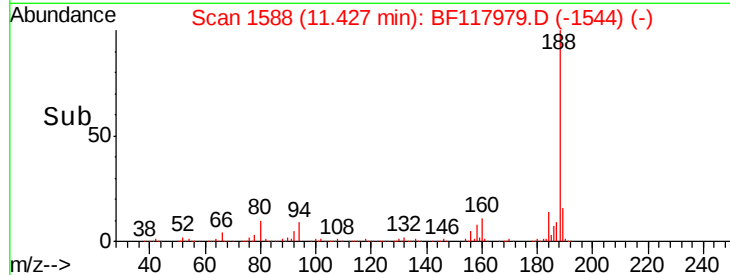
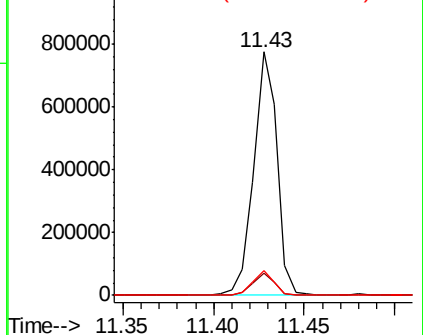



#67
 4-Bromophenyl-phenylether
 Concen: 3.961 ng
 RT: 10.73 min Scan# 1470
 Delta R.T. -0.28 min
 Lab File: BF117979.D
 Acq: 25 Nov 2019 21:26

Tgt Ion:248 Resp: 29627
 Ion Ratio Lower Upper
 248 100
 250 198.1 76.6 115.0#
 141 454.6 55.9 83.9#

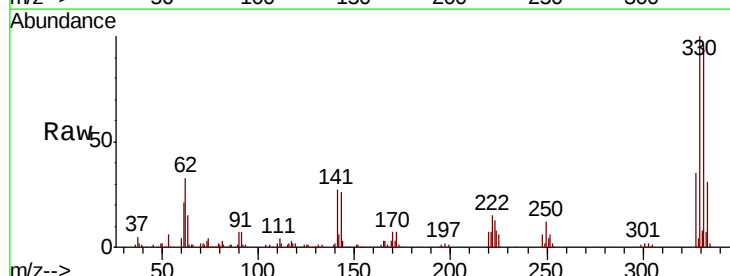

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

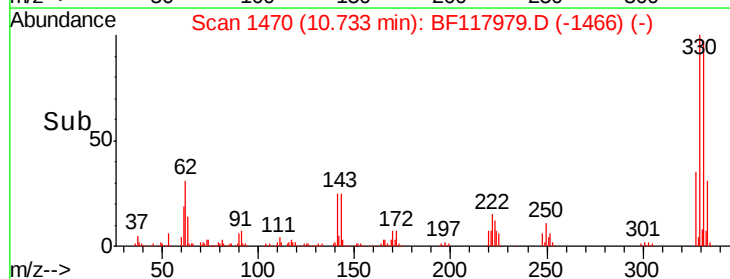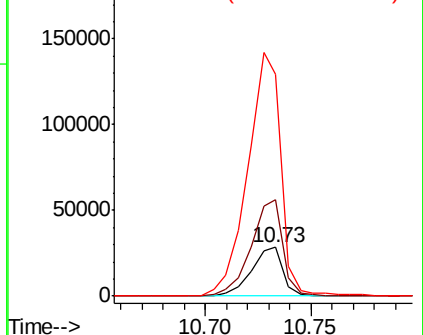



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.08 min Scan# 2039

Delta R.T. -0.04 min

Lab File: BF117979.D

Acq: 25 Nov 2019 21:26

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 559729

Ion Ratio Lower Upper

240 100

120 9.7 9.5 14.3




236 26.7 21.3 31.9

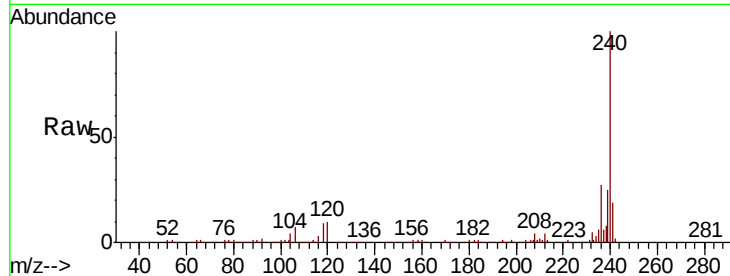

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

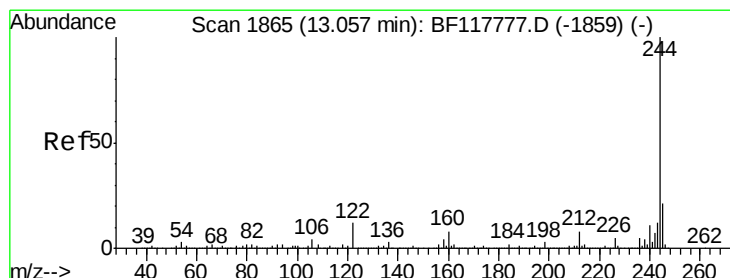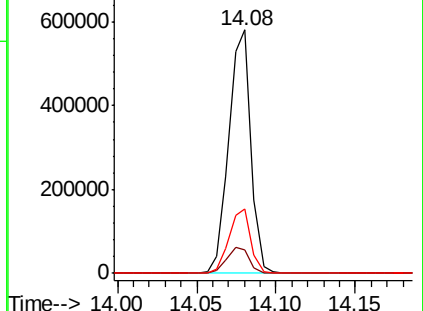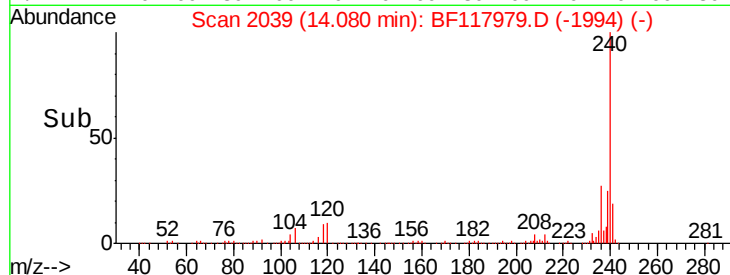

#79

Terphenyl-d14

Concen: 73.113 ng

RT: 13.03 min Scan# 1860

Delta R.T. -0.03 min

Lab File: BF117979.D

Acq: 25 Nov 2019 21:26


Tgt Ion:244 Resp: 2239165

Ion Ratio Lower Upper

244 100

212 7.4 6.3 9.5



122 11.0 9.4 14.2

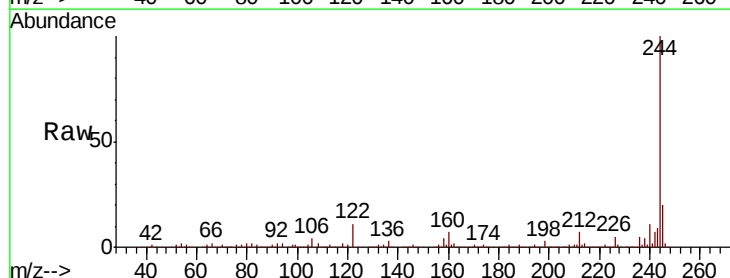


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

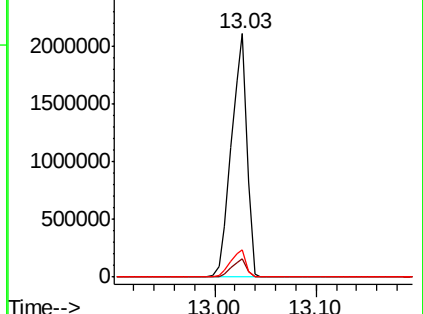


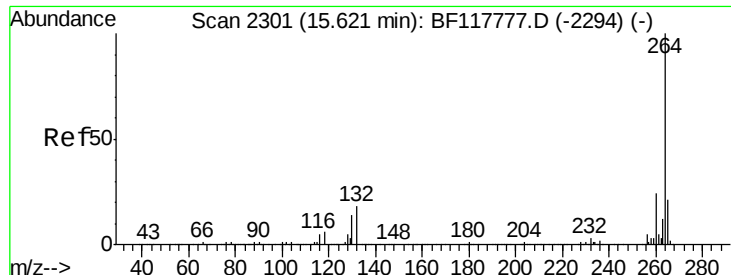

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.57 min Scan# 2293
Delta R.T. -0.05 min
Lab File: BF117979.D
Acq: 25 Nov 2019 21:26

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.4	29.0
265	21.5	17.1	25.7

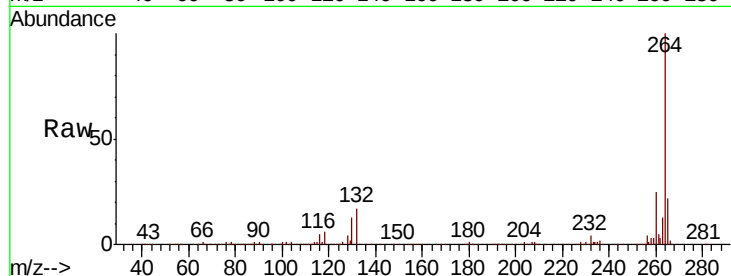

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

