
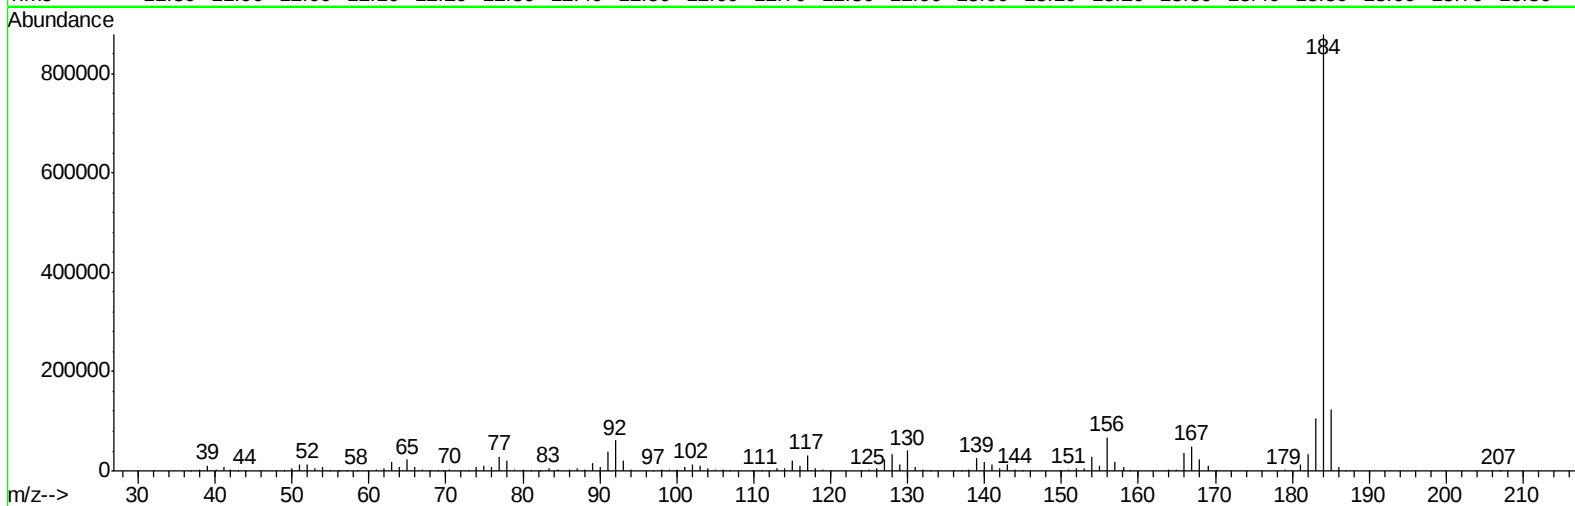


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112519\
Data File : BF117974.D
Acq On : 25 Nov 2019 18:37
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 07:30:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:38:20 2019
Response via : Initial Calibration

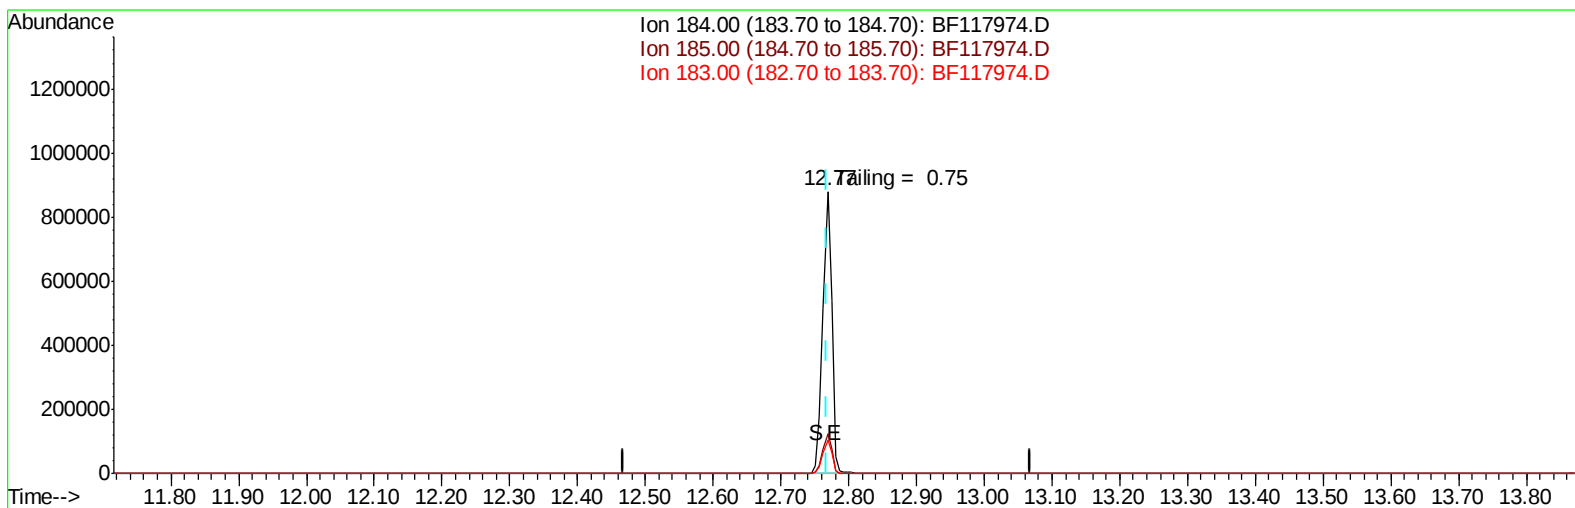

TIC: BF117974.D

(77) Benzidine



12.769min (+0.000) 0.00ng

response 782195

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.14
183.00	11.90	11.96
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112519\
Data File : BF117974.D
Acq On : 25 Nov 2019 18:37
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 07:30:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:38:20 2019
Response via : Initial Calibration

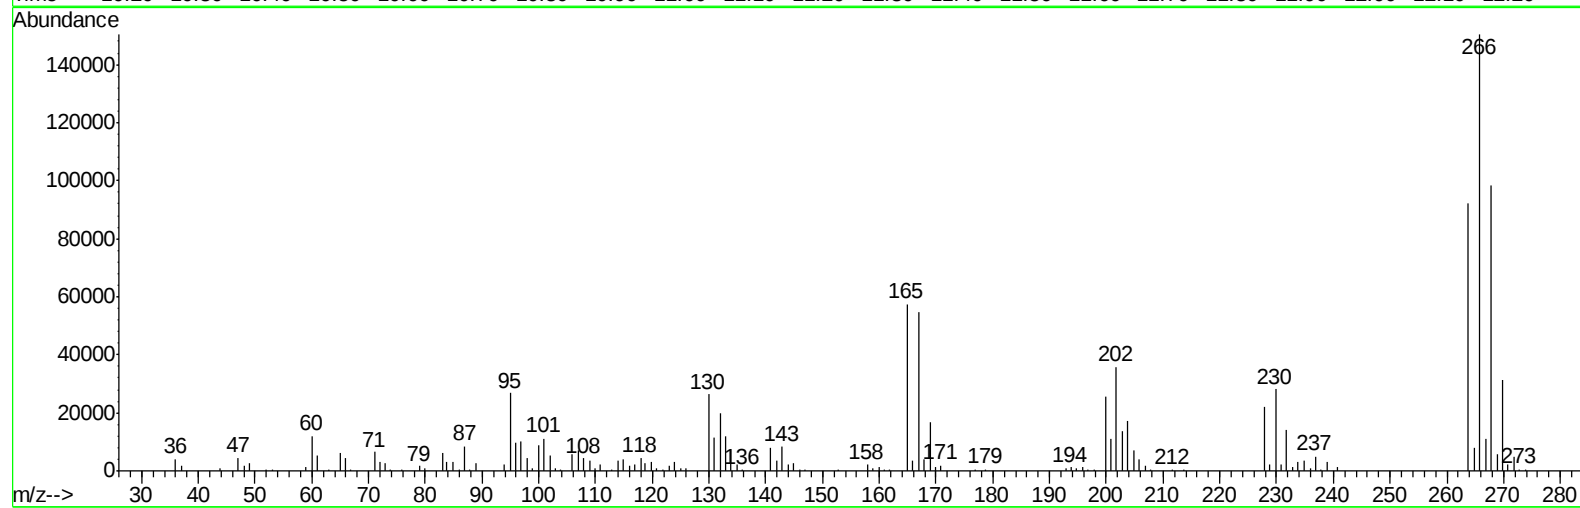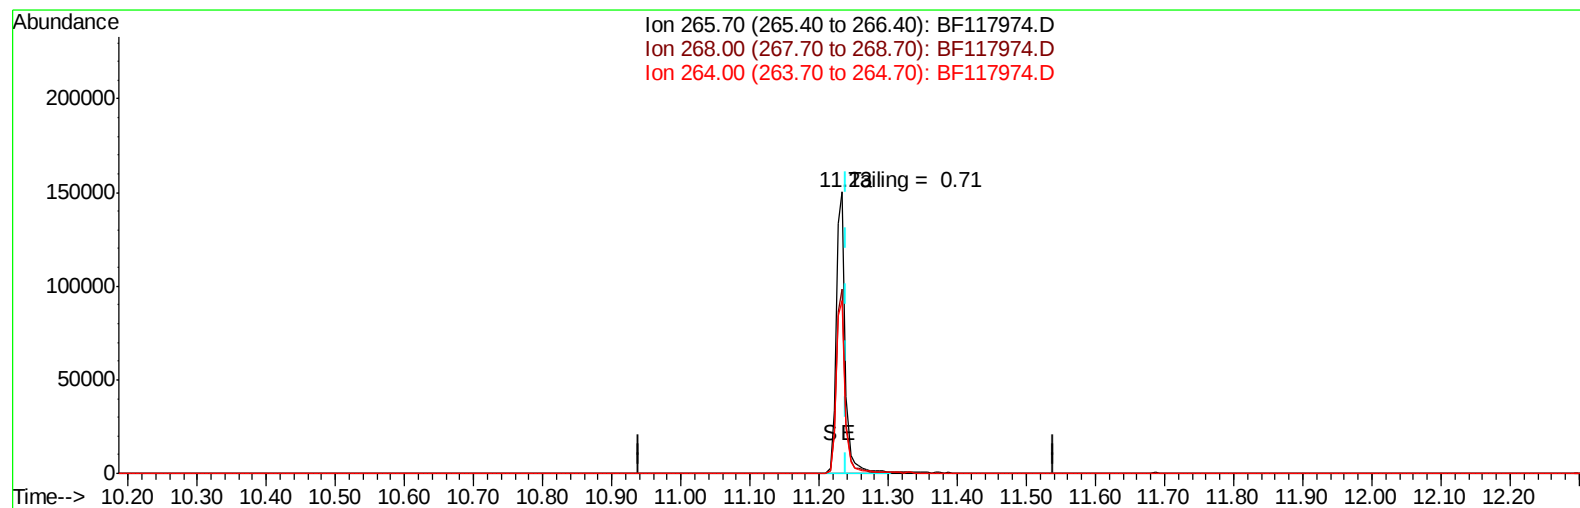

TIC: BF117974.D

(70) Pentachlorophenol (C)

11.233min (-0.006) 38001.58ng

response 138269

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	65.44
264.00	63.40	61.38
0.00	0.00	0.00