


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112519\
 Data File : BF117974.D
 Acq On : 25 Nov 2019 18:37
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 26 05:38:20 2019

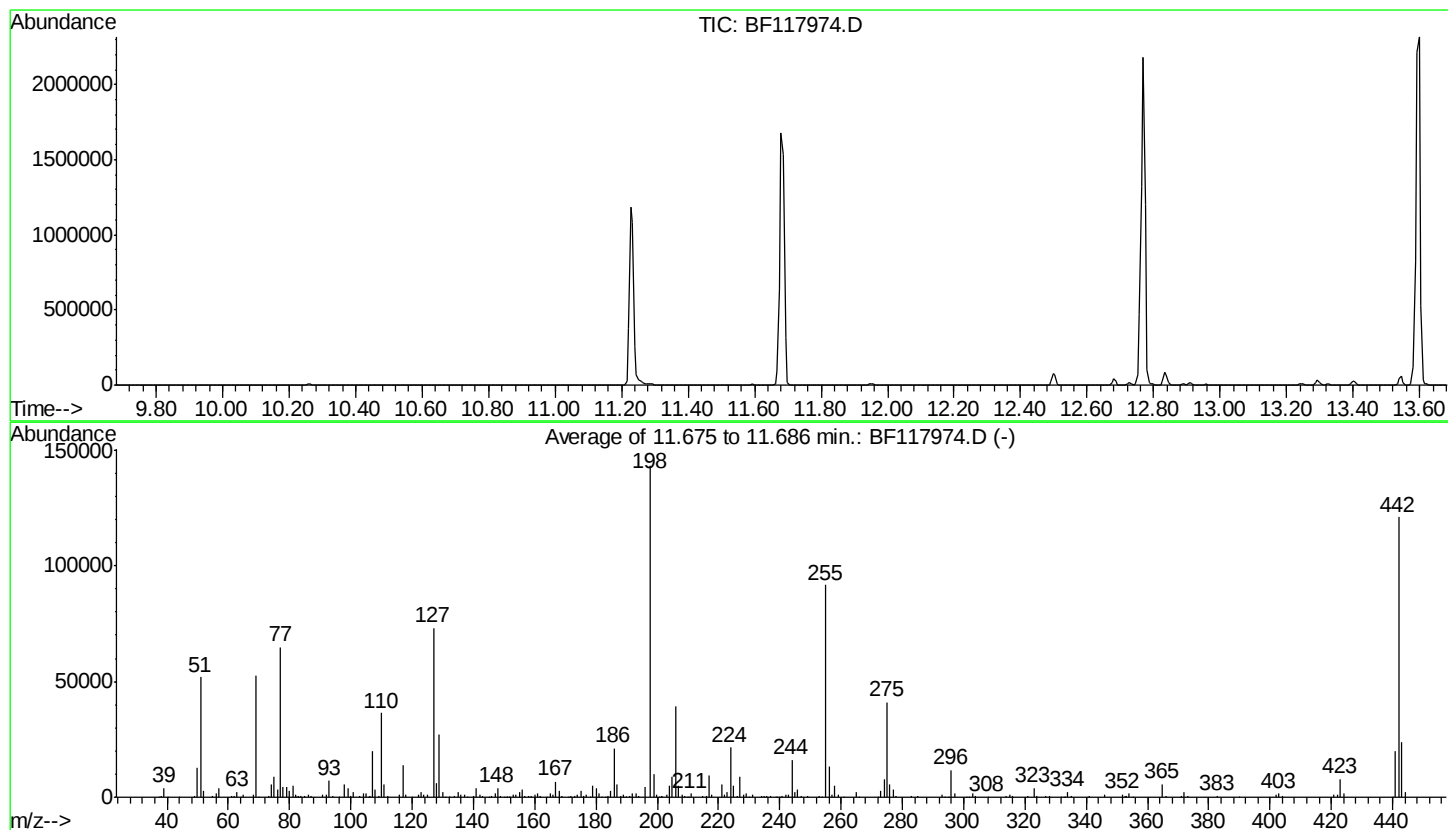

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	51877	PASS
68	69	0.00	2	1.9	993	PASS
69	198	0.00	100	36.7	52600	PASS
70	69	0.00	2	0.2	115	PASS
127	198	10	80	51.1	73282	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	143301	PASS
199	198	5	9	7.0	10067	PASS
275	198	10	60	28.6	41010	PASS
365	198	1	100	4.0	5772	PASS
441	198	0.01	100	13.9	19849	PASS
442	198	50	100	84.5	121074	PASS
443	442	15	24	19.8	23992	PASS