
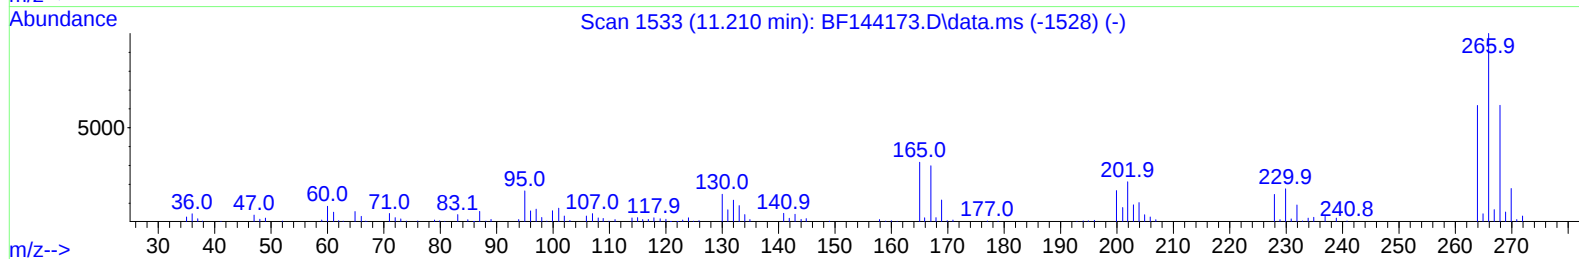
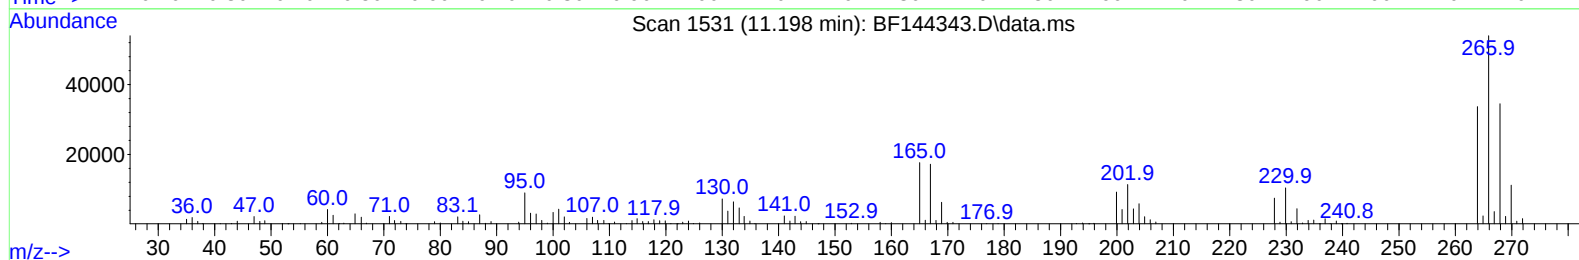


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112525\
Data File : BF144343.D
Acq On : 25 Nov 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 11:30:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

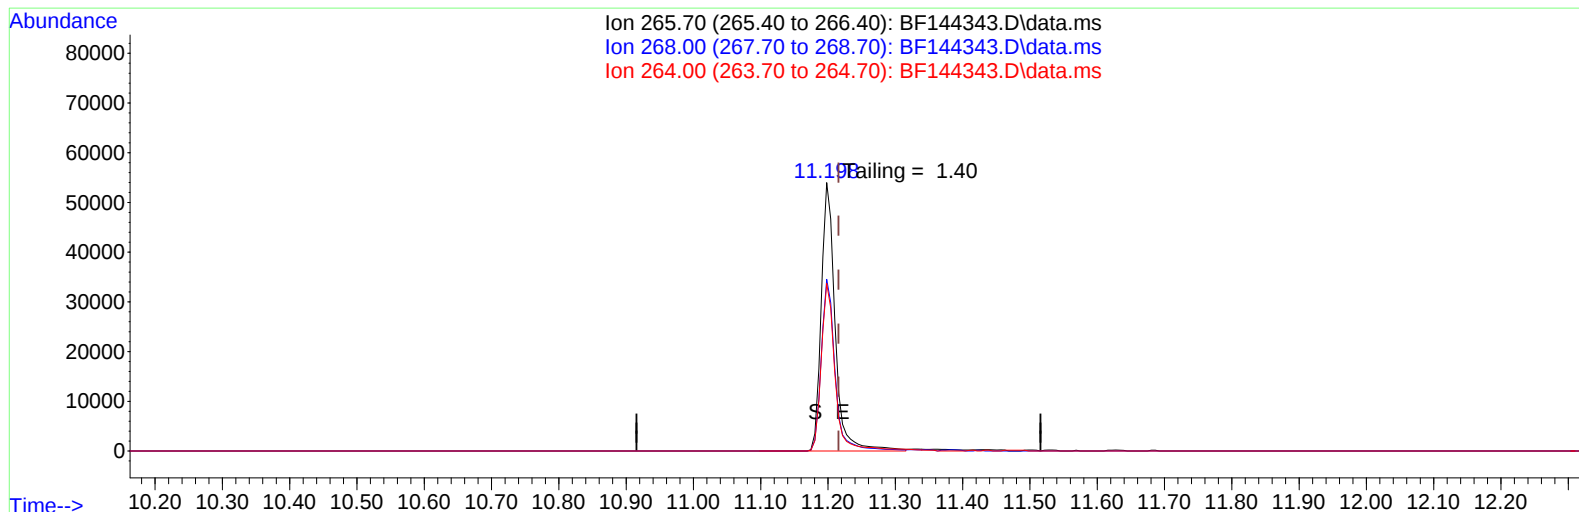

TIC: BF144343.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.018) 42461.47 ng

response 77883

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.97
264.00	61.80	62.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112525\
Data File : BF144343.D
Acq On : 25 Nov 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 11:30:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

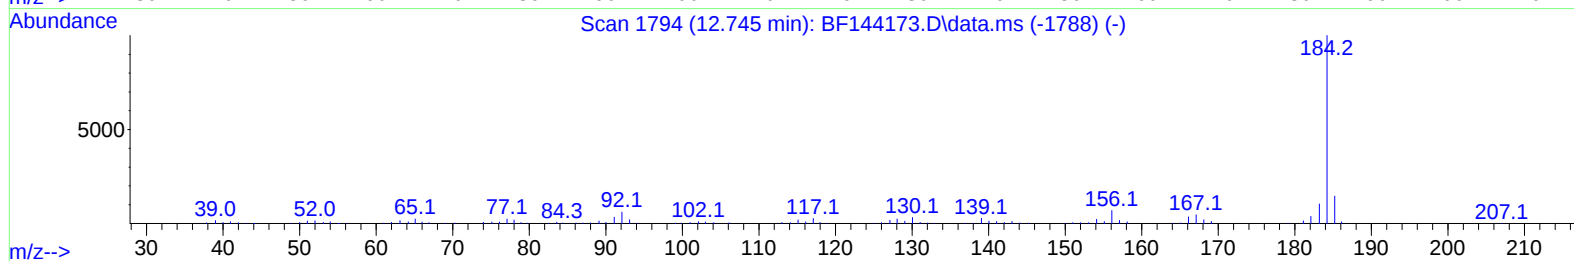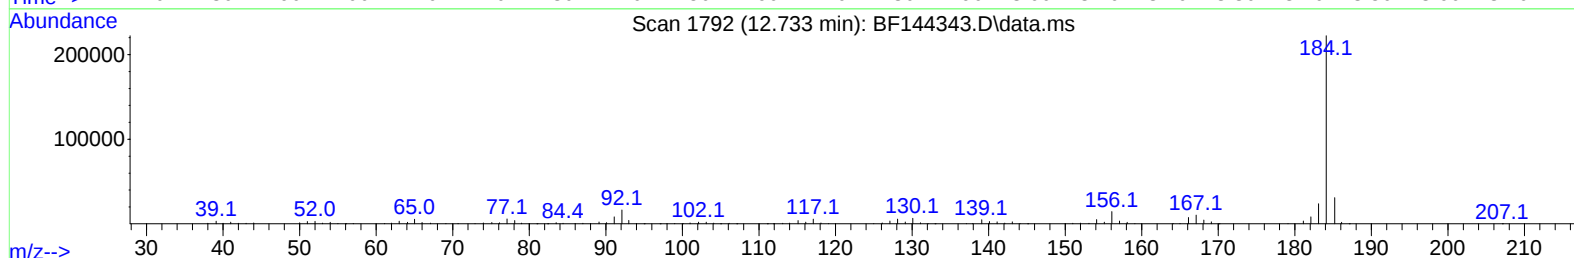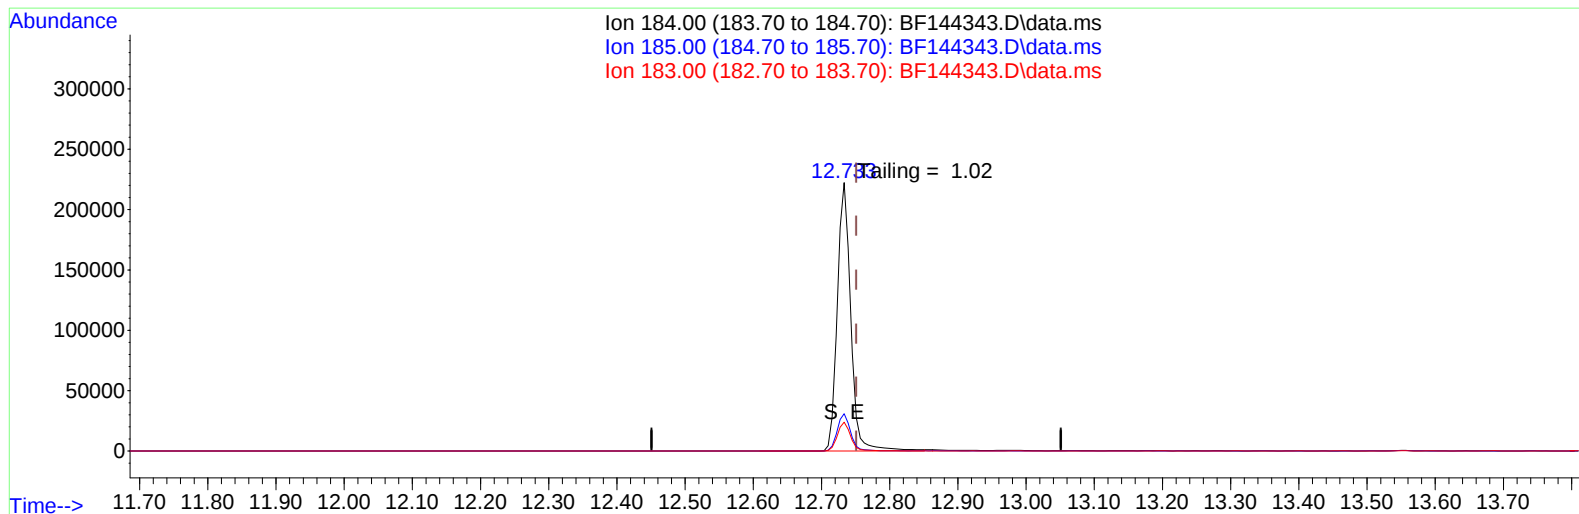

TIC: BF144343.D\data.ms

(77) Benzidine

12.733min (-0.018) 172655.66 ng m

response 301315

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.93
183.00	10.40	10.74
0.00	0.00	0.00