


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112525\
Data File : BF144343.D
Acq On : 25 Nov 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

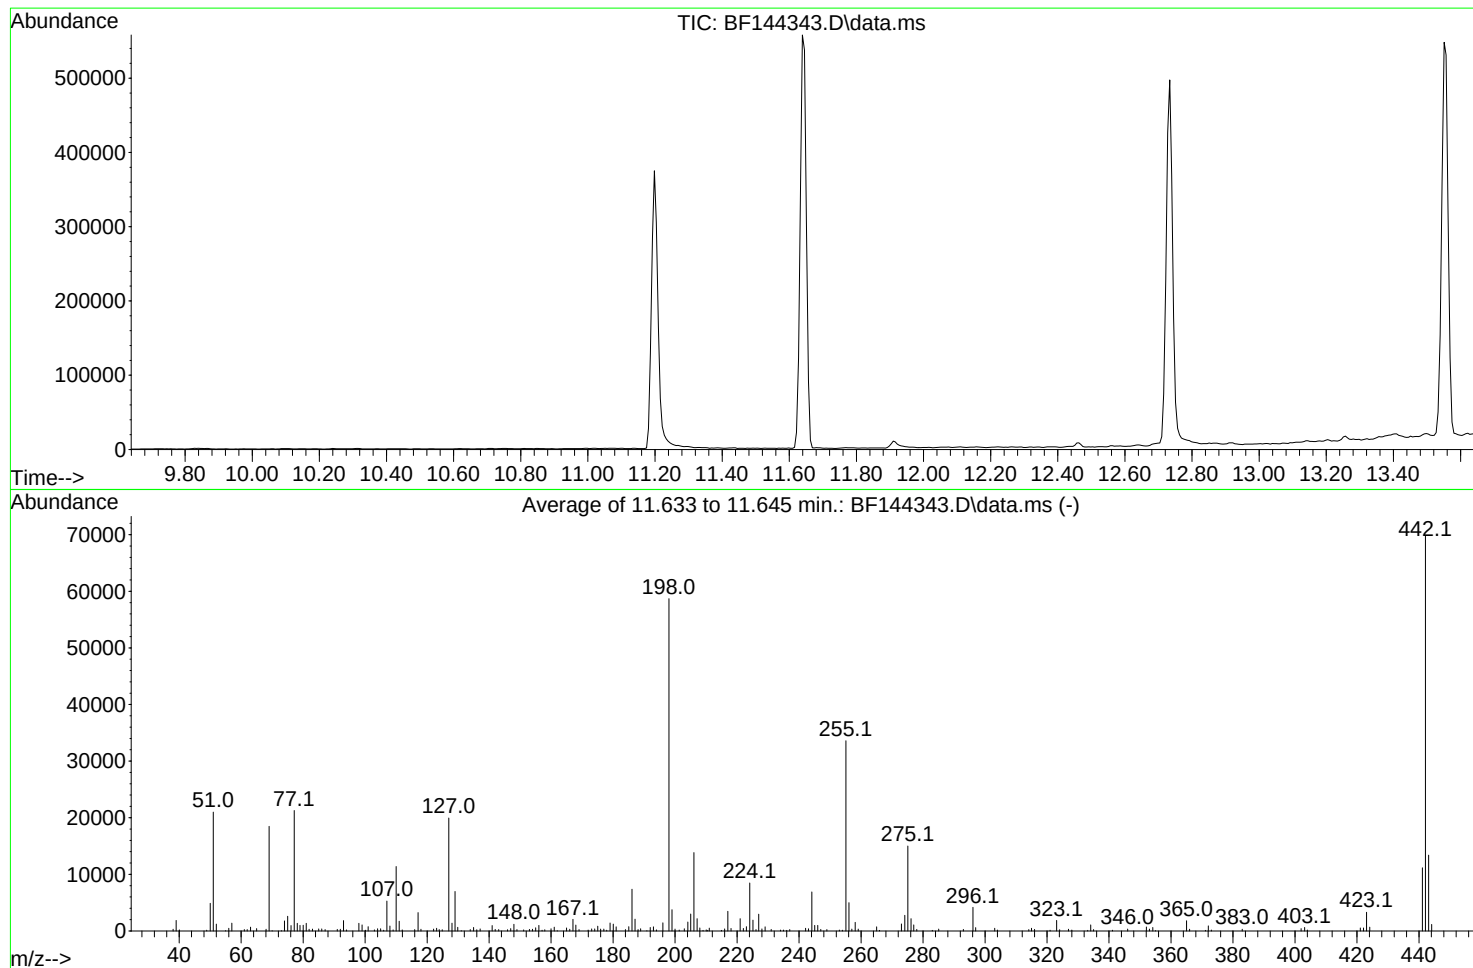


AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	307	PASS
69	69	100	100	100.0	18485	PASS
70	69	0.00	2	0.3	56	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58707	PASS
199	198	5	9	6.4	3761	PASS
365	198	1	100	3.1	1805	PASS
441	443	0.01	150	83.4	11167	PASS
442	442	100	100	100.0	69755	PASS
443	442	15	24	19.2	13383	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112525\
Data File : BF144343.D
Acq On : 25 Nov 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 11:30:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

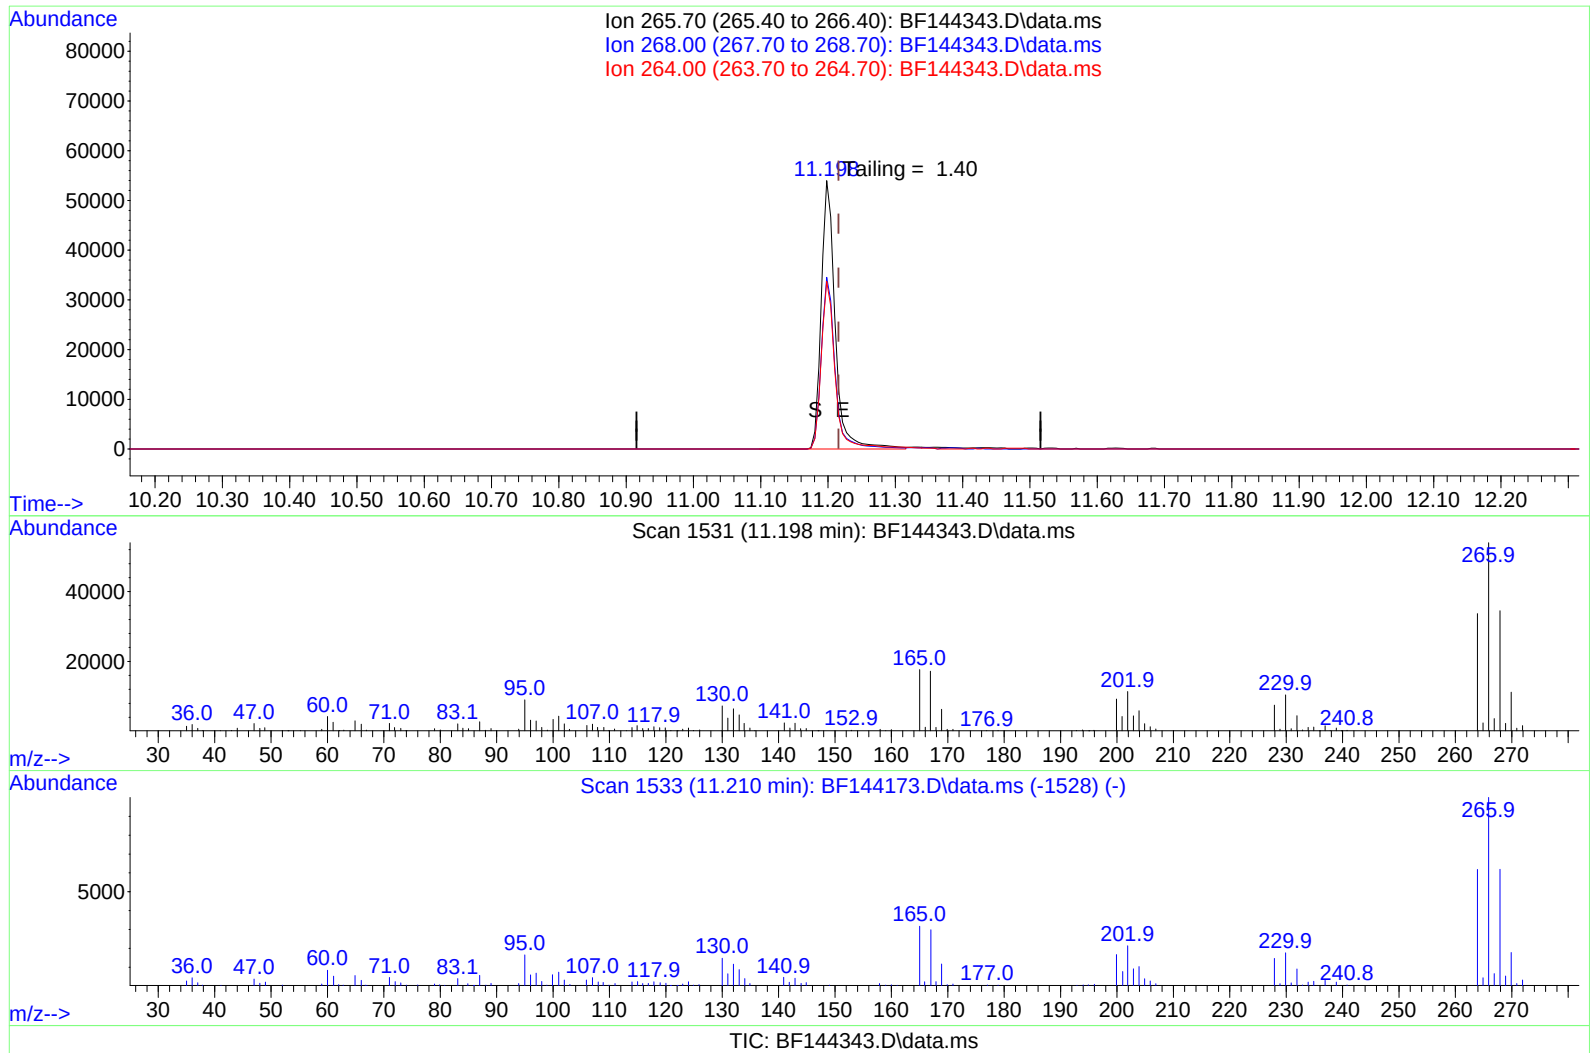

(70) Pentachlorophenol (C)

11.198min (-0.018) 42461.47 ng




response 77883

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	63.97
264.00	61.80	62.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112525\
Data File : BF144343.D
Acq On : 25 Nov 2025 11:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 11:30:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

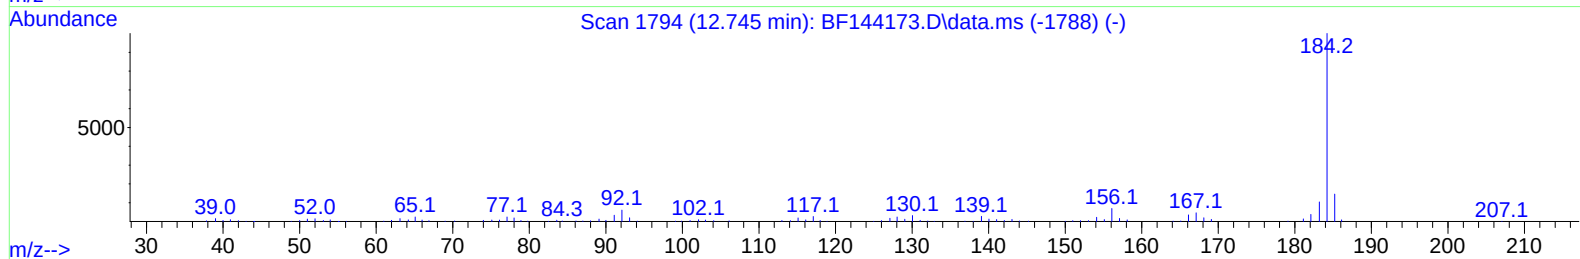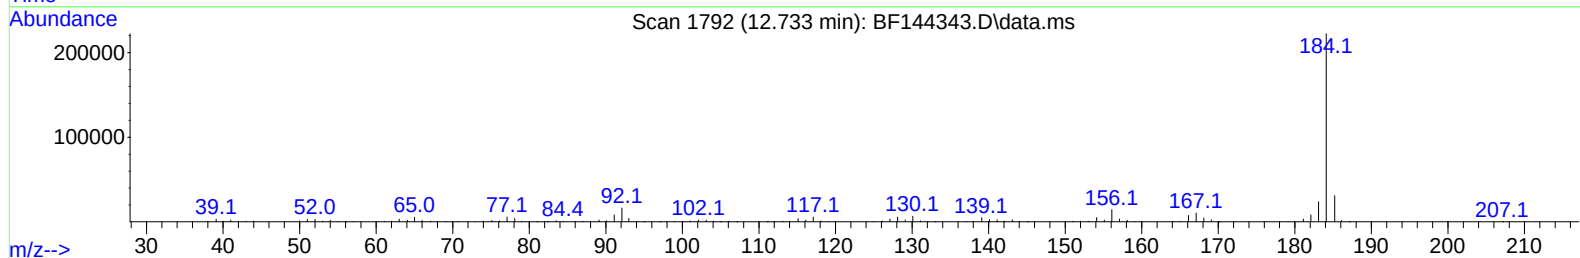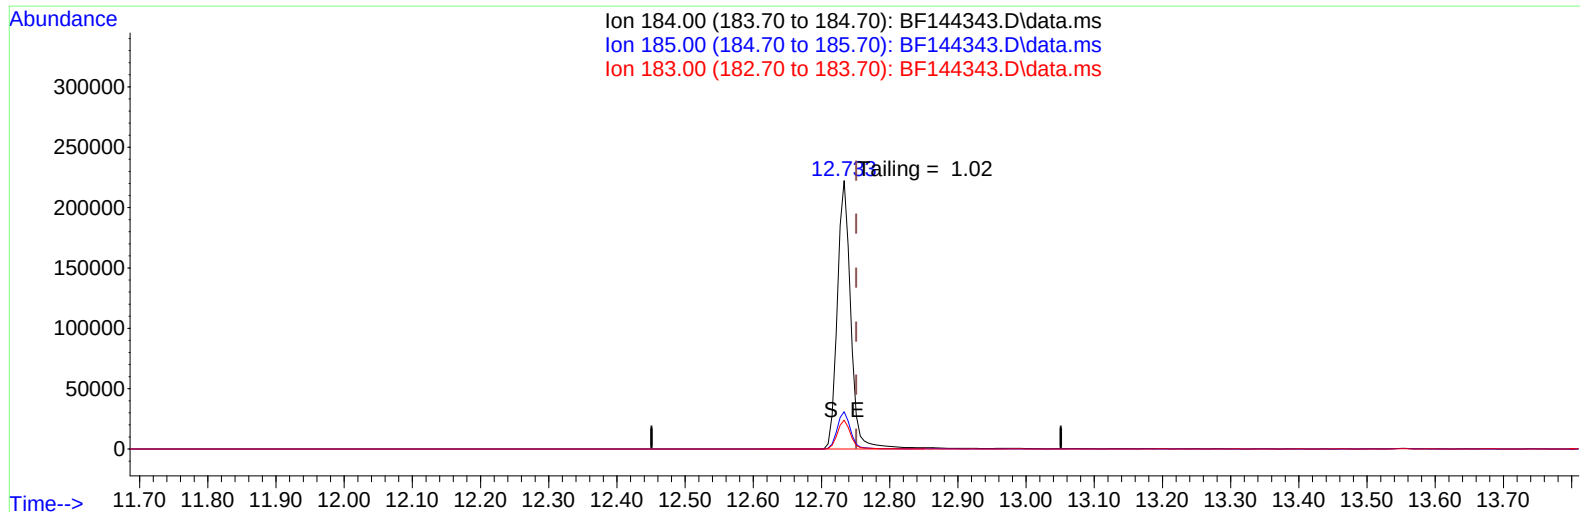

TIC: BF144343.D\data.ms

(77) Benzidine

12.733min (-0.018) 172655.66 ng m

response 301315

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.93
183.00	10.40	10.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/25/2025	BNA_F	<u>BF144343.D</u>
Compound Name	Response	Retention Time
DDT	152873	13.557
DDD	3300	13.257
DDE	416	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3716	156589	2.37

Instrument :
BNA_F
ClientSampleId :
DFTPP