
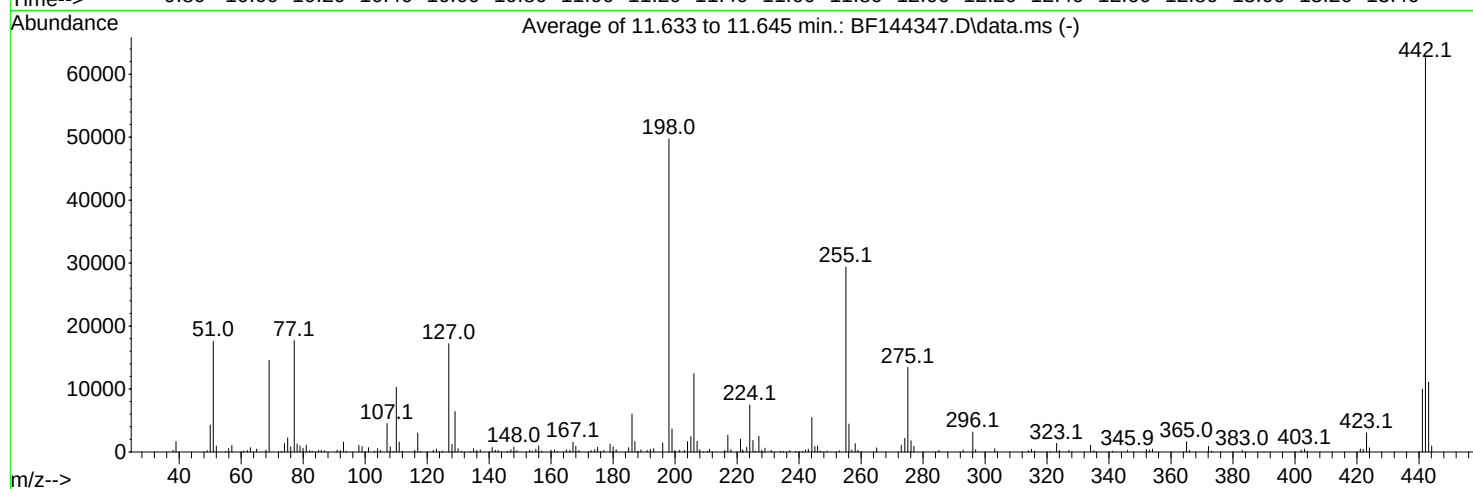


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112525\
Data File : BF144347.D
Acq On : 25 Nov 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 05 18:37:33 2025

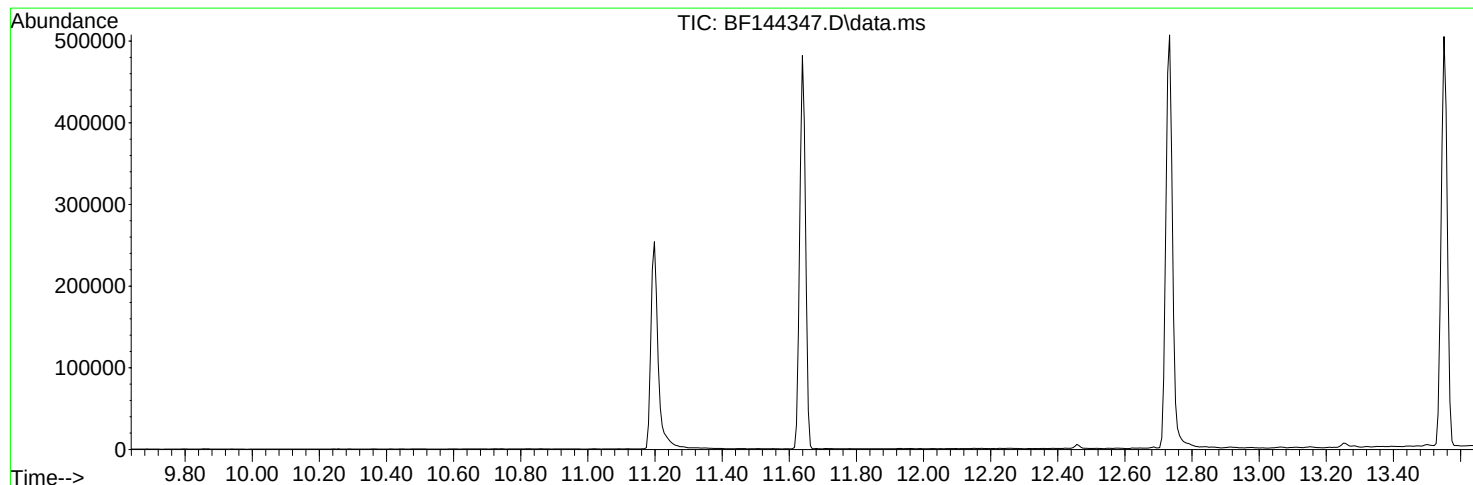




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	284	PASS
69	69	100	100	100.0	14547	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49736	PASS
199	198	5	9	7.3	3647	PASS
365	198	1	100	3.2	1605	PASS
441	443	0.01	150	89.7	9950	PASS
442	442	100	100	100.0	62712	PASS
443	442	15	24	17.7	11093	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112525\
Data File : BF144347.D
Acq On : 25 Nov 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 13:45:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

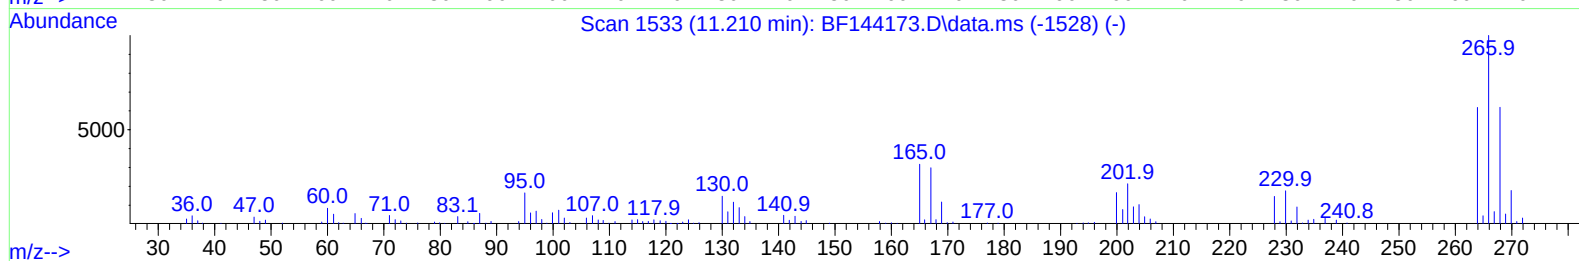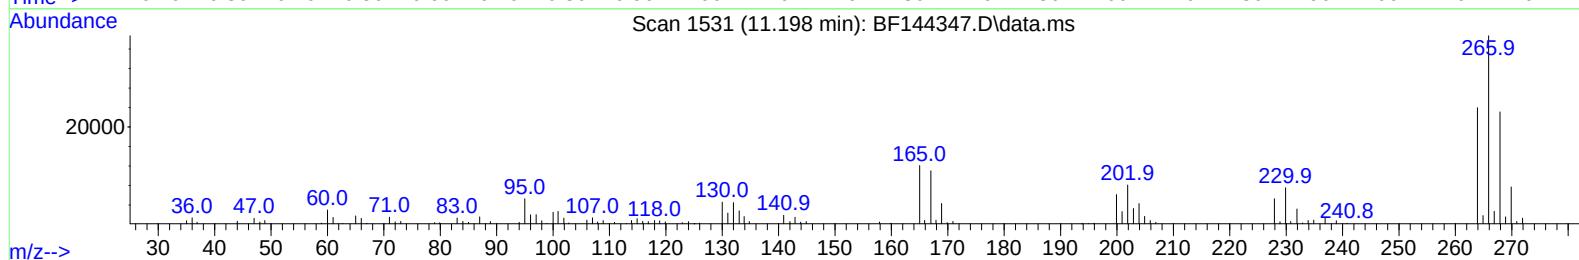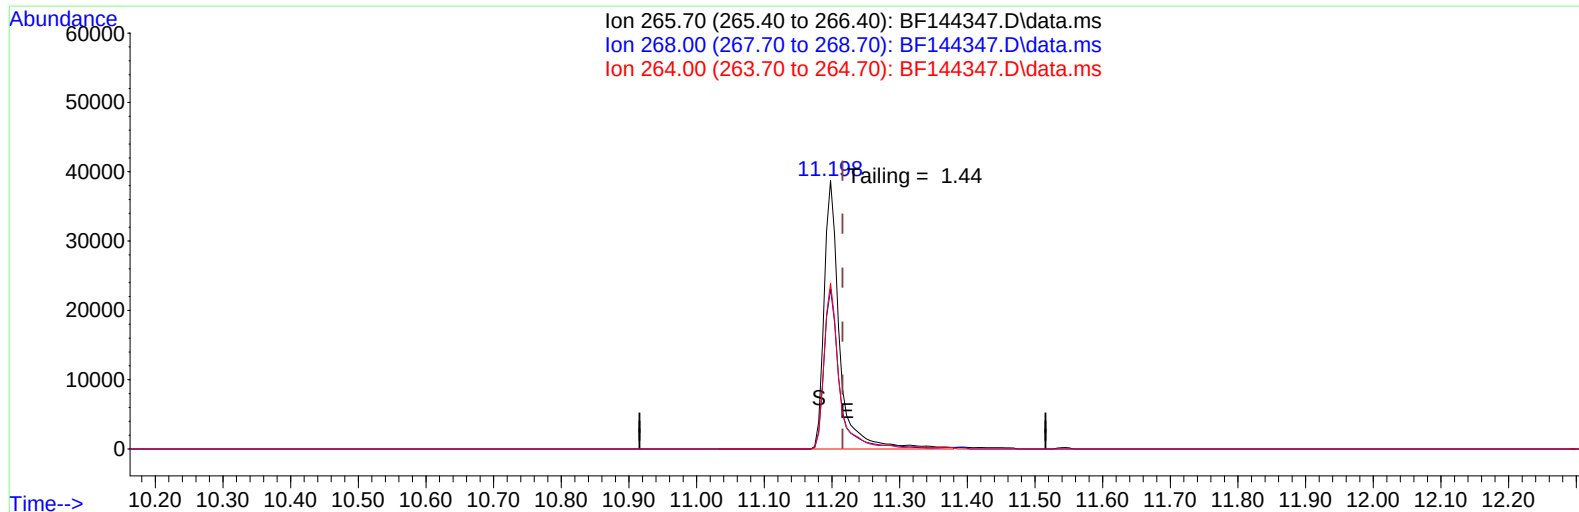

TIC: BF144347.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.018) 72689.45 ng m


response 62038

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	59.63
264.00	61.80	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112525\
Data File : BF144347.D
Acq On : 25 Nov 2025 13:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 25 13:45:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

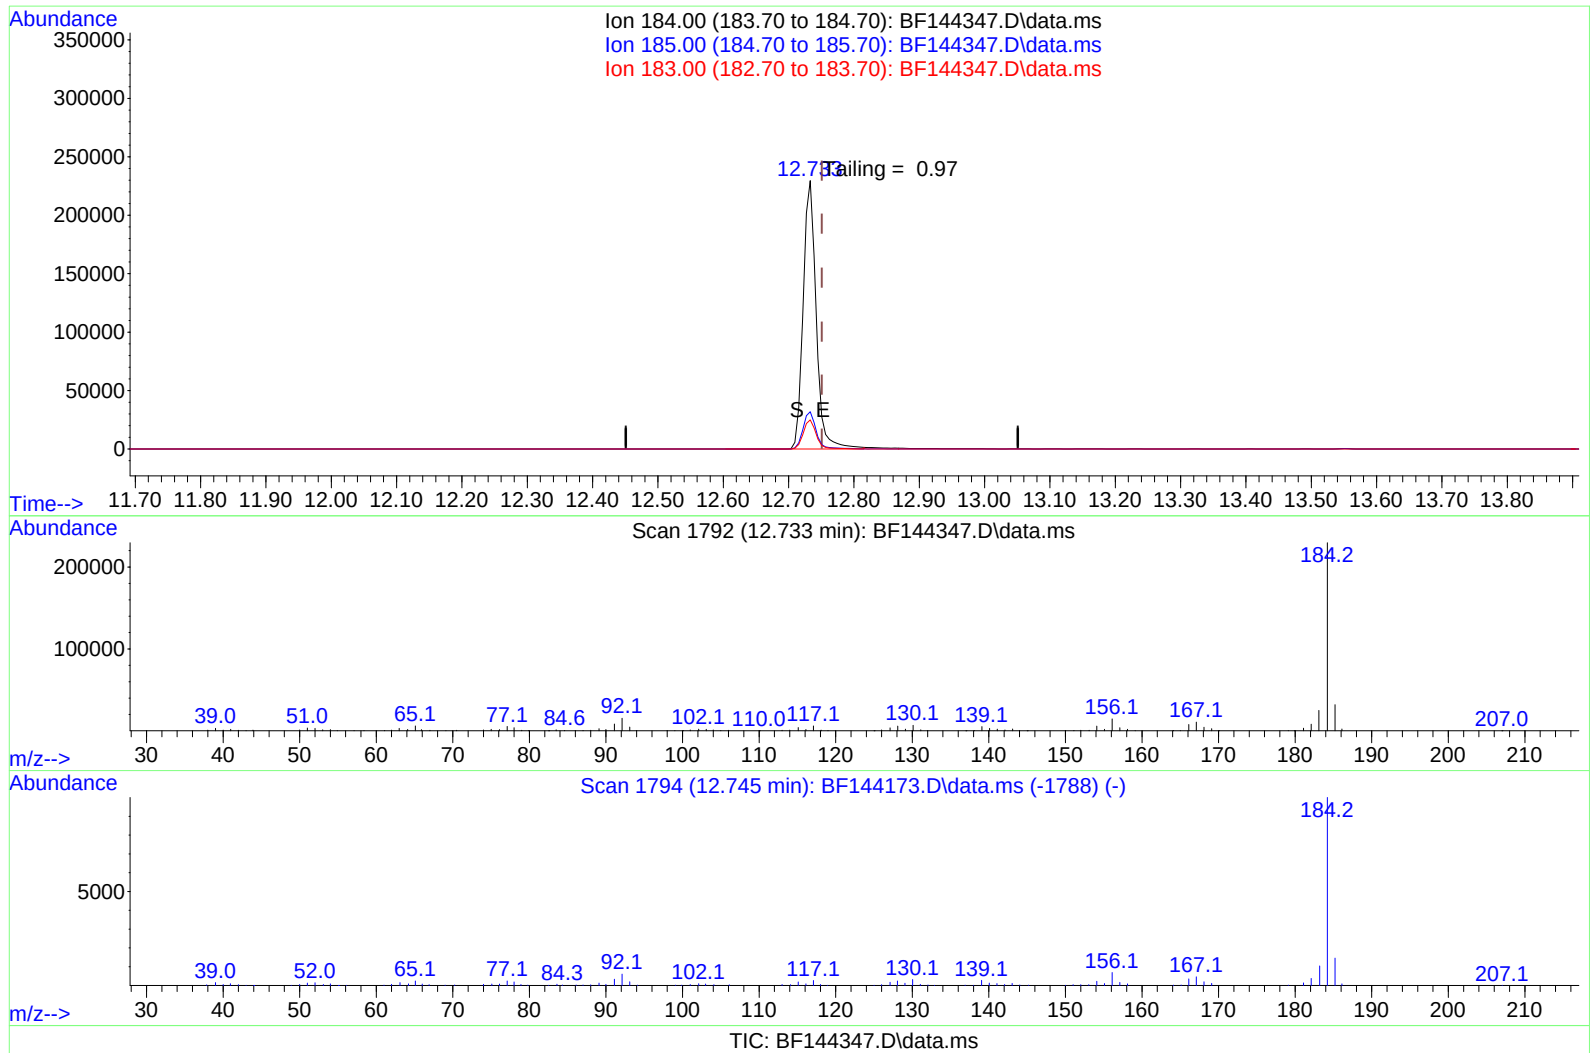

(77) Benzidine

12.733min (-0.018) 0.00 ng

response 322613

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.93
183.00	10.40	10.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/25/2025	BNA_F	<u>BF144347.D</u>
Compound Name	Response	Retention Time
DDT	137621	13.551
DDD	2636	13.257
DDE	363	12.915
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2999	140620	2.13

Instrument :
BNA_F
ClientSampleId :
DFTPP