
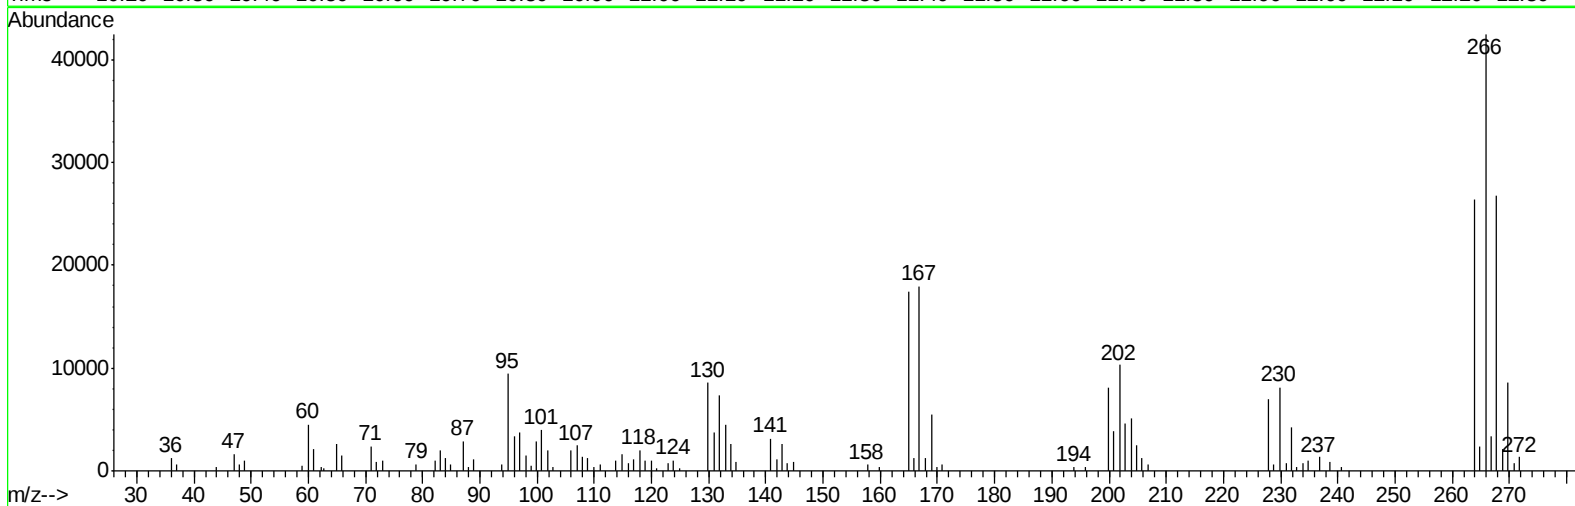


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112619\
Data File : BF118021.D
Acq On : 27 Nov 2019 1:30
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 08:25:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:38:20 2019
Response via : Initial Calibration

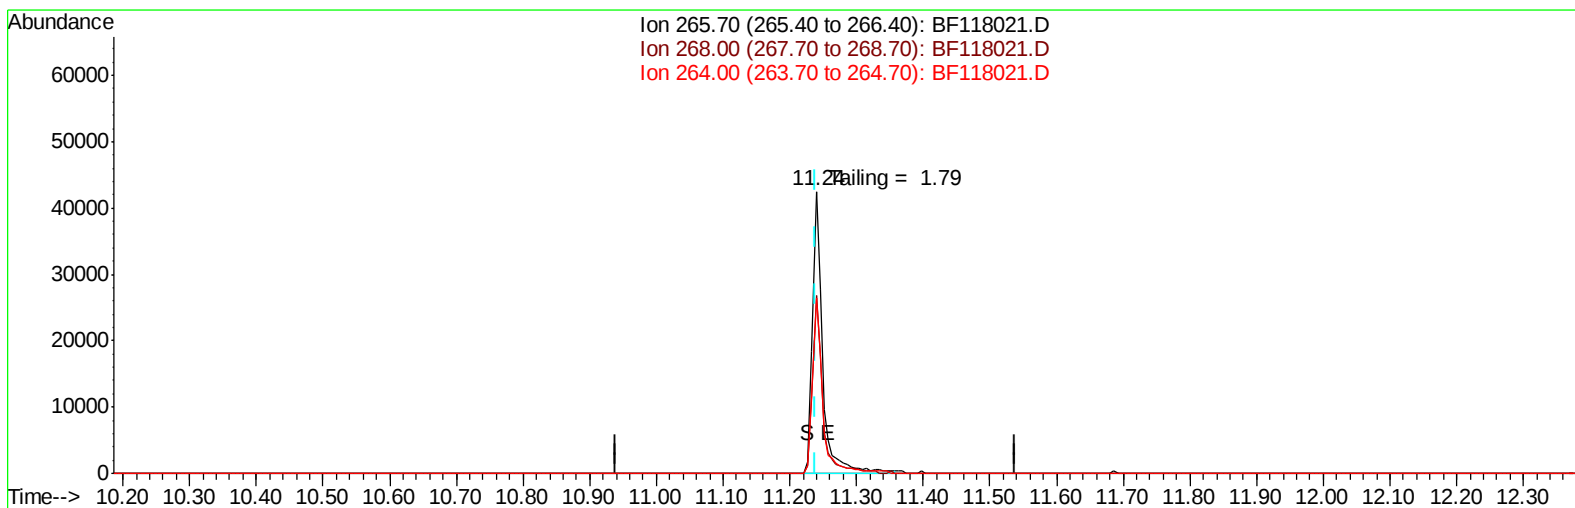

TIC: BF118021.D

(70) Pentachlorophenol (C)

11.239min (0.000) 25803.17ng

response 43244

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	63.03
264.00	63.40	62.07
0.00	0.00	0.00