
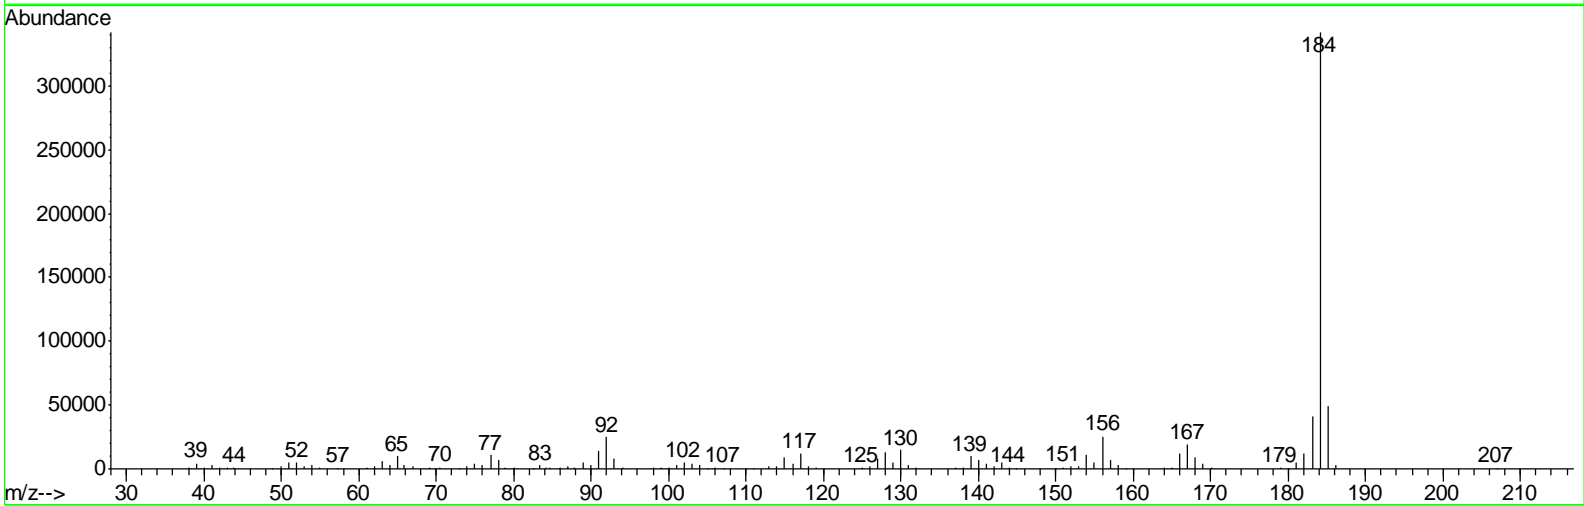


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112619\  
 Data File : BF118021.D  
 Acq On : 27 Nov 2019 1:30  
 Operator : JU  
 Sample : DF7TPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 08:25:19 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Nov 26 05:38:20 2019  
 Response via : Initial Calibration

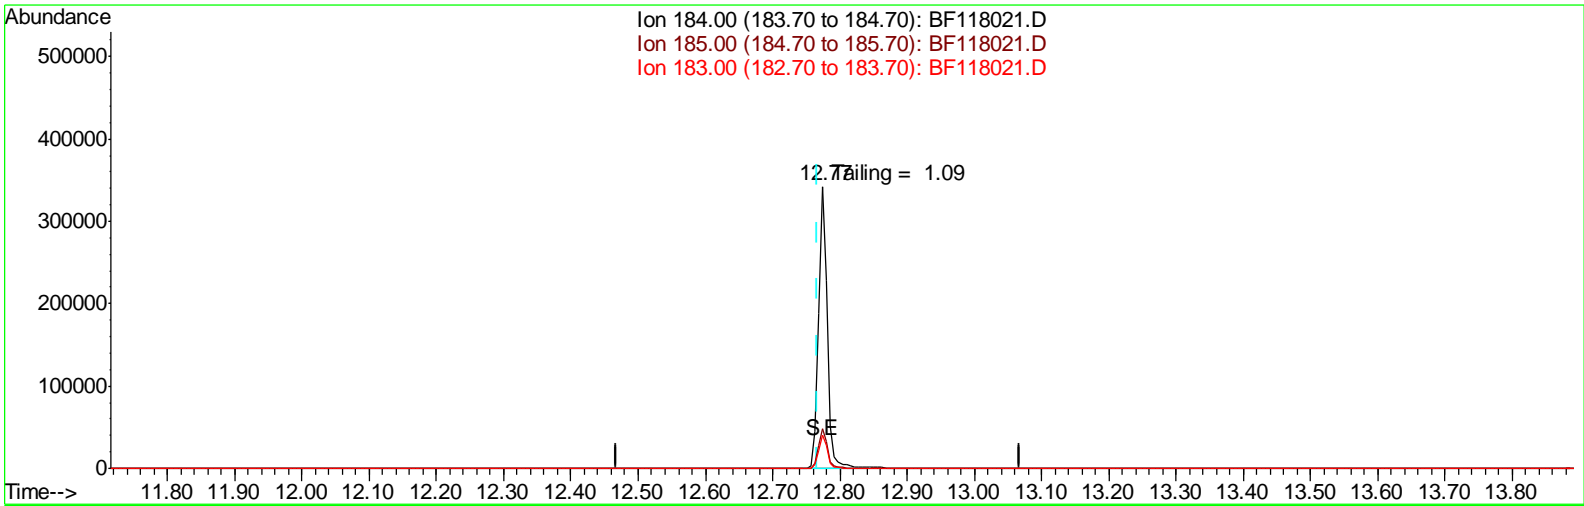

TIC: BF118021.D

(77) Benzidine

12.774min (+0.006) 0.00ng

response 319824

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.32
183.00	11.90	12.00
0.00	0.00	0.00