
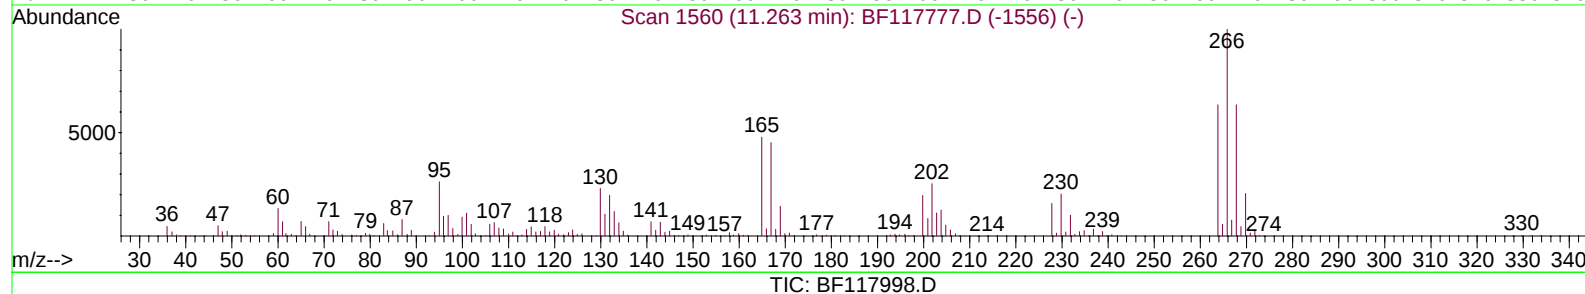
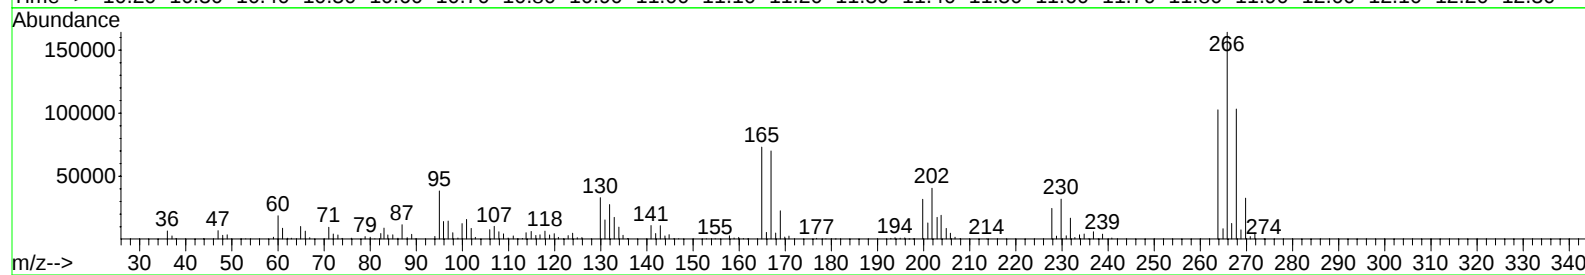


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112619\  
Data File : BF117998.D  
Acq On : 26 Nov 2019 9:51  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 18:12:22 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 26 05:38:20 2019  
Response via : Initial Calibration

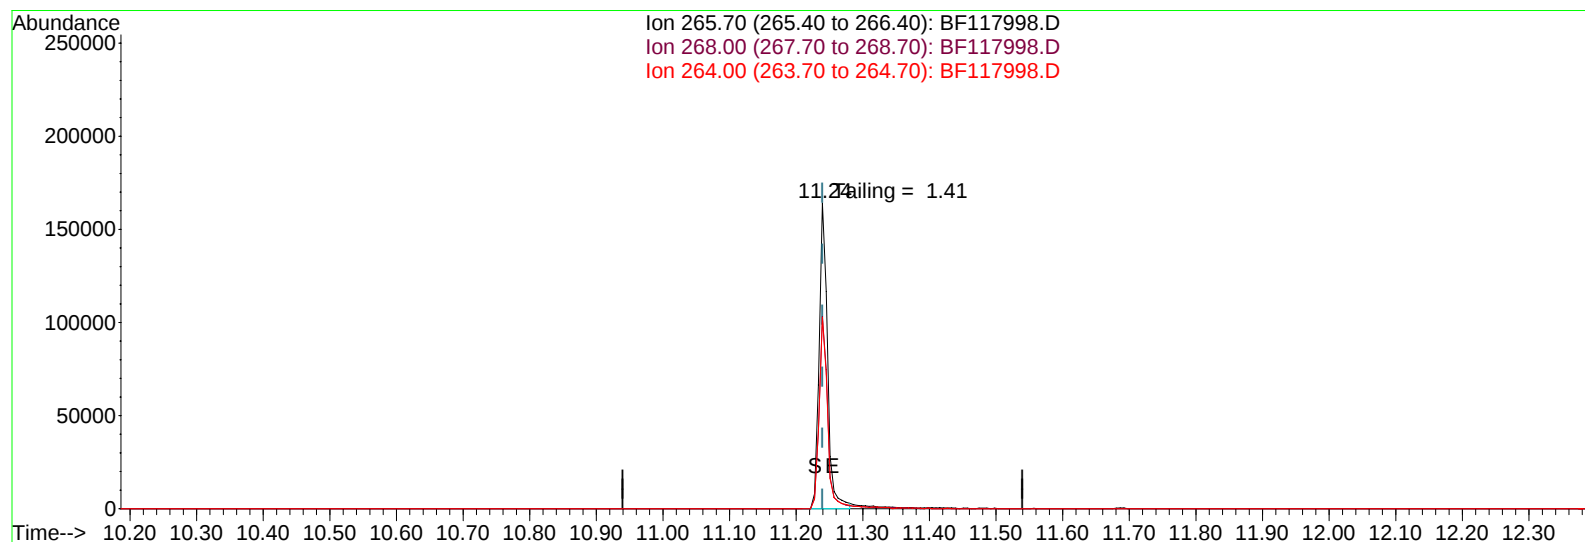

(70) Pentachlorophenol (C)




11.239min (+0.000) 52975.08ng

response 151085

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.50 | 62.90 |
| 264.00 | 63.40 | 62.55 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112619\  
Data File : BF117998.D  
Acq On : 26 Nov 2019 9:51  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 18:12:22 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 26 05:38:20 2019  
Response via : Initial Calibration

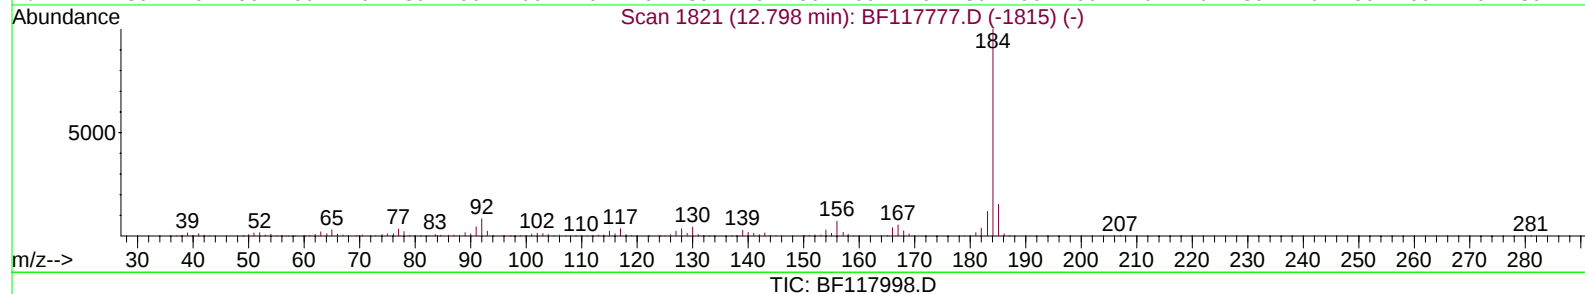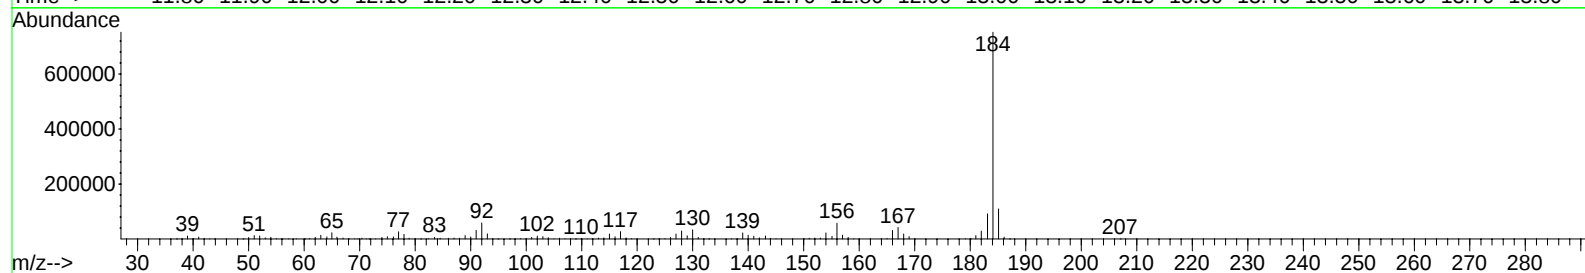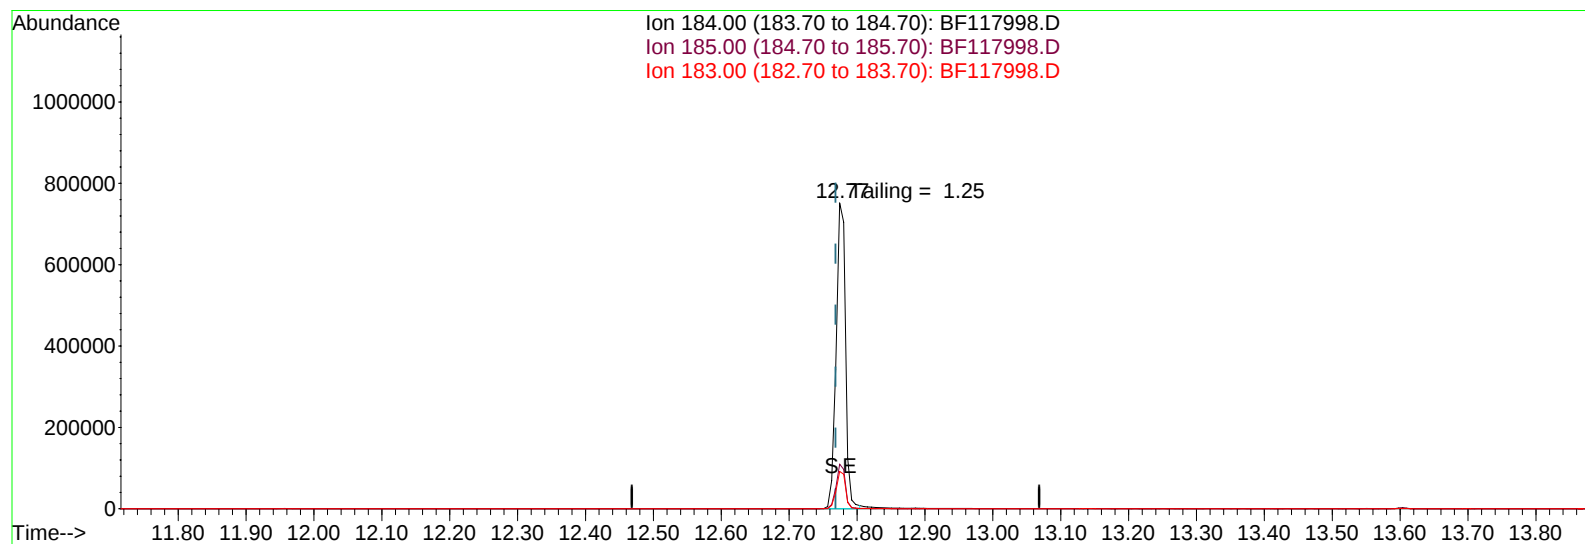

(77) Benzidine

12.774min (+0.006) 81422.59ng

response 730776

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.30 | 14.60 |
| 183.00 | 11.90 | 12.21 |
| 0.00   | 0.00  | 0.00  |