


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112619\
 Data File : BF117998.D
 Acq On : 26 Nov 2019 9:51
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 26 05:38:20 2019

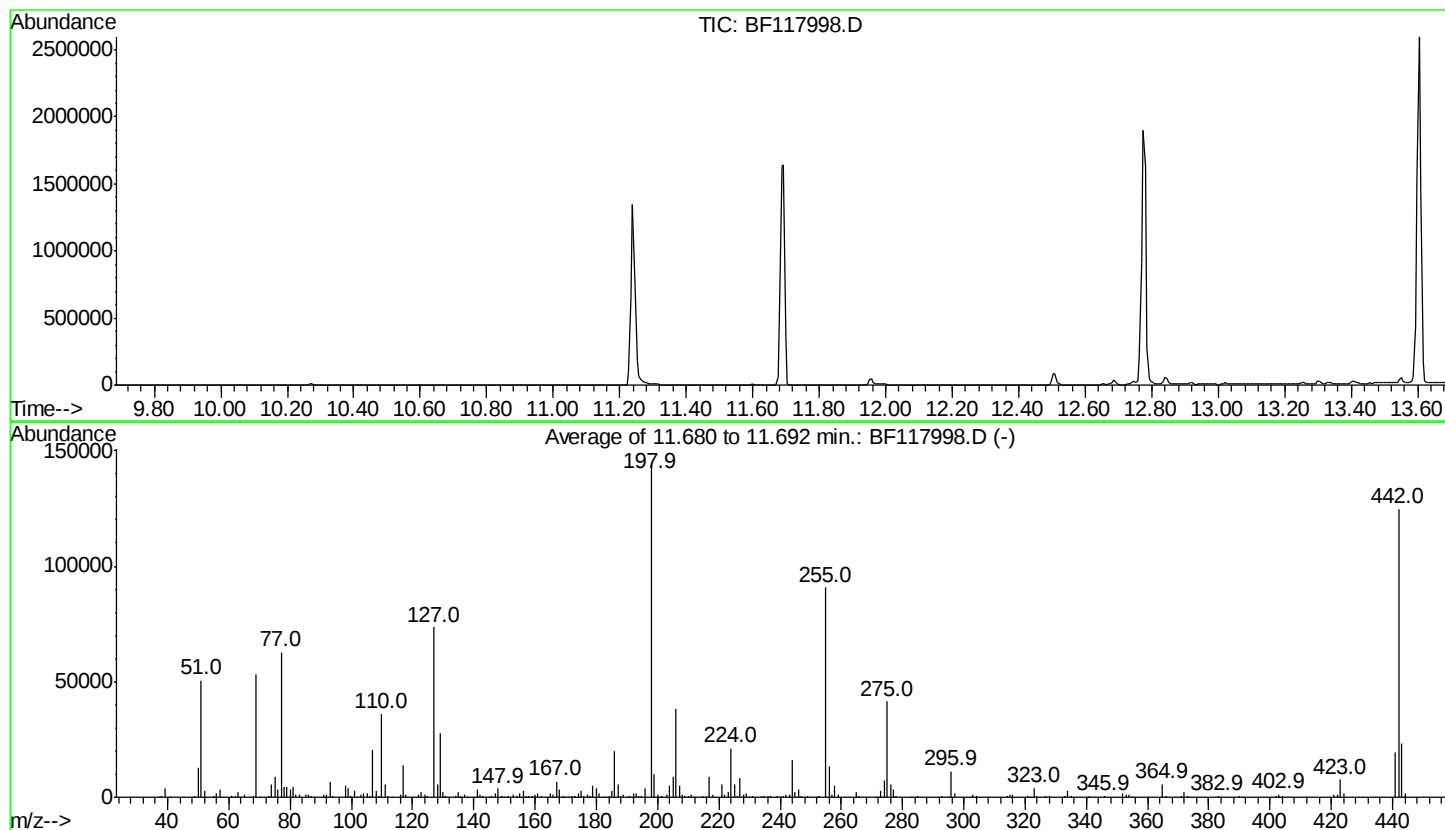

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	50528	PASS
68	69	0.00	2	1.5	774	PASS
69	198	0.00	100	37.2	53317	PASS
70	69	0.00	2	0.3	138	PASS
127	198	10	80	51.3	73661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	143504	PASS
199	198	5	9	6.8	9778	PASS
275	198	10	60	28.8	41297	PASS
365	198	1	100	4.0	5687	PASS
441	198	0.01	100	13.6	19464	PASS
442	198	50	100	87.0	124797	PASS
443	442	15	24	18.5	23055	PASS