

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112718\
 Data File : BF110999.D
 Acq On : 27 Nov 2018 10:25
 Operator : JU/SJ
 Sample : J5774-05RE 2X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 27 12:56:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 27 06:43:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	54654	20.00	ng	0.00
21) Naphthalene-d8	8.22	136	204102	20.00	ng	0.00
39) Acenaphthene-d10	9.98	164	75419	20.00	ng	0.00
64) Phenanthrene-d10	11.47	188	121838	20.00	ng	0.00
76) Chrysene-d12	14.13	240	131552	20.00	ng	0.00
87) Perylene-d12	15.67	264	115395	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	163076	49.48	ng	0.00
7) Phenol-d6	6.56	99	206555	48.09	ng	0.00
23) Nitrobenzene-d5	7.50	82	127996	35.89	ng	0.00
42) 2,4,6-Tribromophenol	10.78	330	31473	42.02	ng	0.00
45) 2-Fluorobiphenyl	9.29	172	200724	38.56	ng	0.00
79) Terphenyl-d14	13.06	244	165636	24.51	ng	0.00


Target Compounds				Qvalue		
9) Benzaldehyde	6.63	77	600	Below Cal	#	1
10) Phenol	6.58	94	11209	2.317 ng		92
19) n-Nitroso-di-n-propylamine	7.50	70	16855	6.025 ng	#	83
25) Isophorone	7.50	82	127996	21.880 ng	#	67
50) Dimethylphthalate	9.69	163	25204	4.557 ng		99
51) 2,6-Dinitrotoluene	9.98	165	9951	8.081 ng	#	21
52) Acenaphthene	10.01	154	12614	2.745 ng		96
56) 4-Nitrophenol	10.19	139	4544	9.631 ng	#	6
57) 2,4-Dinitrotoluene	9.98	165	9951	6.229 ng	#	17
58) Fluorene	10.53	166	21445	4.111 ng		96
71) Phenanthrene	11.50	178	120743	18.711 ng		99
72) Anthracene	11.56	178	35164	5.351 ng		97
75) Fluoranthene	12.70	202	151951	22.911 ng		99
78) Pyrene	12.93	202	165035	17.176 ng		97
81) Benzo(a)anthracene	14.12	228	79392	10.222 ng		98
83) Chrysene	14.12	228	79392	10.384 ng		95
86) Indeno(1,2,3-cd)pyrene	17.27	276	23378	4.260 ng		94
88) Benzo(b)fluoranthene	15.22	252	90021	13.279 ng	#	94
89) Benzo(k)fluoranthene	15.22	252	90021	12.902 ng	#	93
90) Benzo(a)pyrene	15.61	252	52839	8.374 ng	#	96
92) Benzo(a,h,i)perylene	17.76	276	23201	4.622 ng		96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112718\
Data File : BF110999.D
Acq On : 27 Nov 2018 10:25
Operator : JU/SJ
Sample : J5774-05RE 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 27 12:56:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 27 06:43:50 2018
Response via : Initial Calibration

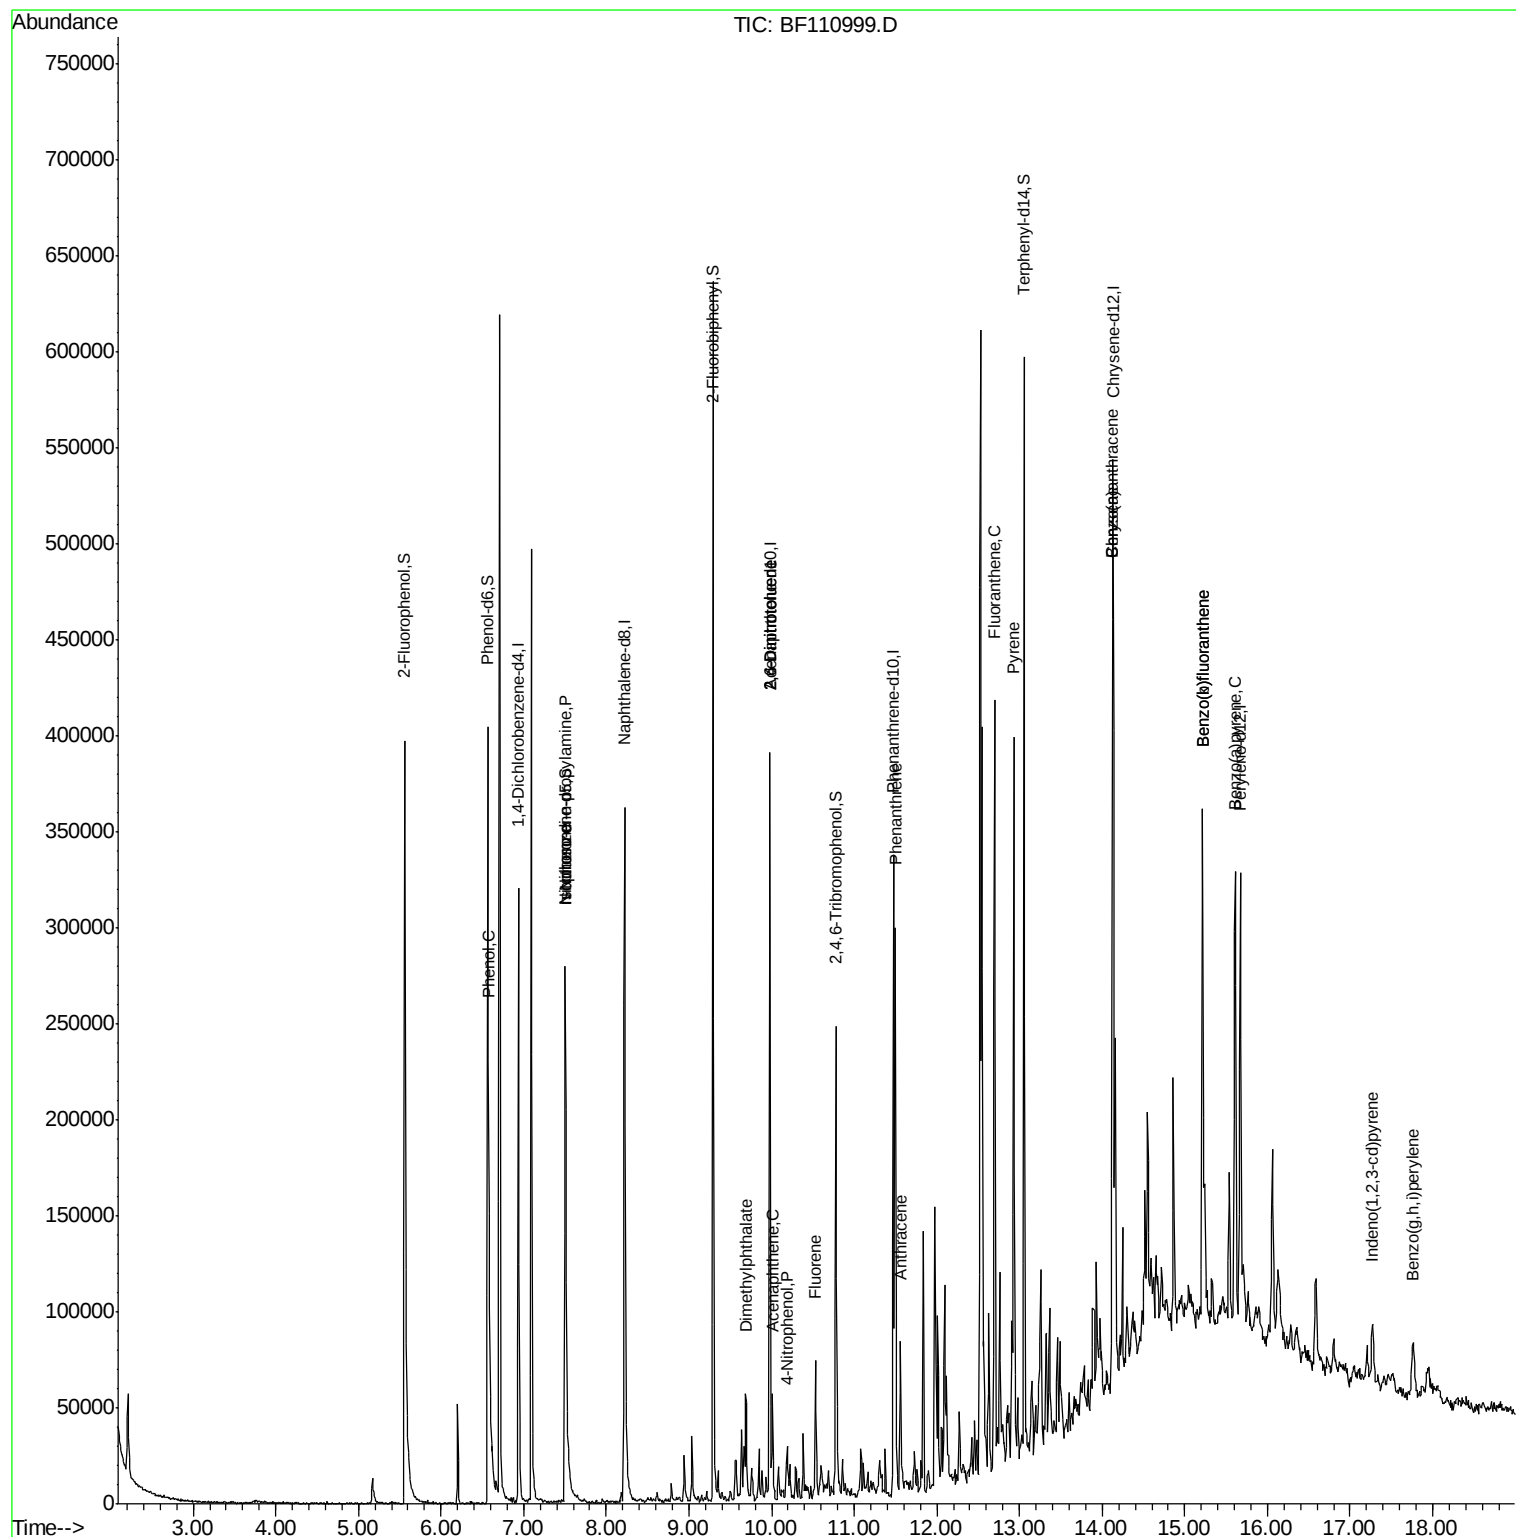

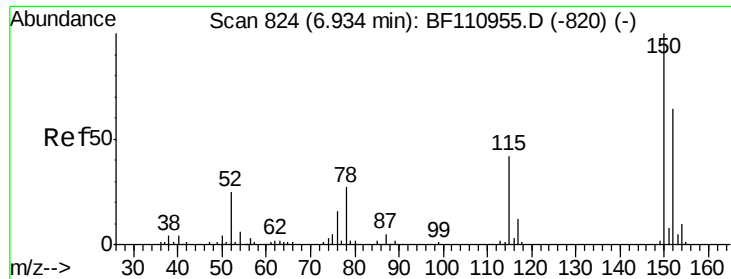


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.94 min Scan# 825
Delta R.T. 0.01 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 54654
Ion Ratio Lower Upper
152 100
150 157.0 122.7 184.1
115 60.6 49.1 73.7

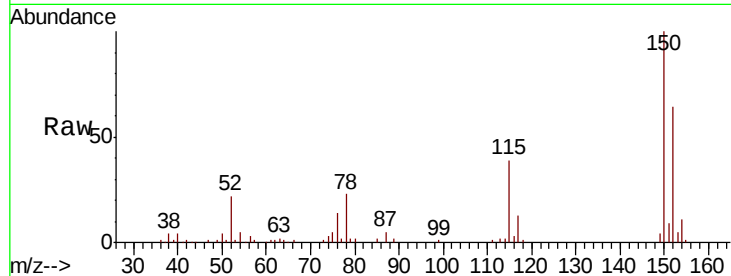


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

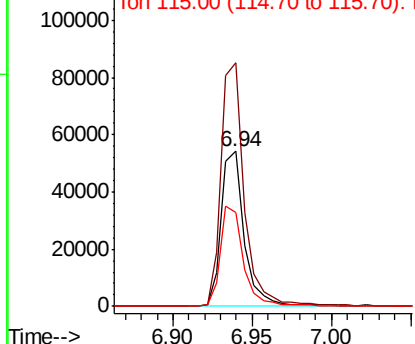



#5


2-Fluorophenol
Concen: 49.481 ng
RT: 5.56 min Scan# 590
Delta R.T. 0.01 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Tgt Ion:112 Resp: 163076
Ion Ratio Lower Upper
112 100
64 61.5 44.1 66.1
63 32.9 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

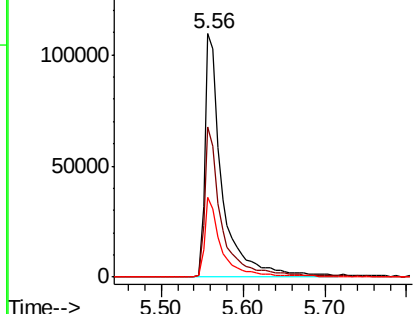

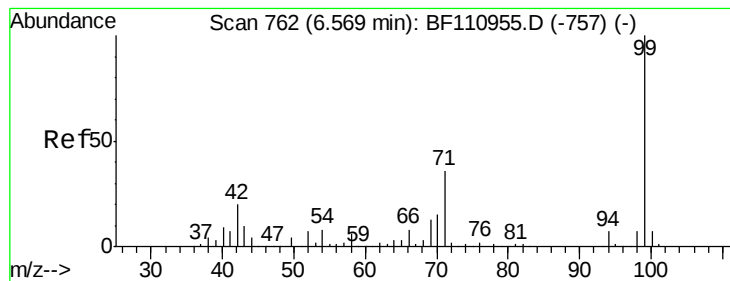

#7

Phenol-d6

Concen: 48.093 ng

RT: 6.56 min Scan# 761

Delta R.T. -0.01 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 206555

Ion Ratio Lower Upper




99 100

42 20.5 15.8 23.6

71 36.7 28.0 42.0



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

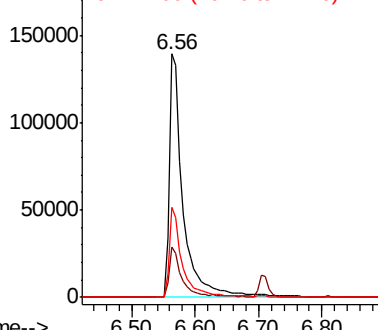

#10

Phenol

Concen: 2.317 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.00 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25


Tgt Ion: 94 Resp: 11209

Ion Ratio Lower Upper



94 100


65 40.8 25.3 65.3

66 82.2 54.5 94.5



Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1




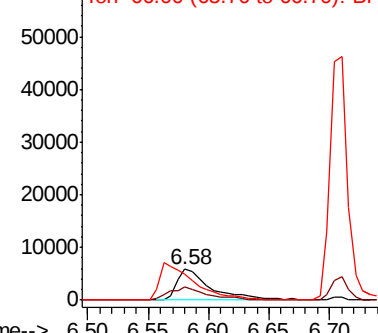




#19
n-Nitroso-di-n-propylamine
Concen: 6.025 ng
RT: 7.50 min Scan# 921
Delta R.T. 0.16 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 70 Resp: 16855
Ion Ratio Lower Upper
70 100
42 52.8 47.4 71.2
101 0.0 7.3 10.9#
130 2.8 16.2 24.2#

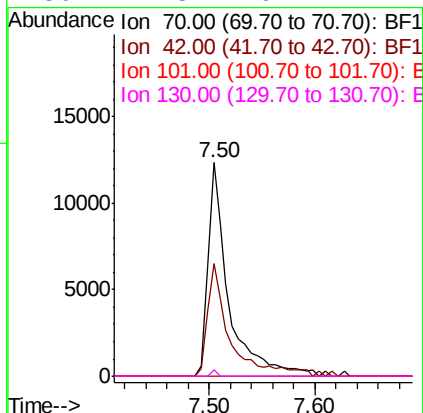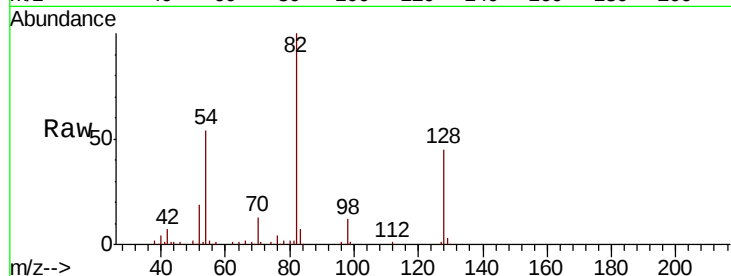

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.22 min Scan# 1043
Delta R.T. -0.00 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Tgt Ion: 136 Resp: 204102
Ion Ratio Lower Upper
136 100
137 10.9 8.8 13.2
54 7.9 5.4 8.2
68 4.8 4.2 6.2

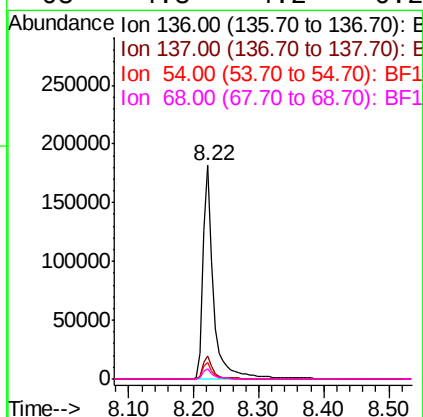







#23
 Nitrobenzene-d5
 Concen: 35.890 ng
 RT: 7.50 min Scan# 921
 Delta R.T. -0.01 min
 Lab File: BF110999.D
 Acq: 27 Nov 2018 10:25

Instrument :
 BNA_F
 ClientSampleID :

Tot Ion	82	Resp	127996
Ion Ratio	Lower	Upper	
82	100		
128	45.0	34.2	51.2
54	53.9	38.6	58.0

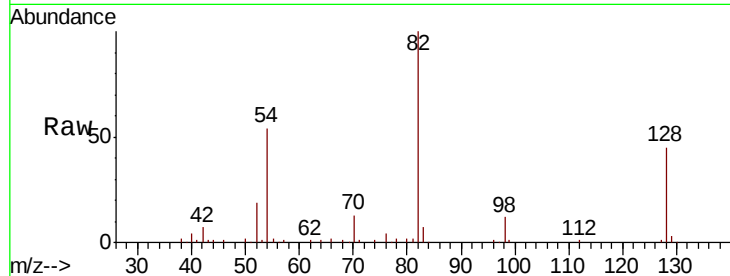


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1


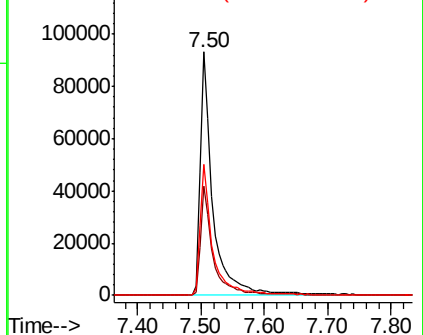



#25
 Isophorone
 Concen: 21.880 ng
 RT: 7.50 min Scan# 921
 Delta R.T. -0.26 min
 Lab File: BF110999.D
 Acq: 27 Nov 2018 10:25

Tgt Ion	82	Resp	127996
Ion Ratio	Lower	Upper	
82	100		
95	0.0	5.7	8.5#
138	0.0	13.2	19.8#



Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 95.00 (94.70 to 95.70): BF1
 Ion 138.00 (137.70 to 138.70): BF1

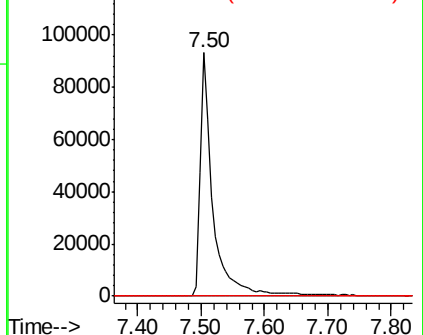


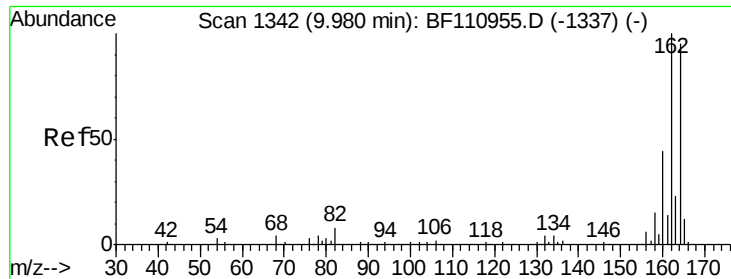




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.98 min Scan# 1342
Delta R.T. -0.00 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Instrument :
BNA_F
ClientSampleId :

Tot Ion:164 Resp: 75419
Ion Ratio Lower Upper
164 100
162 103.1 83.0 124.6
160 46.8 37.0 55.6

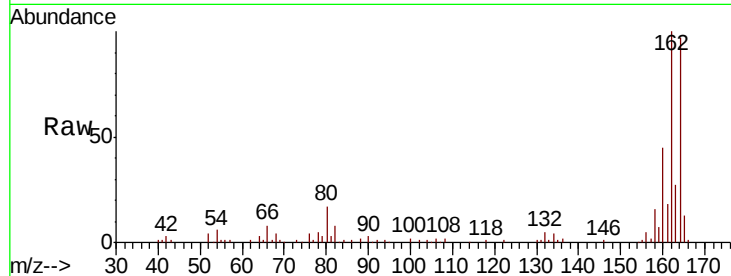


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

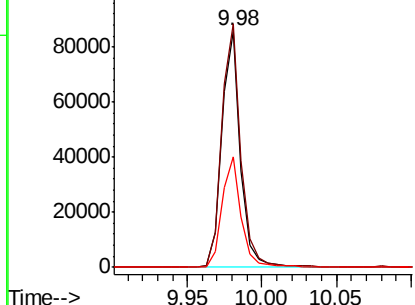
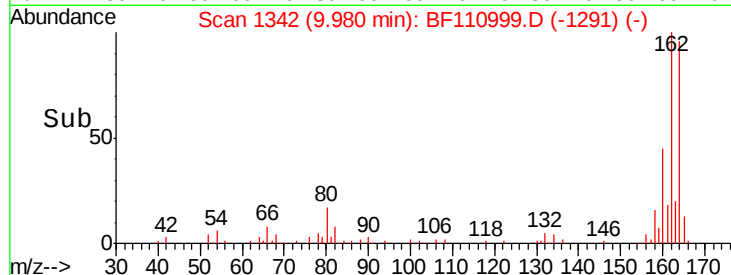



#42
2,4,6-Tribromophenol
Concen: 42.019 ng
RT: 10.78 min Scan# 1478
Delta R.T. -0.00 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Tgt Ion:330 Resp: 31473
Ion Ratio Lower Upper
330 100
332 94.8 77.1 115.7
141 40.4 27.0 40.4#



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

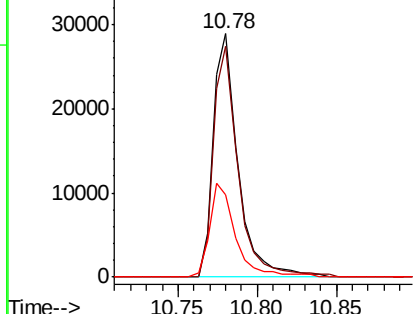


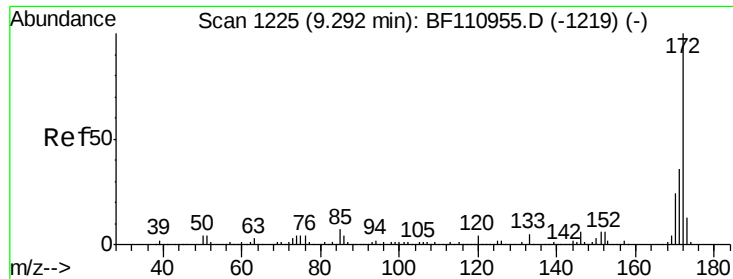




#45
 2-Fluorobiphenyl
 Concen: 38.558 ng
 RT: 9.29 min Scan# 1225
 Delta R.T. -0.00 min
 Lab File: BF110999.D
 Acq: 27 Nov 2018 10:25

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 200724
 Ion Ratio Lower Upper
 172 100
 171 34.8 28.6 43.0
 170 23.1 19.7 29.5

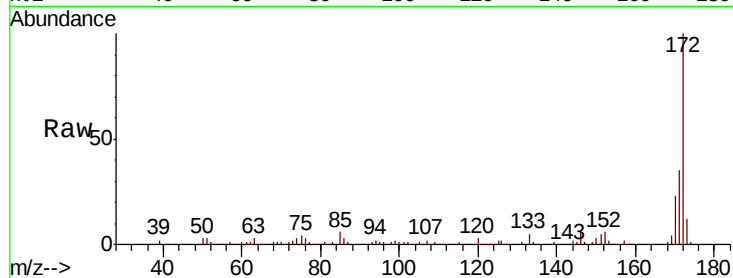


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

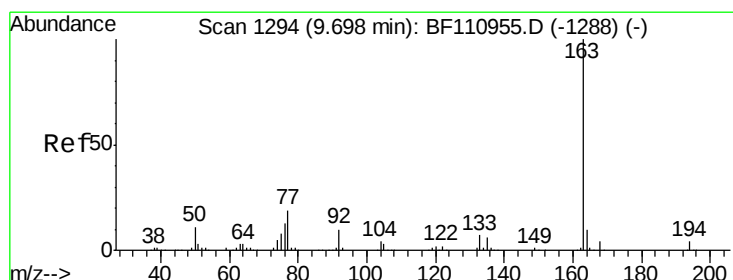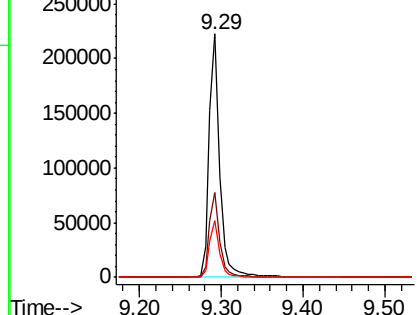
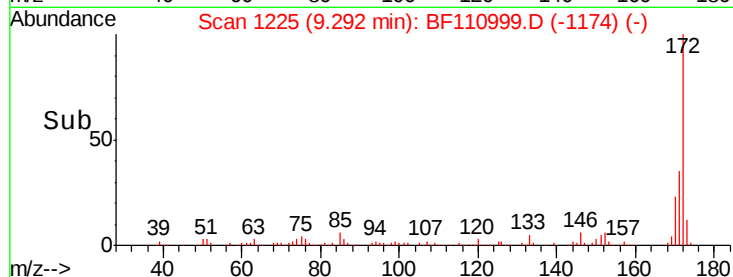



#50
 Dimethylphthalate
 Concen: 4.557 ng
 RT: 9.69 min Scan# 1292
 Delta R.T. -0.01 min
 Lab File: BF110999.D
 Acq: 27 Nov 2018 10:25

Tgt Ion:163 Resp: 25204
 Ion Ratio Lower Upper
 163 100
 194 3.5 3.2 4.8
 164 10.0 8.1 12.1

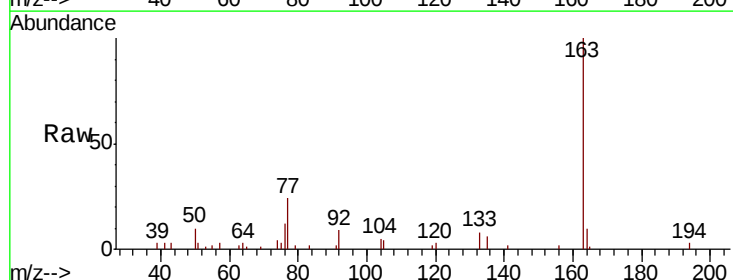

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

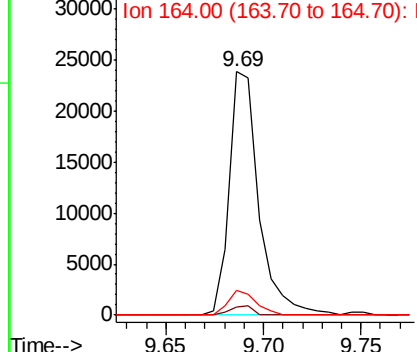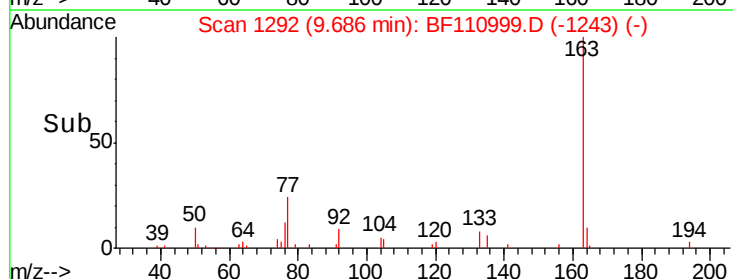


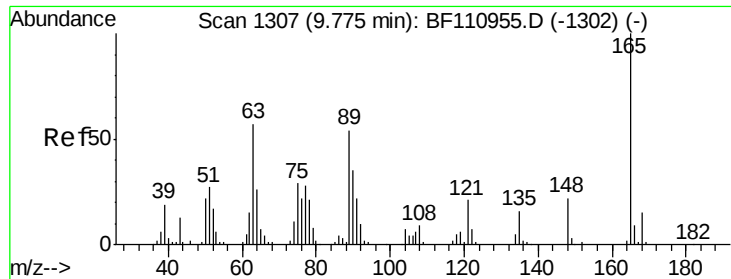




#51
2,6-Dinitrotoluene
Concen: 8.081 ng
RT: 9.98 min Scan# 1342
Delta R.T. 0.21 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Instrument :
BNA_F
ClientSampled :

Tot Ion:165 Resp: 9951
Ion Ratio Lower Upper
165 100
63 0.0 48.9 73.3#
89 0.0 46.6 69.8#

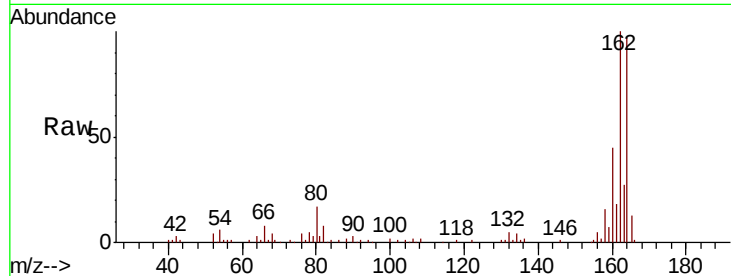


Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1


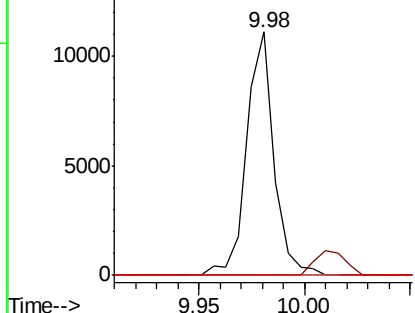



#52
Acenaphthene
Concen: 2.745 ng
RT: 10.01 min Scan# 1347
Delta R.T. -0.01 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Tgt Ion:154 Resp: 12614
Ion Ratio Lower Upper
154 100
153 108.8 90.1 135.1
152 51.8 43.4 65.2



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E

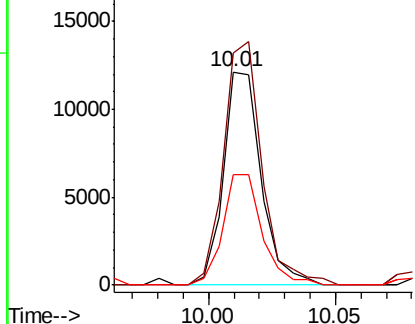


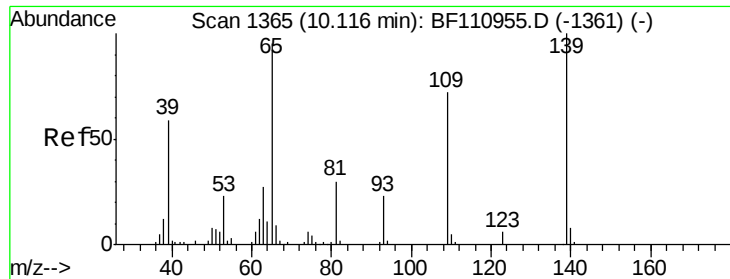




#56
4-Nitrophenol
Concen: 9.631 ng
RT: 10.19 min Scan# 1378
Delta R.T. 0.08 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Instrument :
BNA_F
ClientSampleId :

Tot Ion:139 Resp: 4544
Ion Ratio Lower Upper
139 100
109 0.0 55.8 95.8#
65 0.0 77.9 117.9#

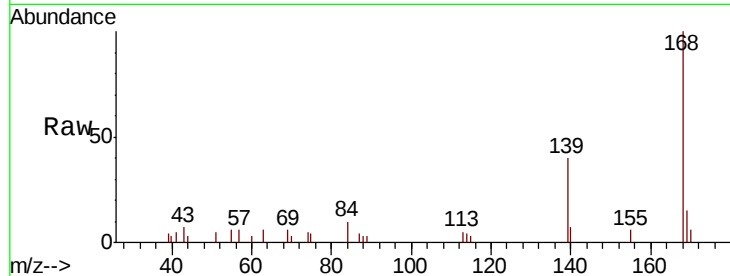


Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BF1


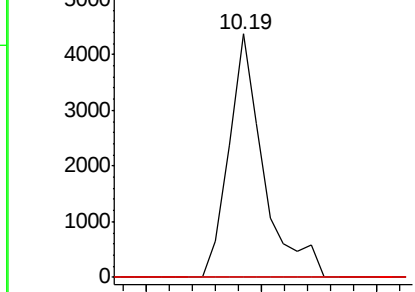



#57
2,4-Dinitrotoluene
Concen: 6.229 ng
RT: 9.98 min Scan# 1342
Delta R.T. -0.21 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Tgt Ion:165 Resp: 9951
Ion Ratio Lower Upper
165 100
63 0.0 44.8 67.2#
89 0.0 62.2 93.4#
182 0.0 2.1 3.1#



Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1
Ion 182.00 (181.70 to 182.70): BF1

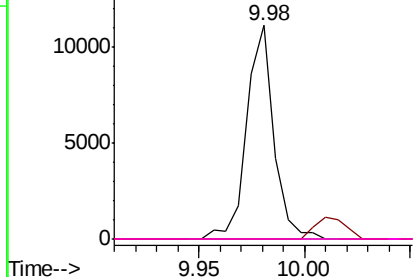

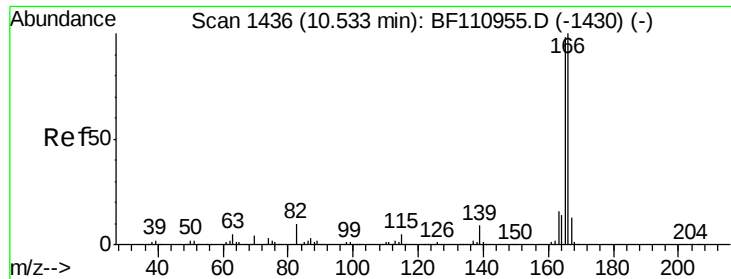

#58

Fluorene

Concen: 4.111 ng

RT: 10.53 min Scan# 1436

Delta R.T. -0.00 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25

Instrument :

BNA_F

ClientSampleId :





Tot Ion:166 Resp: 21445

Ion Ratio Lower Upper

166 100

165 102.1 78.6 117.8

167 13.7 10.8 16.2

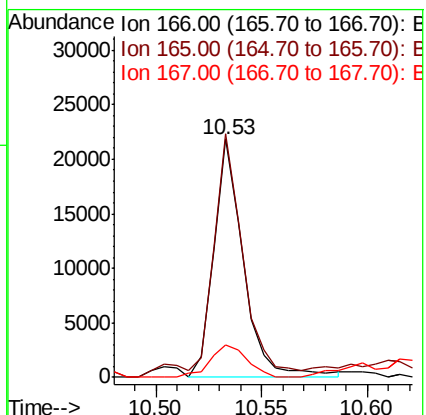

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.47 min Scan# 1596

Delta R.T. -0.00 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25




Tgt Ion:188 Resp: 121838


Ion Ratio Lower Upper

188 100

94 9.1 7.2 10.8

80 9.7 7.9 11.9

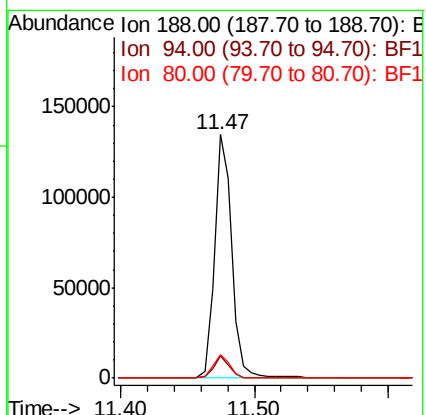


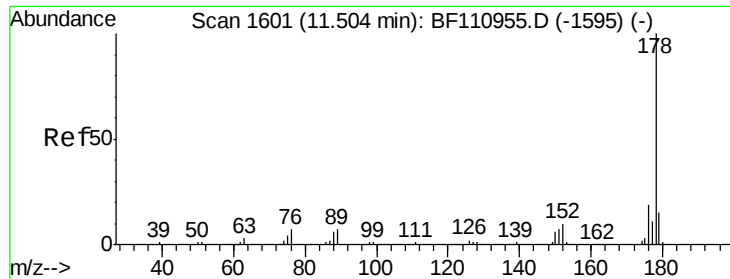




#71
Phenanthrene
Concen: 18.711 ng
RT: 11.50 min Scan# 1600
Delta R.T. -0.01 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Instrument :
BNA_F
ClientSampleId :

Tot Ion:178 Resp: 120743
Ion Ratio Lower Upper
178 100
176 18.5 15.5 23.3
179 15.5 12.5 18.7




Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

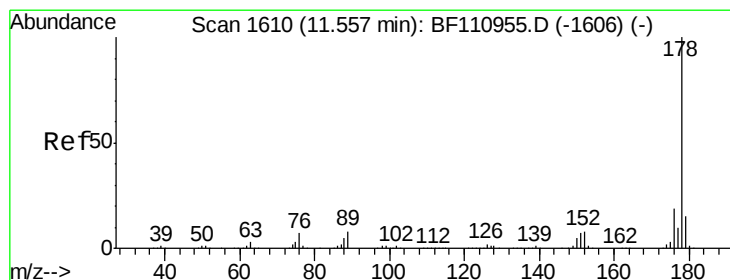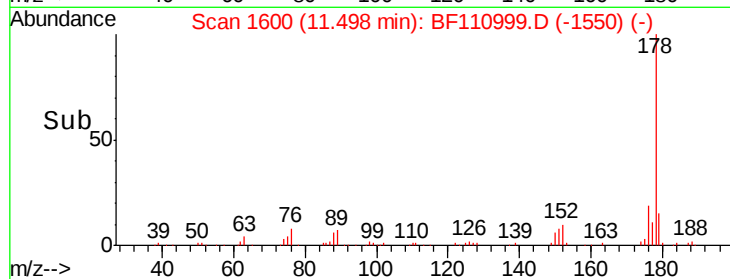
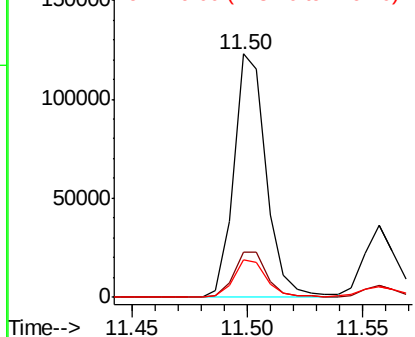



#72
Anthracene
Concen: 5.351 ng
RT: 11.56 min Scan# 1610
Delta R.T. -0.00 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Tgt Ion:178 Resp: 35164
Ion Ratio Lower Upper
178 100
176 17.2 15.4 23.2
179 15.2 12.6 18.8

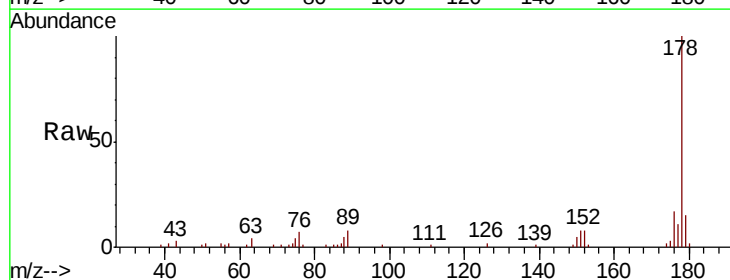

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

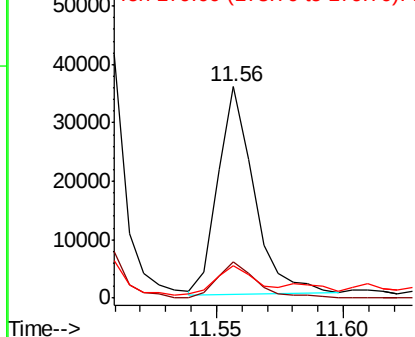

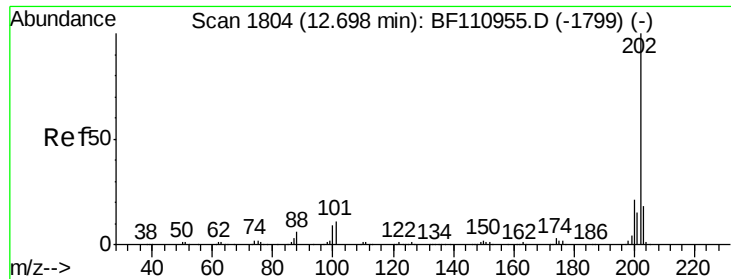

#75

Fluoranthene

Concen: 22.911 ng

RT: 12.70 min Scan# 1804

Delta R.T. -0.00 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25

Instrument :

BNA_F

ClientSampleId :


Tot Ion:202 Resp: 151951

Ion Ratio Lower Upper

202 100

101 10.3 0.0 31.4




203 17.8 0.0 37.7



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

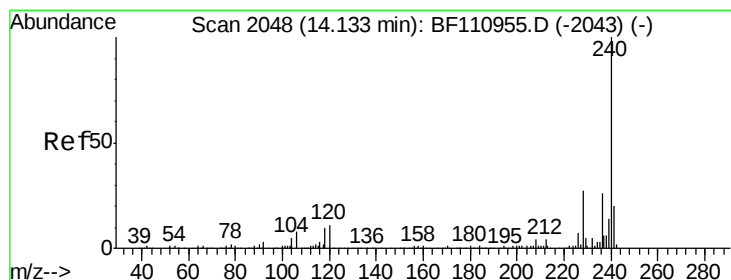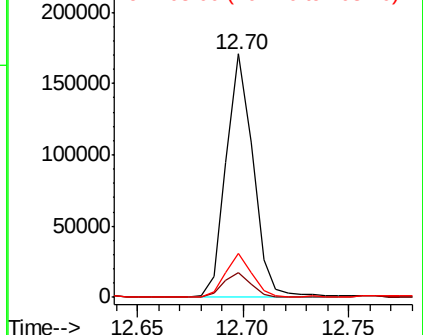

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.13 min Scan# 2048

Delta R.T. -0.00 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25


Tgt Ion:240 Resp: 131552

Ion Ratio Lower Upper

240 100

120 10.8 8.3 12.5



236 25.0 21.2 31.8

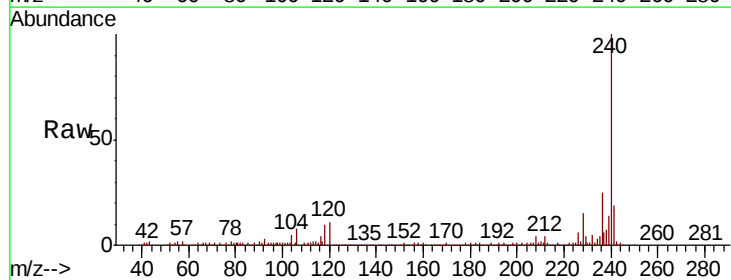


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



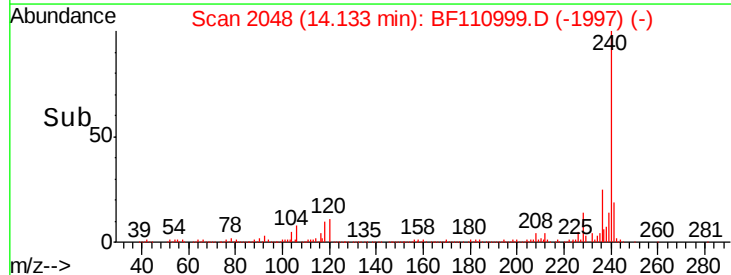
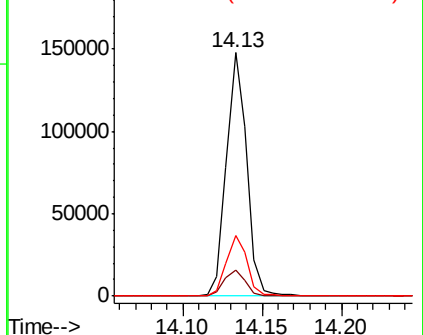


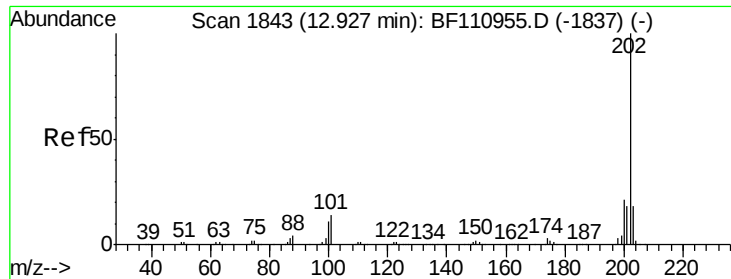

#78
Pvrene
Concen: 17.176 ng
RT: 12.93 min Scan# 1844
Delta R.T. -0.00 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25




Instrument :
BNA_F
ClientSampleId :


Tot Ion:202 Resp: 165035
Ion Ratio Lower Upper
202 100
200 20.1 17.8 26.6
203 17.4 14.2 21.4

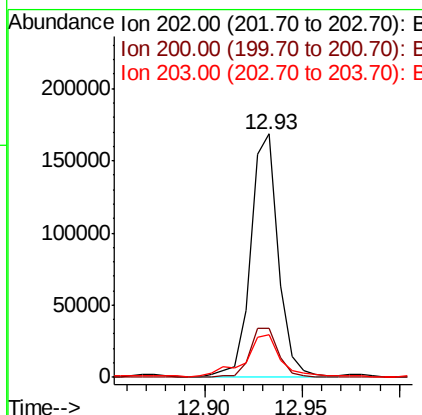

#79
Terphenyl-d14
Concen: 24.510 ng
RT: 13.06 min Scan# 1865
Delta R.T. -0.00 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Tgt Ion:244 Resp: 165636
Ion Ratio Lower Upper
244 100
212 7.0 5.8 8.8
122 10.4 8.7 13.1

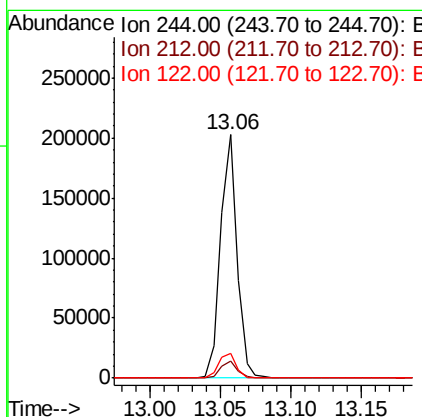



#81

Benzo(a)anthracene

Concen: 10.222 ng

RT: 14.12 min Scan# 2046

Delta R.T. -0.00 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25

Instrument :

BNA_F

ClientSampleId :


Tot Ion:228 Resp: 79392

Ion Ratio Lower Upper

228 100

226 27.7 22.1 33.1




229 21.8 15.6 23.4



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

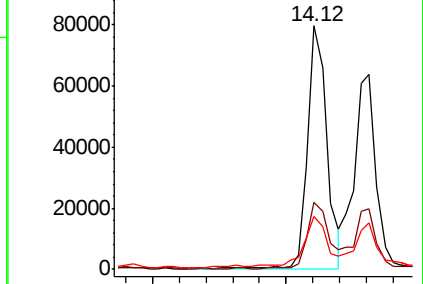

#83

Chrysene

Concen: 10.384 ng

RT: 14.12 min Scan# 2046

Delta R.T. -0.04 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25


Tgt Ion:228 Resp: 79392

Ion Ratio Lower Upper

228 100

226 27.7 24.7 37.1



229 21.8 15.9 23.9




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

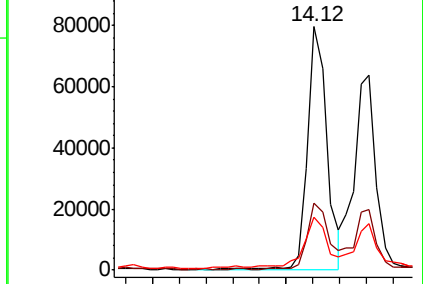


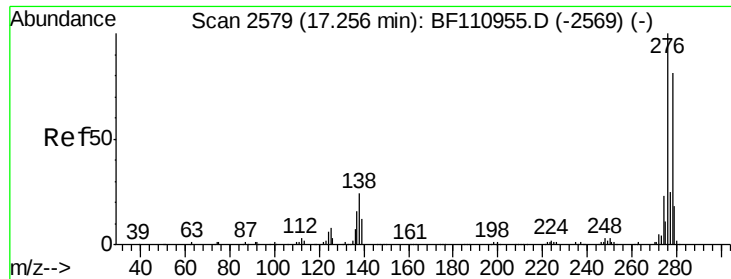




#86
 Indeno(1,2,3-cd)pyrene
 Concen: 4.260 ng
 RT: 17.27 min Scan# 2582
 Delta R.T. 0.02 min
 Lab File: BF110999.D
 Acq: 27 Nov 2018 10:25

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
138	25.5	18.5	27.7
277	28.2	20.0	30.0




Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

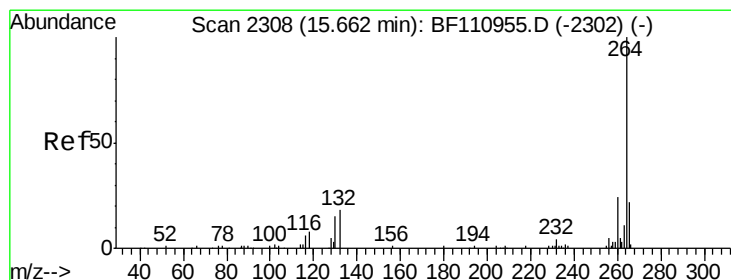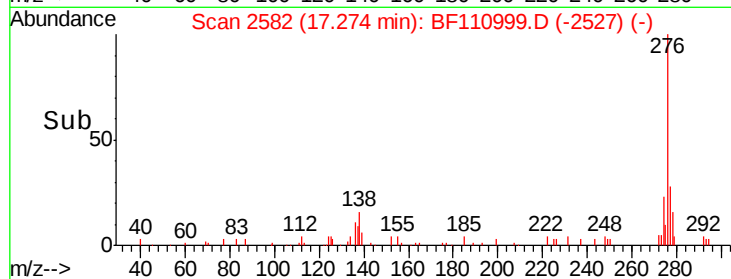
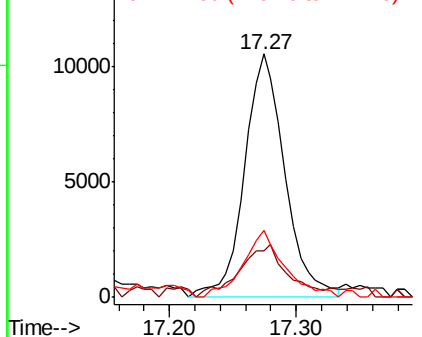



#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.67 min Scan# 2310
 Delta R.T. 0.01 min
 Lab File: BF110999.D
 Acq: 27 Nov 2018 10:25

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.6	18.7	28.1
265	21.8	16.7	25.1

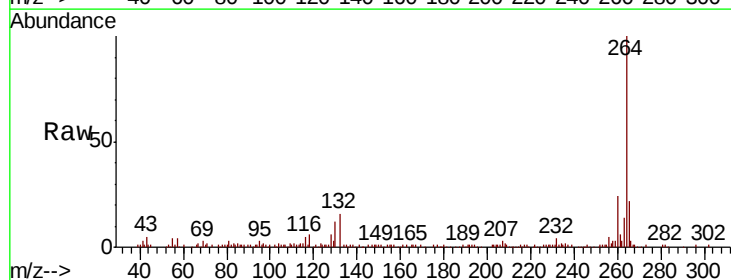

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E




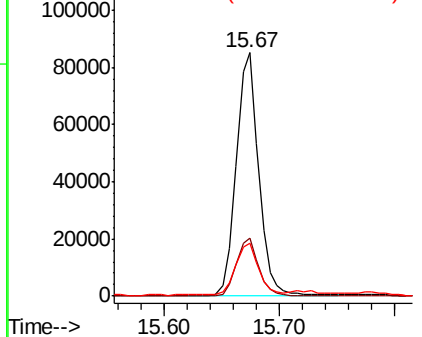




#88
Benzo(b)fluoranthene
Concen: 13.279 ng
RT: 15.22 min Scan# 2232
Delta R.T. 0.01 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25




Instrument :
BNA_F
ClientSampled :


Tot Ion:252 Resp: 90021
Ion Ratio Lower Upper
252 100
253 23.9 17.2 25.8
125 13.6 8.2 12.4#

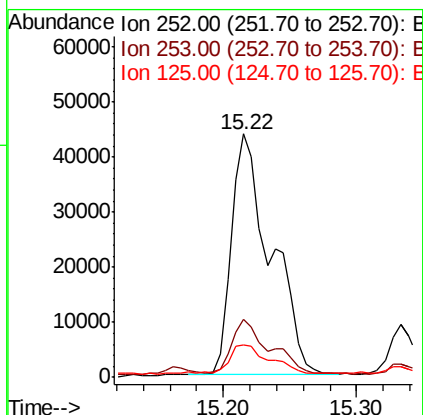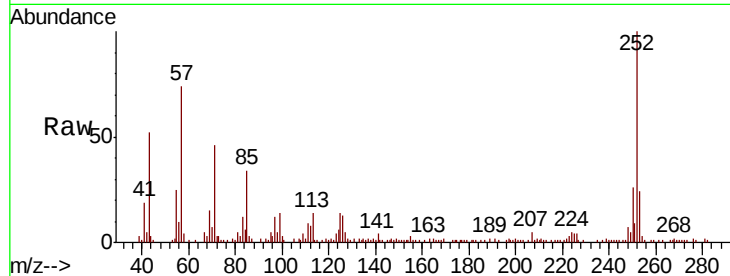

#89
Benzo(k)fluoranthene
Concen: 12.902 ng
RT: 15.22 min Scan# 2232
Delta R.T. -0.02 min
Lab File: BF110999.D
Acq: 27 Nov 2018 10:25

Tgt Ion:252 Resp: 90021
Ion Ratio Lower Upper
252 100
253 23.9 17.2 25.8
125 13.6 7.4 11.0#

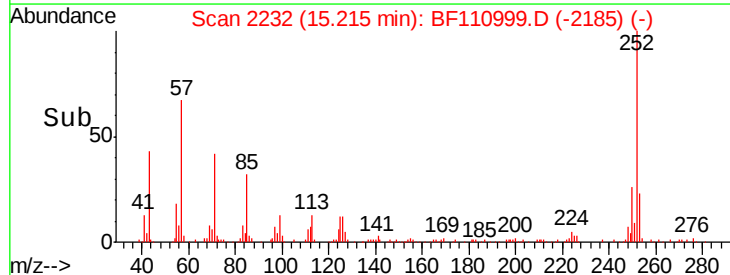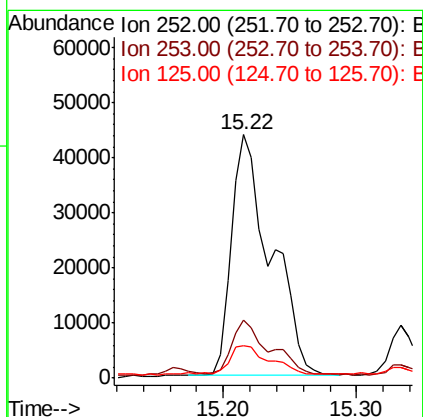



#90

Benzo(a)pyrene

Concen: 8.374 ng

RT: 15.61 min Scan# 2299

Delta R.T. 0.01 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25

Instrument :

BNA_F

ClientSampled :


Tot Ion:252 Resp: 52839

Ion Ratio Lower Upper

252 100

253 23.8 18.2 27.4




125 14.1 9.0 13.6#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

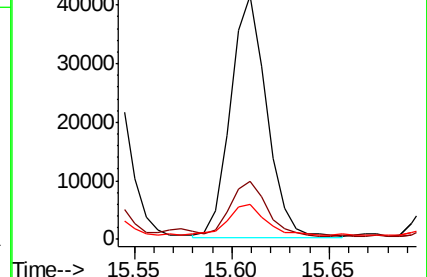

#92

Benzo(g,h,i)perylene

Concen: 4.622 ng

RT: 17.76 min Scan# 2665

Delta R.T. 0.02 min

Lab File: BF110999.D

Acq: 27 Nov 2018 10:25


Tgt Ion:276 Resp: 23201

Ion Ratio Lower Upper

276 100

277 25.6 18.8 28.2

138 21.4 16.0 24.0



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

