

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112718\
 Data File : BF111023.D
 Acq On : 27 Nov 2018 22:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 28 01:00:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 27 15:32:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-6.93
21) Naphthalene-d8	0.00	136	0	0.00	ng	-8.22
39) Acenaphthene-d10	0.00	164	0	0.00	ng	-9.98
64) Phenanthrene-d10	0.00	188	0	0.00	ng	-11.47
76) Chrysene-d12	0.00	240	0	0.00	ng	-14.13
87) Perylene-d12	0.00	264	0	0.00	ng	-15.67
System Monitoring Compounds						
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	0.00	82	0	0.00	ng	
42) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
45) 2-Fluorobiphenyl	0.00	172	0	0.00	ng	
79) Terphenyl-d14	0.00	244	0	0.00	ng	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112718\
Data File : BF111023.D
Acq On : 27 Nov 2018 22:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 28 01:00:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 27 15:32:10 2018
Response via : Initial Calibration

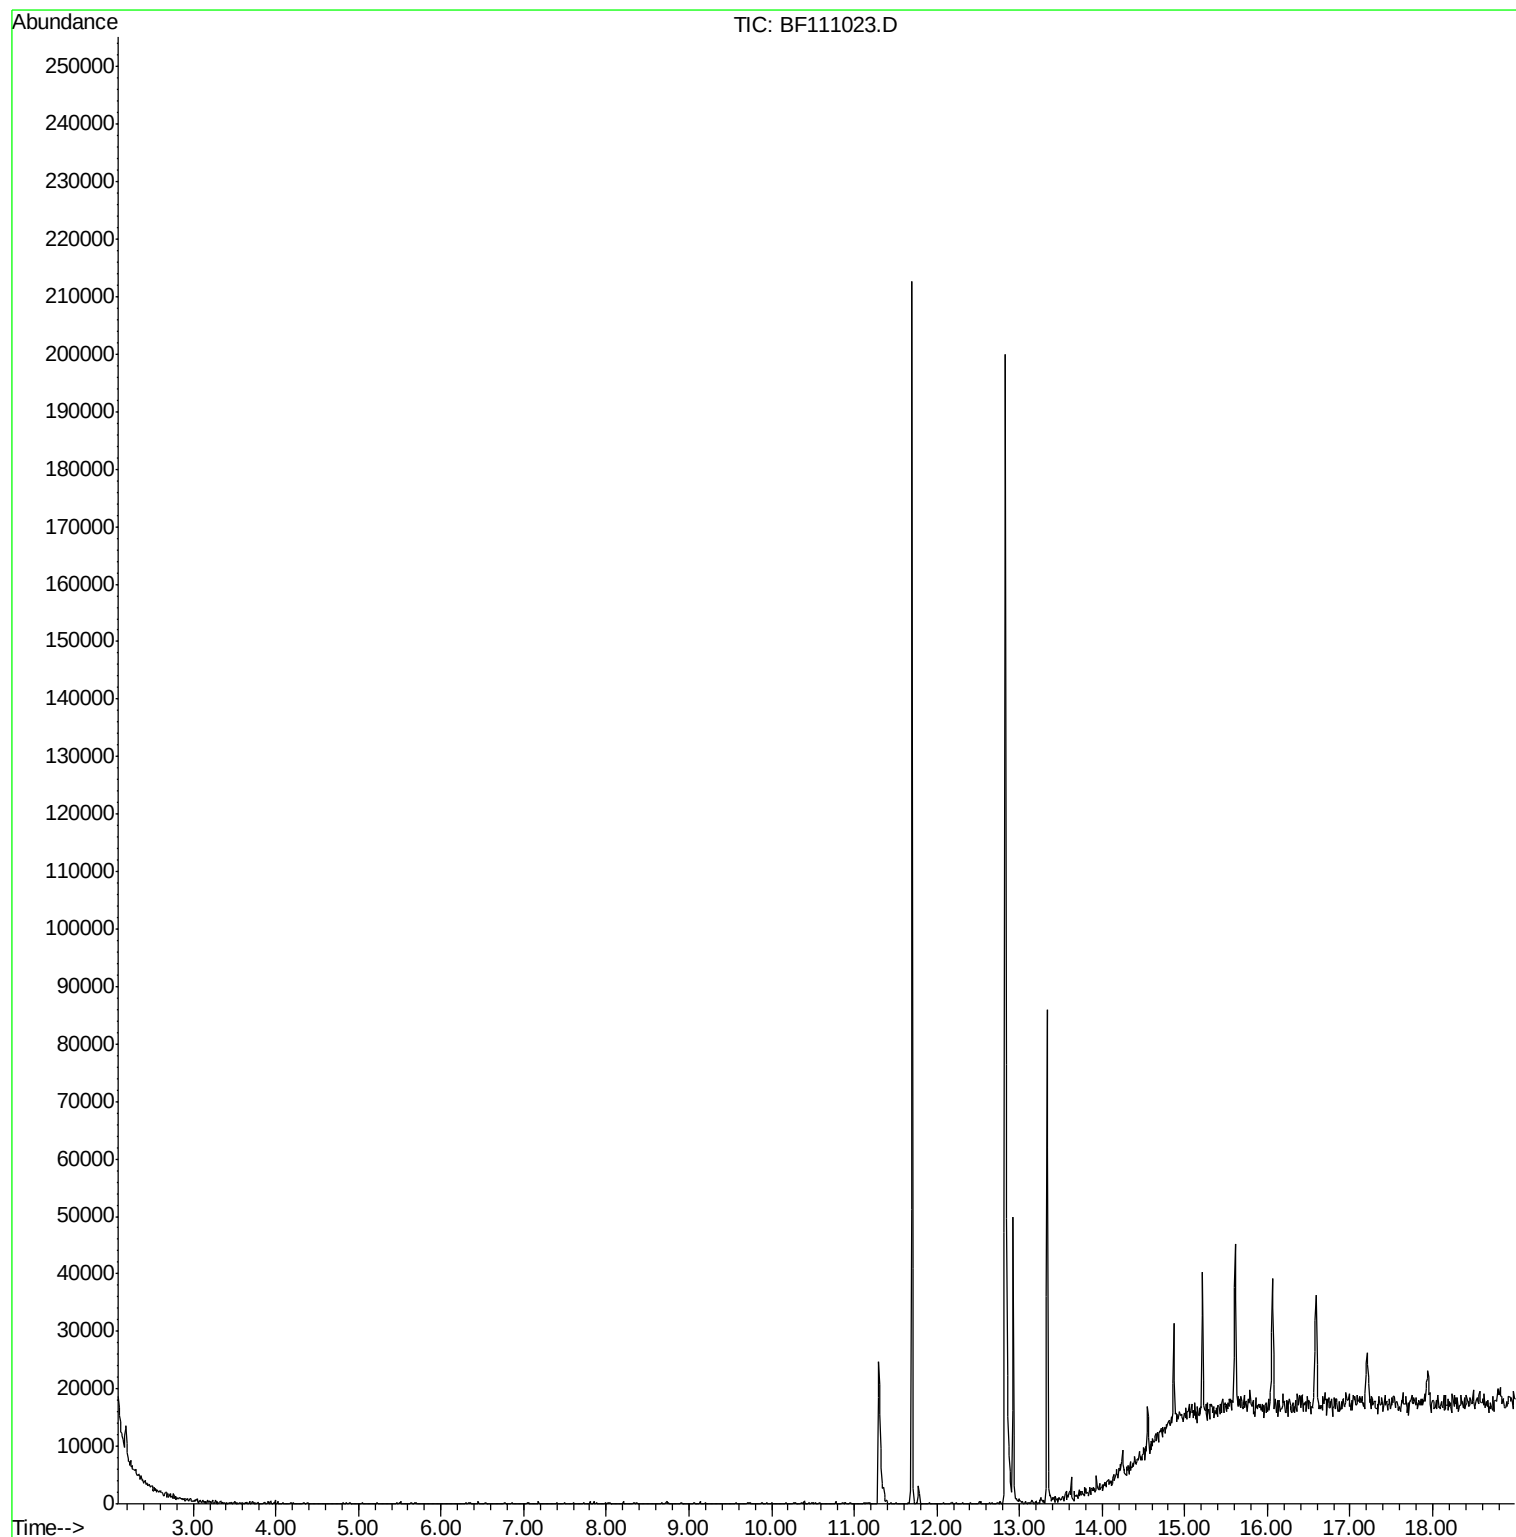

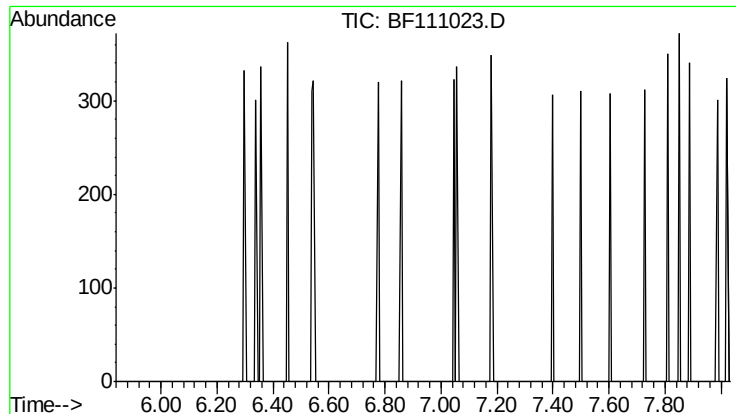

#1

1,4-Dichlorobenzene-d4

Concen: 0.000 ng

Expected RT: 6.93 min

Lab File: BF111023.D

Acq: 27 Nov 2018 22:23

Instrument :

BNA_F

ClientSampleId :

DFTPP



Tgt Ion: 152

Sig Exp Ratio

152 100

150 153.4

115 61.4

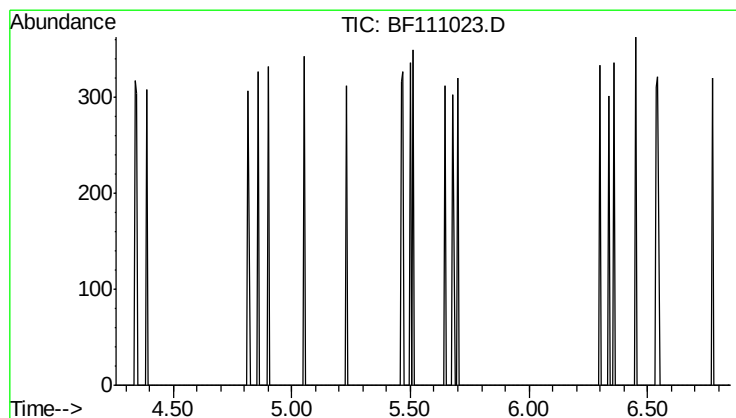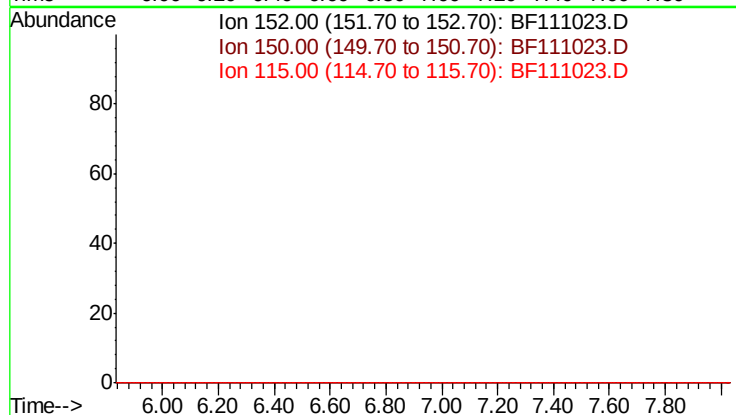

#5

2-Fluorophenol

Concen: 0.000 ng

Expected RT: 5.55 min

Lab File: BF111023.D

Acq: 27 Nov 2018 22:23


Tgt Ion: 112


Sig Exp Ratio

112 100

64 55.1

63 29.6

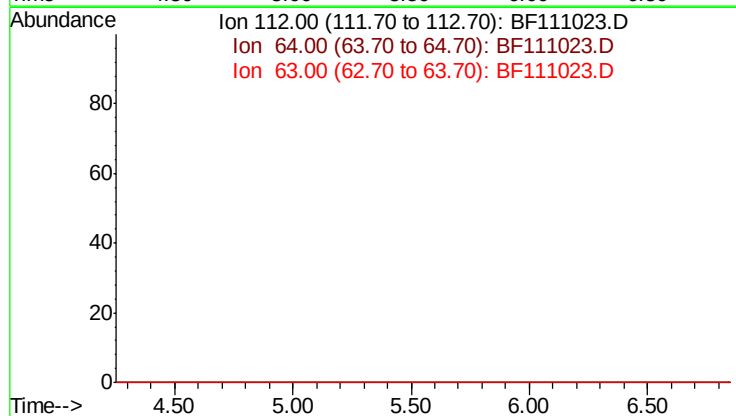

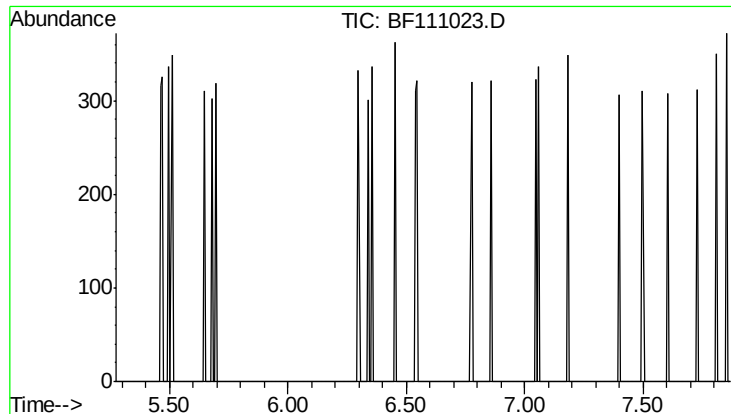

#7

Phenol-d6

Concen: 0.000 ng

Expected RT: 6.57 min

Lab File: BF111023.D

Acq: 27 Nov 2018 22:23

Instrument :

BNA_F

ClientSampleId :

DFTPP



Tgt Ion: 99

Sig Exp Ratio

99 100

42 19.7

71 35.0

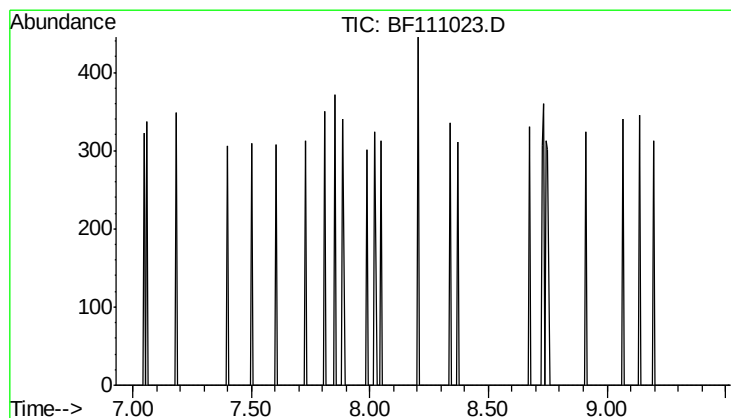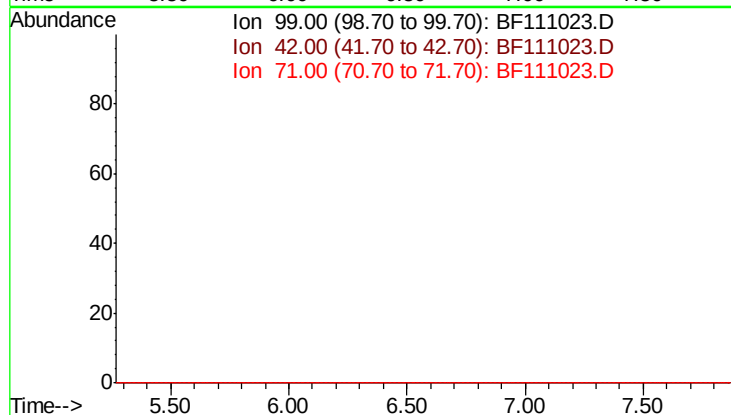

#21

Naphthalene-d8

Concen: 0.000 ng

Expected RT: 8.22 min

Lab File: BF111023.D

Acq: 27 Nov 2018 22:23

Tgt Ion: 136


Sig Exp Ratio


136 100

137 11.0

54 6.8

68 5.2


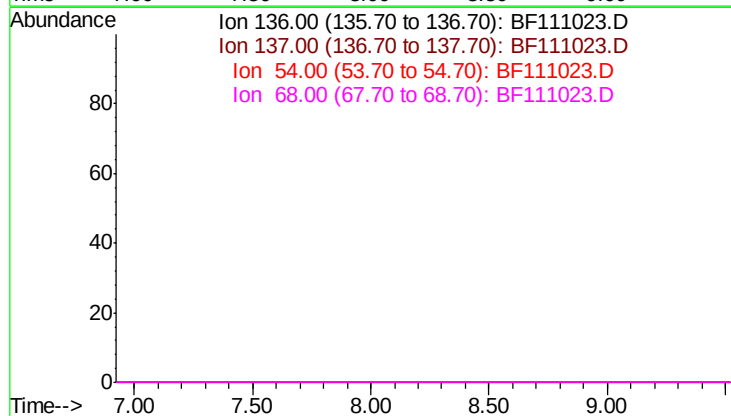


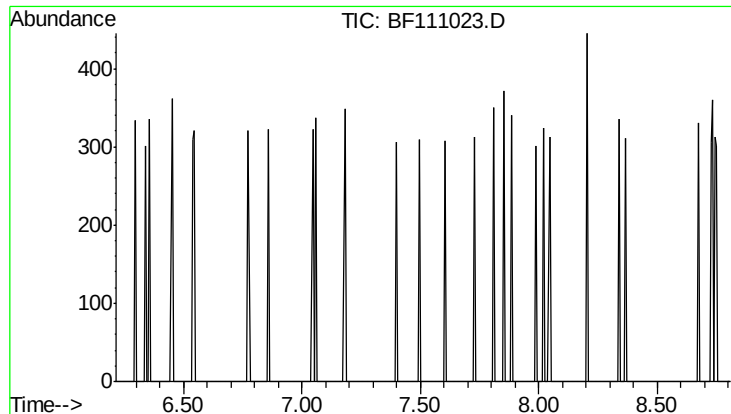

#23
Nitrobenzene-d5
Concen: 0.000 ng
Expected RT: 7.51 min
Lab File: BF111023.D
Acq: 27 Nov 2018 22:23


Instrument :
BNA_F
ClientSampleId :
DFTPP


Tgt Ion:	82
Sig	Exp Ratio
82	100
128	42.7
54	48.3

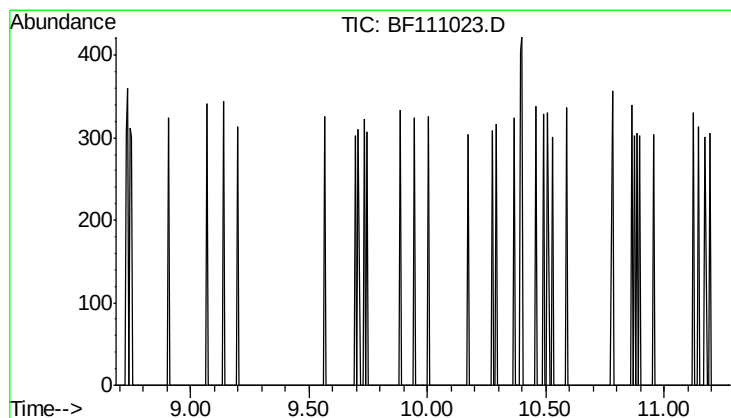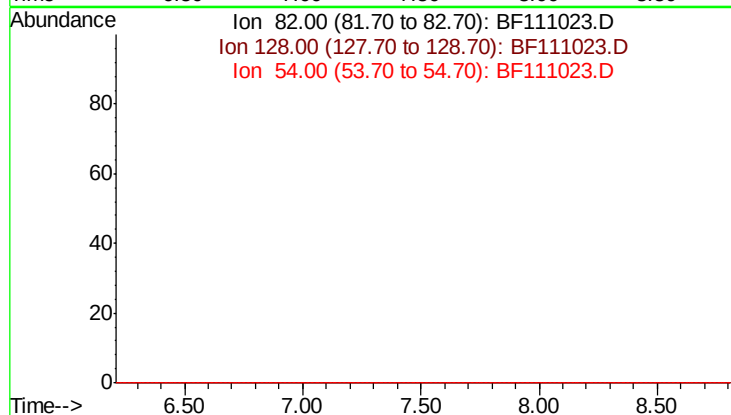

#39
Acenaphthene-d10
Concen: 0.000 ng
Expected RT: 9.98 min
Lab File: BF111023.D
Acq: 27 Nov 2018 22:23

Tgt Ion:	164
Sig	Exp Ratio
164	100
162	103.8
160	46.3


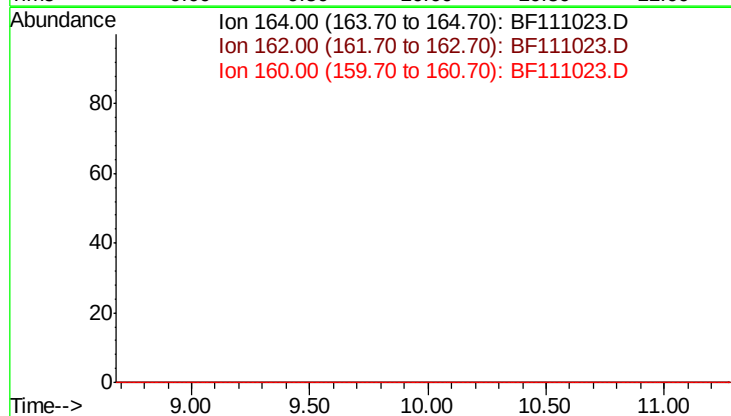


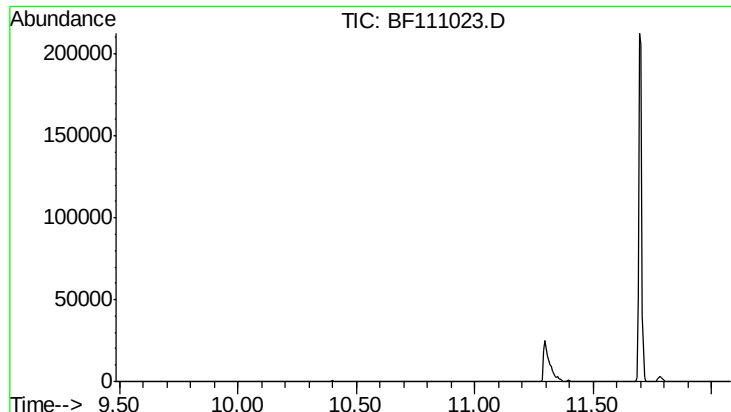

#42
 2,4,6-Tribromophenol
 Concen: 0.000 ng
 Expected RT: 10.78 min
 Lab File: BF111023.D
 Acq: 27 Nov 2018 22:23


Instrument :
 BNA_F
 ClientSampleId :
 DFTPP


Tgt Ion: 330
 Sig Exp Ratio
 330 100
 332 96.4
 141 33.7

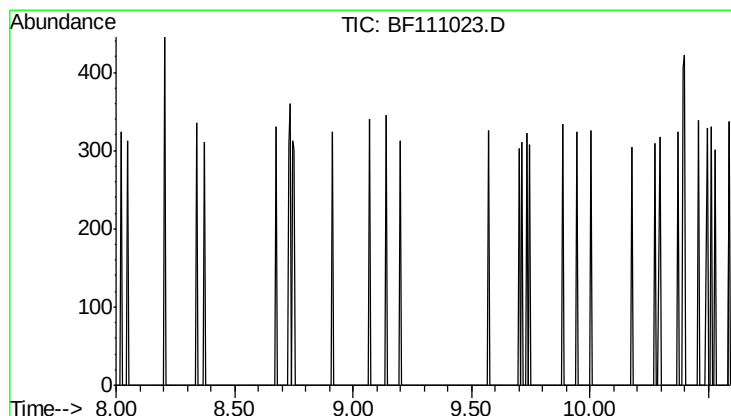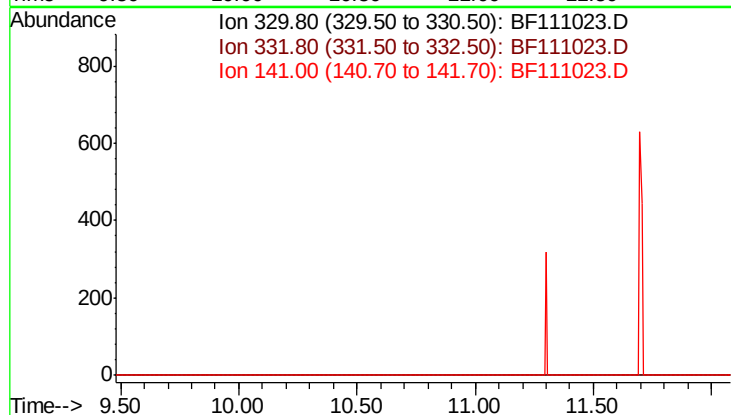

#45
 2-Fluorobiphenyl
 Concen: 0.000 ng
 Expected RT: 9.29 min
 Lab File: BF111023.D
 Acq: 27 Nov 2018 22:23

Tgt Ion: 172
 Sig Exp Ratio
 172 100
 171 35.8
 170 24.6

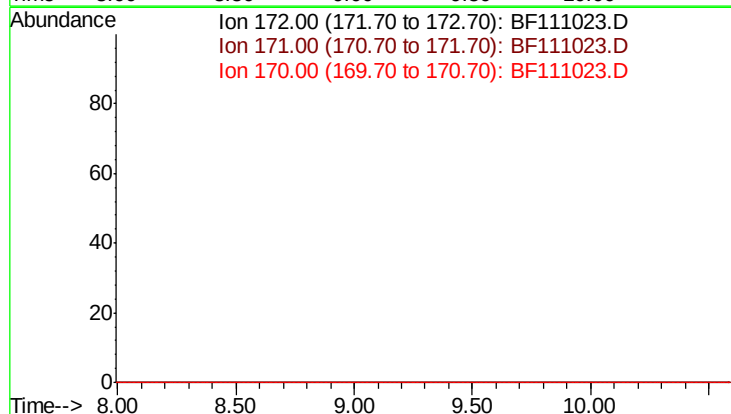


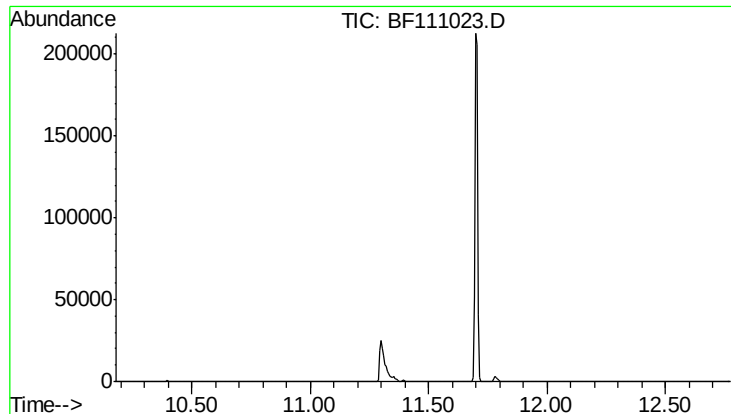


#64
 Phenanthrene-d10
 Concen: 0.000 ng
 Expected RT: 11.47 min
 Lab File: BF111023.D
 Acq: 27 Nov 2018 22:23

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Tgt Ion: 188


Sig	Exp Ratio
188	100
94	9.0
80	9.9

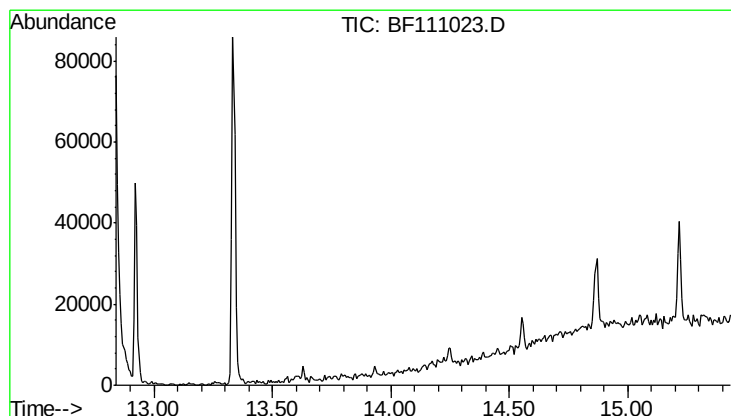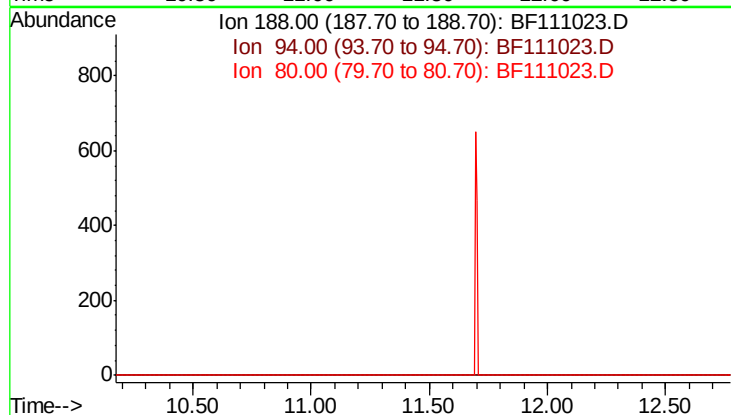


#76
 Chrysene-d12
 Concen: 0.000 ng
 Expected RT: 14.13 min
 Lab File: BF111023.D
 Acq: 27 Nov 2018 22:23

Tgt Ion: 240

Sig	Exp Ratio
240	100
120	10.4
236	26.5


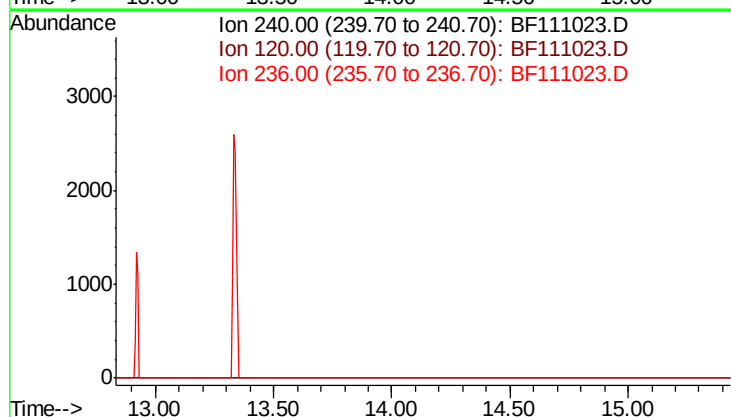


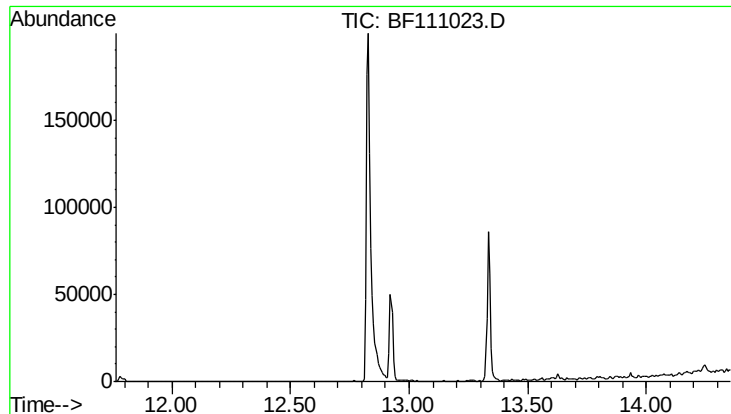

#79
 Terphenyl-d14
 Concen: 0.000 ng
 Expected RT: 13.06 min
 Lab File: BF111023.D
 Acq: 27 Nov 2018 22:23

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Tgt Ion	Exp Ratio
244	100
212	7.3
122	10.9

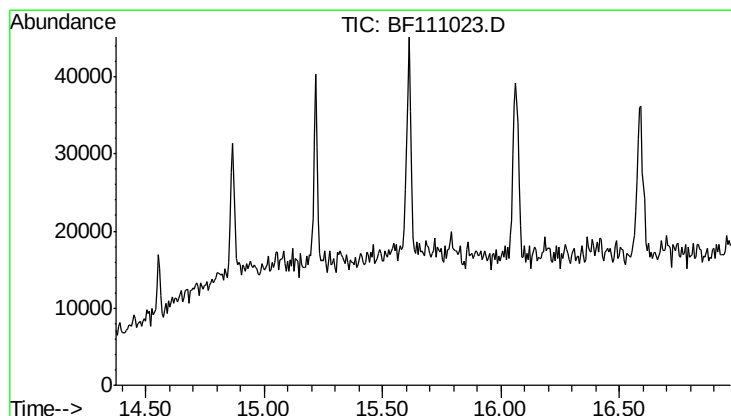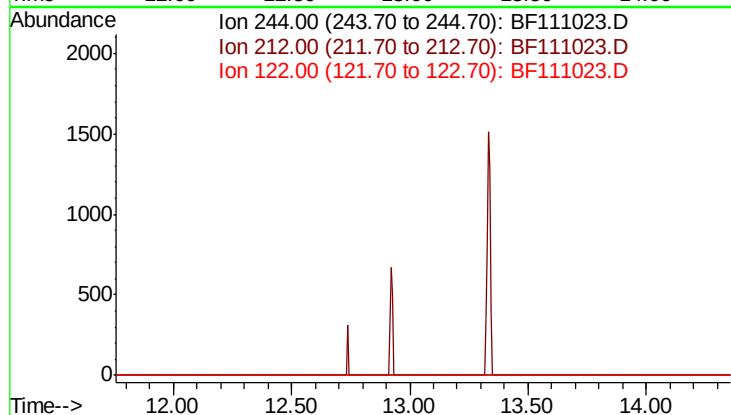

#87
 Perylene-d12
 Concen: 0.000 ng
 Expected RT: 15.67 min
 Lab File: BF111023.D
 Acq: 27 Nov 2018 22:23

Tgt Ion	Exp Ratio
264	100
260	23.4
265	20.9

