
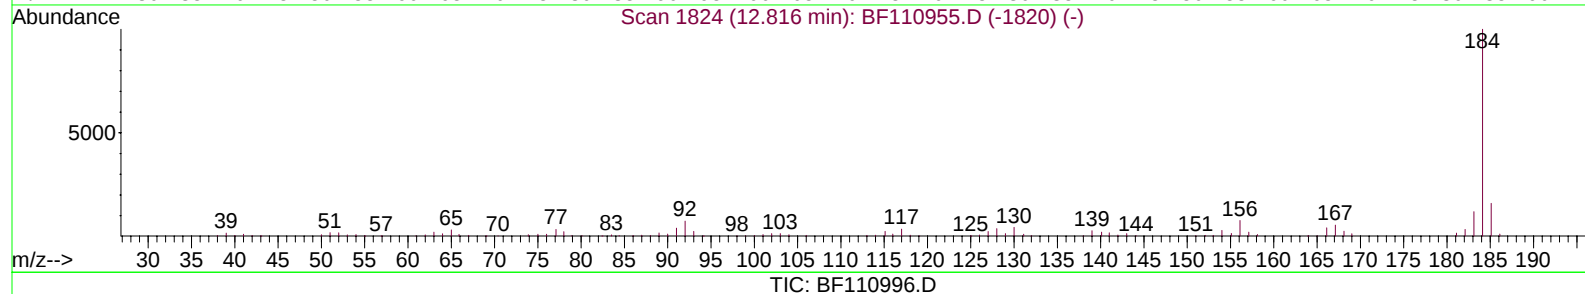
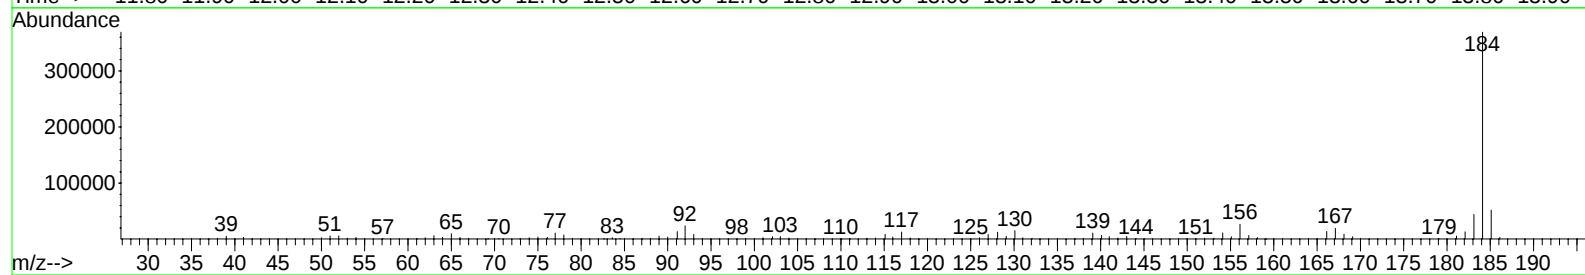


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112718\
Data File : BF110996.D
Acq On : 27 Nov 2018 9:01
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 10:06:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 27 06:43:50 2018
Response via : Initial Calibration

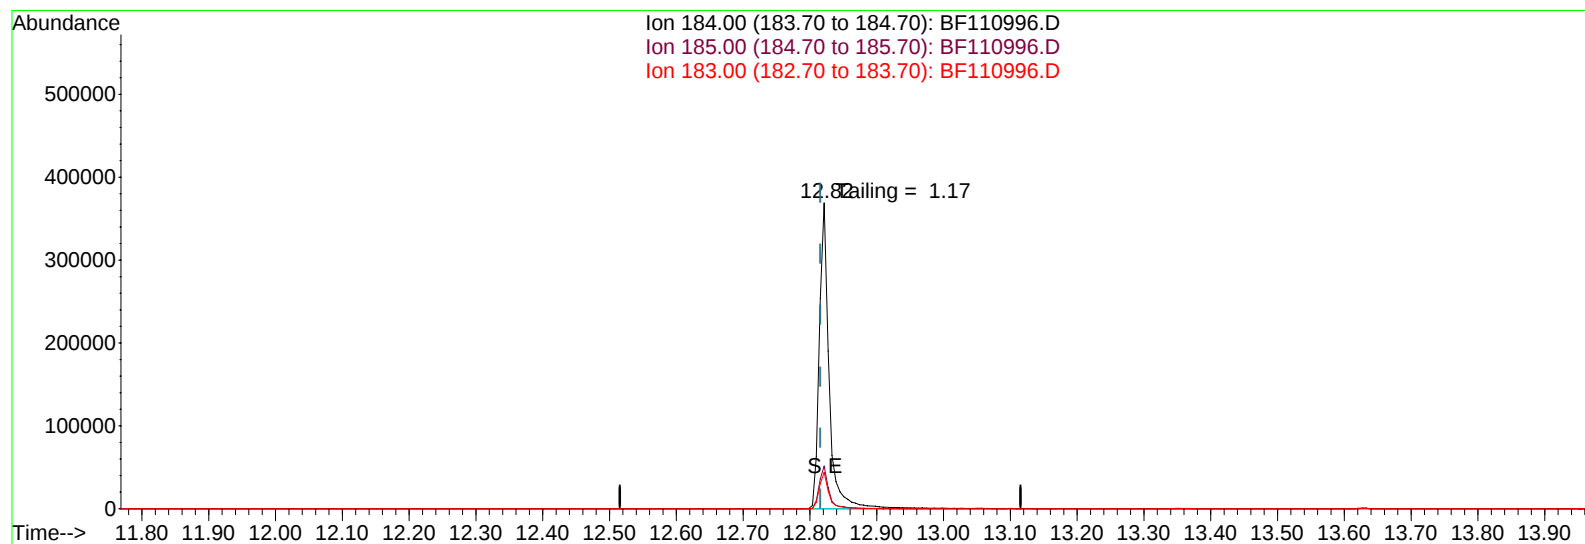

(77) Benzidine




12.821min (+0.006) 0.00ng

response 378413

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	13.99
183.00	11.80	11.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112718\
Data File : BF110996.D
Acq On : 27 Nov 2018 9:01
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 10:06:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 27 06:43:50 2018
Response via : Initial Calibration

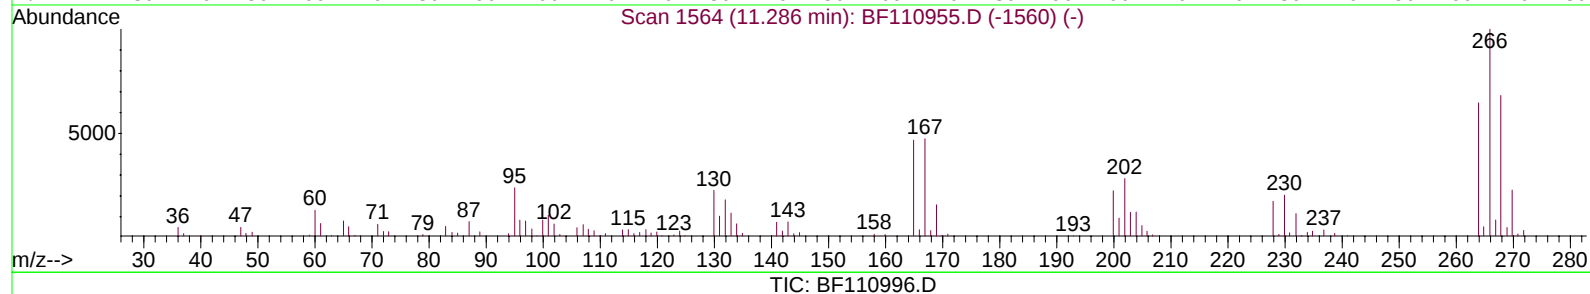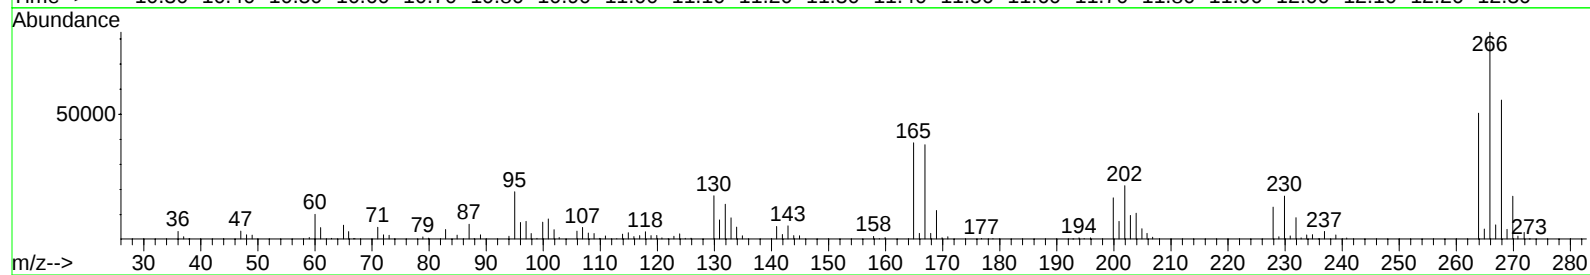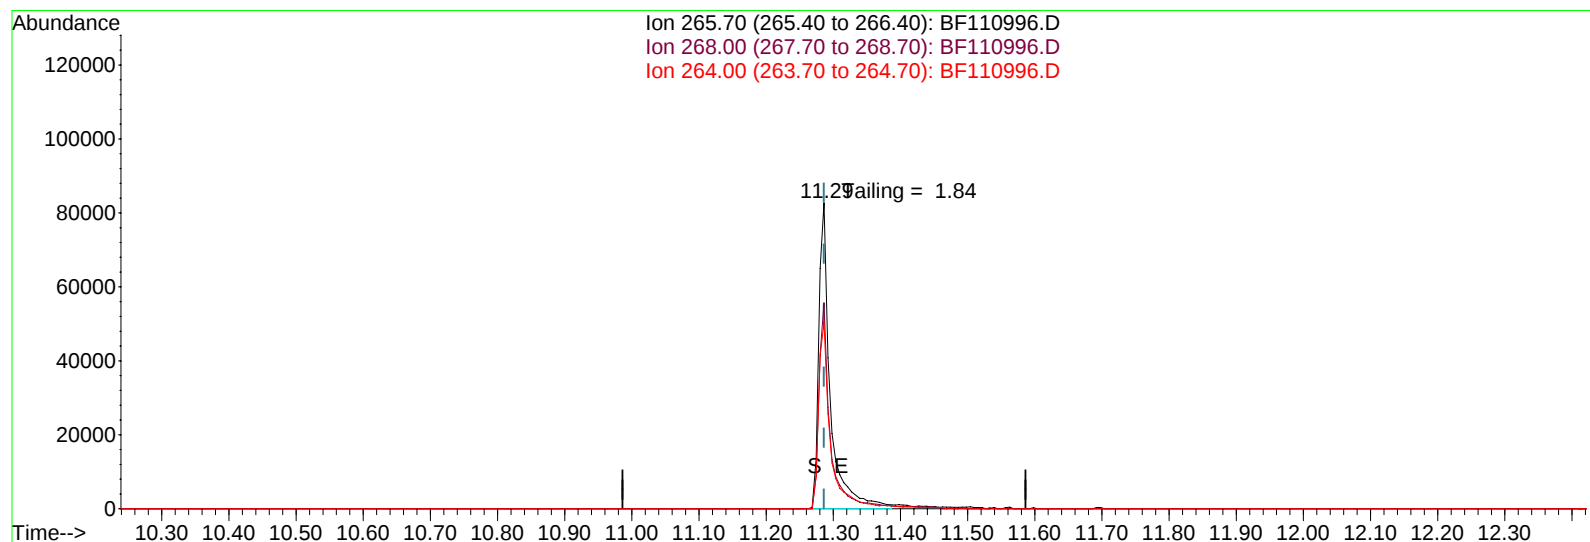

(70) Pentachlorophenol (C)

11.286min (-0.000) 154231.32ng

response 101788

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	67.33
264.00	63.20	60.99
0.00	0.00	0.00