

Data File : BF111023.D

Acq On : 27 Nov 2018 22:23

Operator : JU/SJ

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Nov 28 07:53:34 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Nov 27 15:32:10 2018

Response via : Initial Calibration

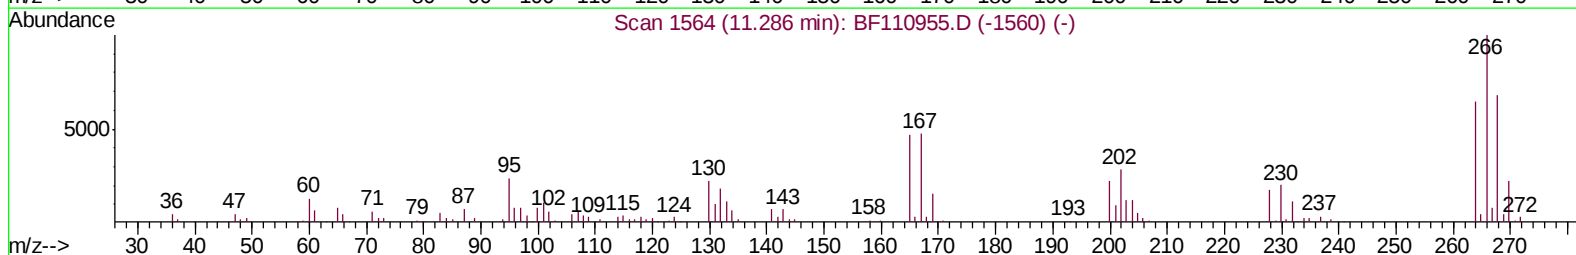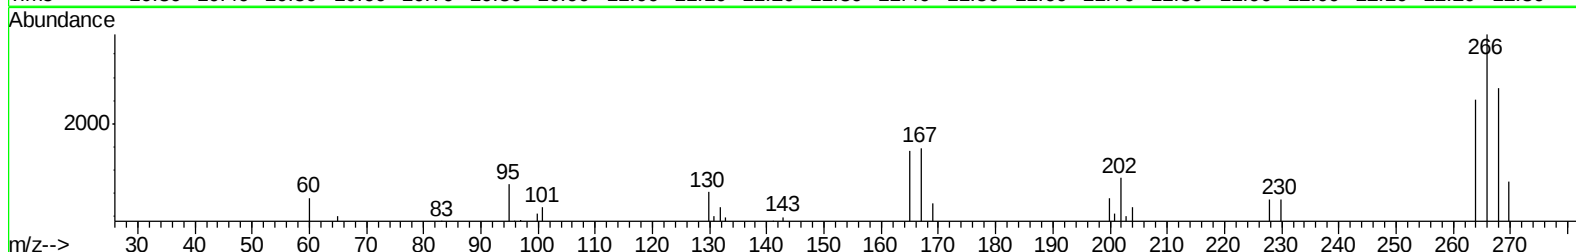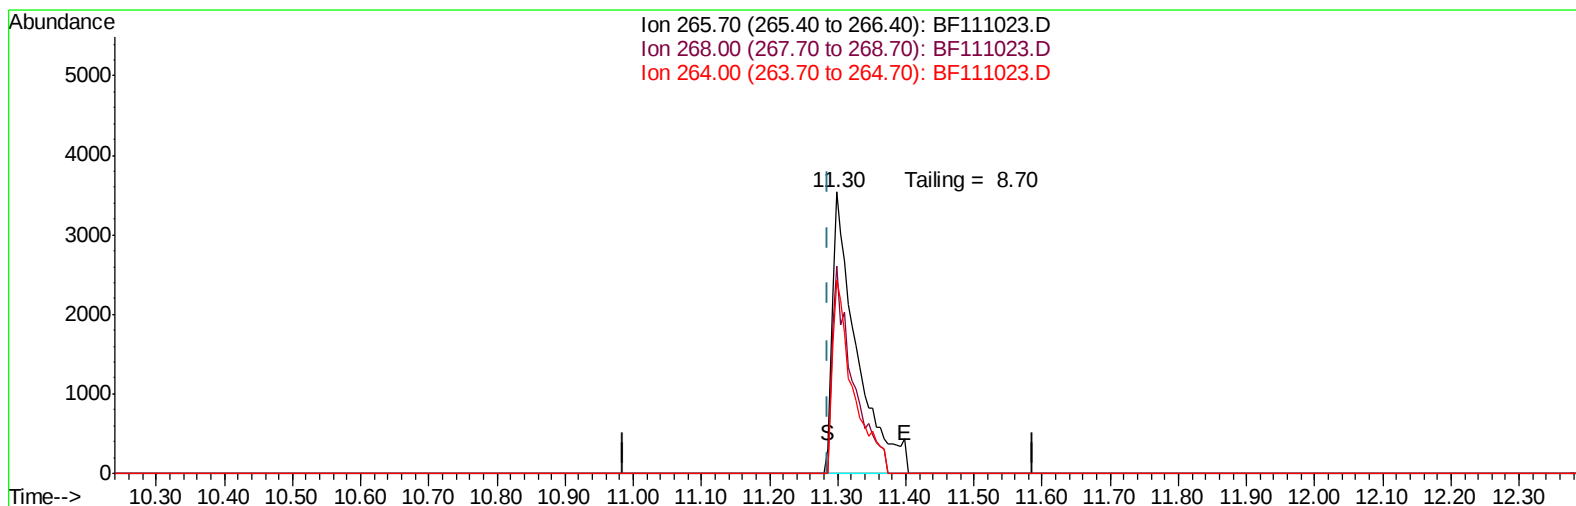

TIC: BF111023.D

(70) Pentachlorophenol (C)




11.298min (+0.012) 0.00ng

response 8480

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	73.54
264.00	63.20	68.48
0.00	0.00	0.00

Data File : BF111023.D
Acq On : 27 Nov 2018 22:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 07:53:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 27 15:32:10 2018
Response via : Initial Calibration

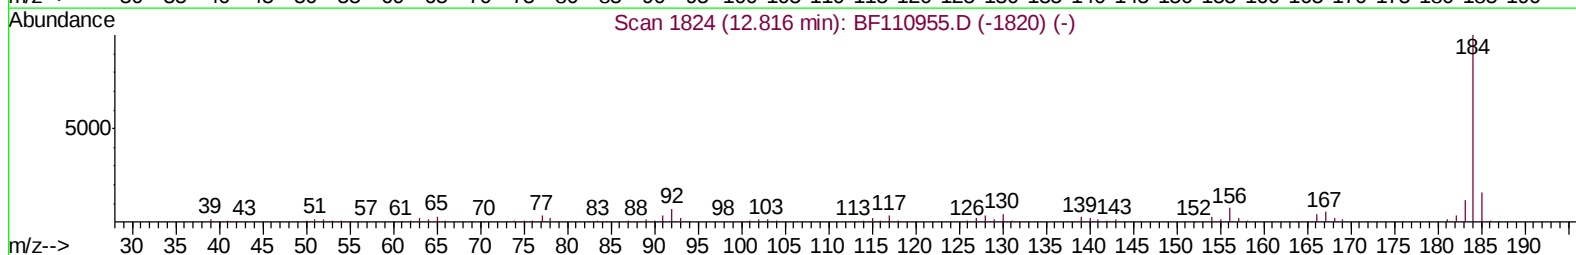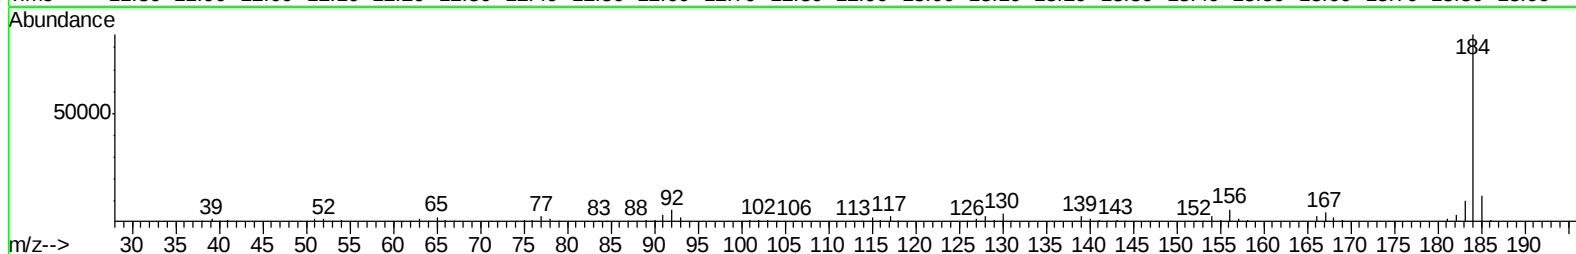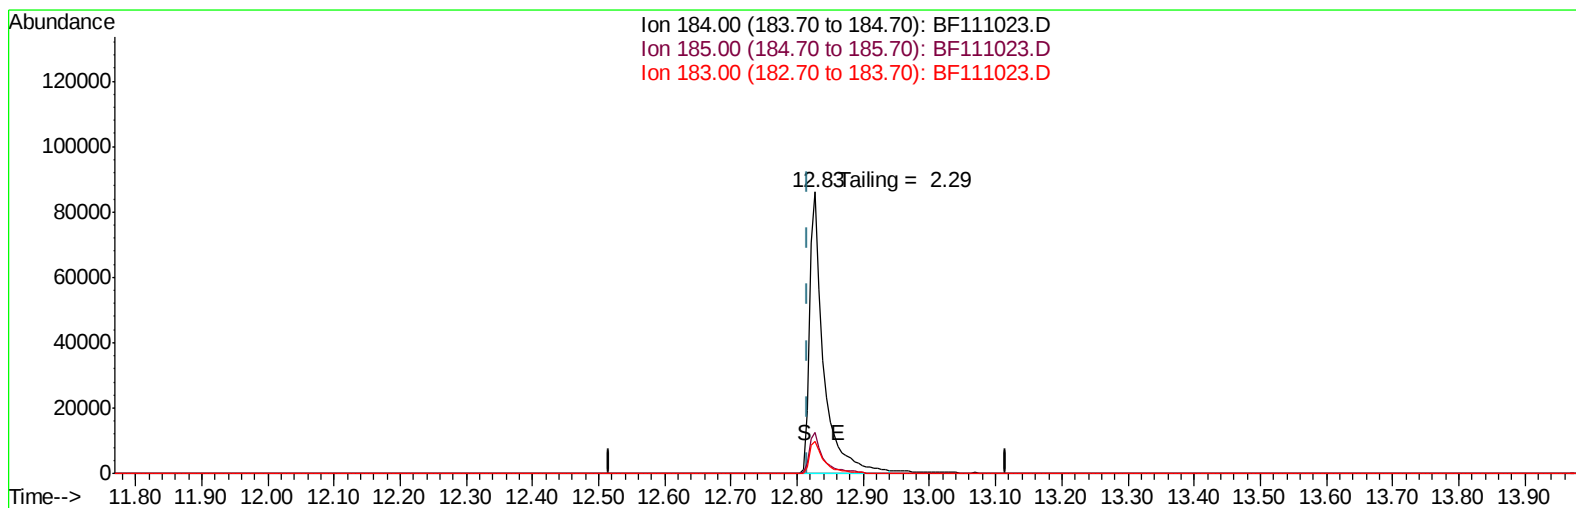

TIC: BF111023.D

(77) Benzidine

12.827min (+0.012) 0.00ng

response 129866

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.36
183.00	11.80	11.60
0.00	0.00	0.00