

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112718\
 Data File : BF111030.D
 Acq On : 28 Nov 2018 1:36
 Operator : JU/SJ
 Sample : J6070-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 112118-CHDE-E-U-S

Quant Time: Nov 28 03:48:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 27 15:32:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	46643	20.00	ng	0.00
21) Naphthalene-d8	8.22	136	169783	20.00	ng	0.00
39) Acenaphthene-d10	9.98	164	68694	20.00	ng	0.00
64) Phenanthrene-d10	11.48	188	134956	20.00	ng	0.00
76) Chrysene-d12	14.13	240	112907	20.00	ng	0.00
87) Perylene-d12	15.67	264	71506	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	114872	40.84	ng	0.01
7) Phenol-d6	6.57	99	79658	21.73	ng	0.00
23) Nitrobenzene-d5	7.50	82	281323	94.83	ng	0.00
42) 2,4,6-Tribromophenol	10.78	330	60317	88.41	ng	0.00
45) 2-Fluorobiphenyl	9.29	172	466771	98.44	ng	0.00
79) Terphenyl-d14	13.06	244	514130	88.64	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112718\
Data File : BF111030.D
Acq On : 28 Nov 2018 1:36
Operator : JU/SJ
Sample : J6070-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112118-CHDE-E-U-S

Quant Time: Nov 28 03:48:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 27 15:32:10 2018
Response via : Initial Calibration

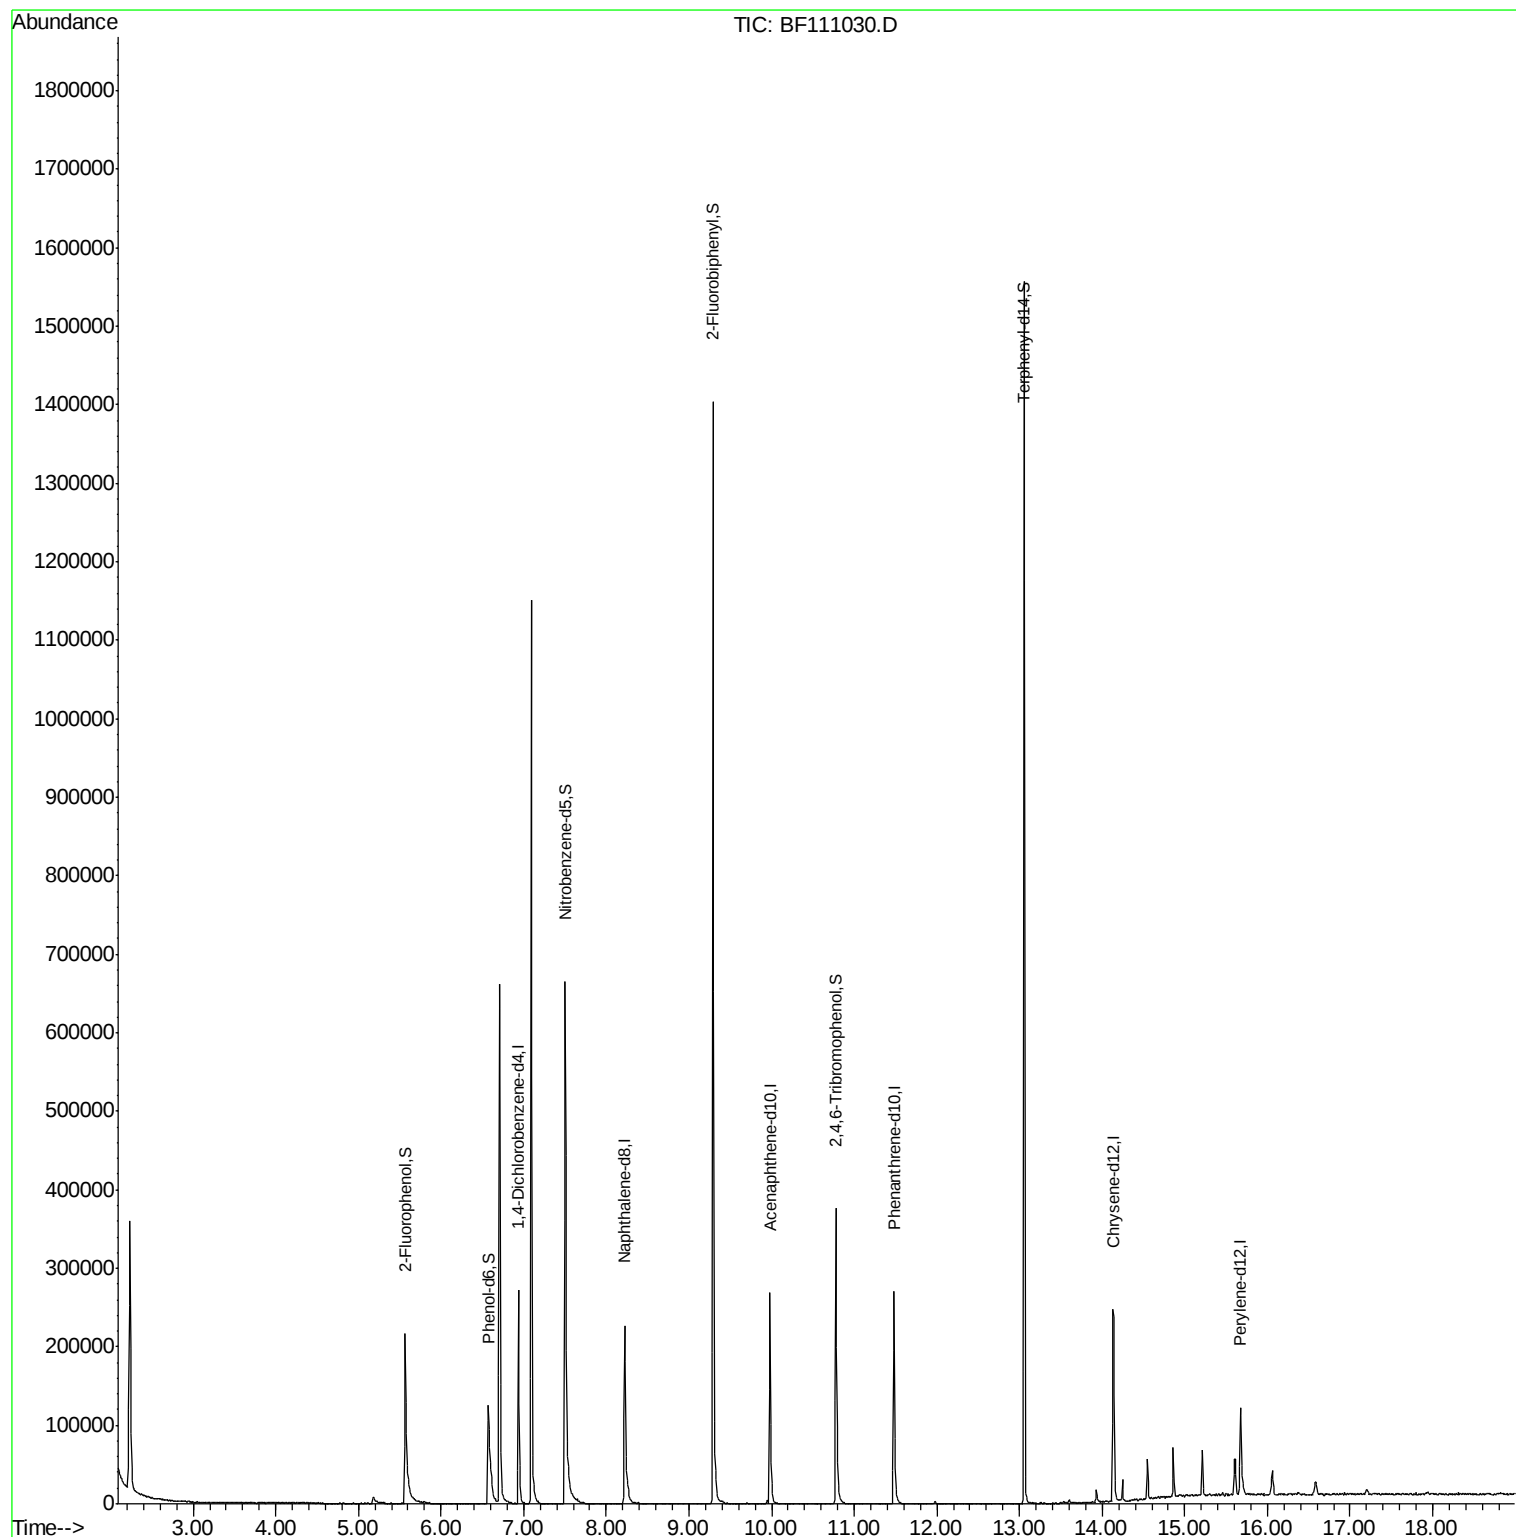

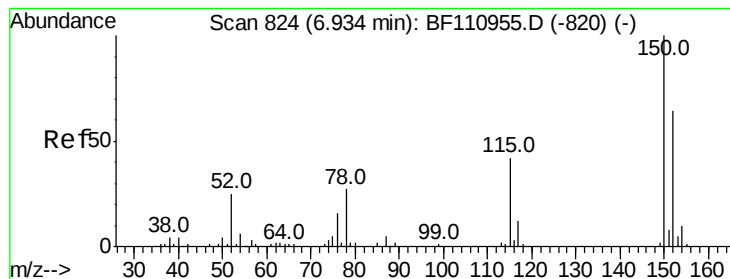


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.94 min Scan# 825
Delta R.T. 0.01 min
Lab File: BF111030.D
Acq: 28 Nov 2018 1:36

Instrument :
BNA_F
ClientSampleId :
112118-CHDE-E-U-S

Tot Ion:152 Resp: 46643
Ion Ratio Lower Upper
152 100
150 159.3 122.7 184.1
115 61.2 49.1 73.7

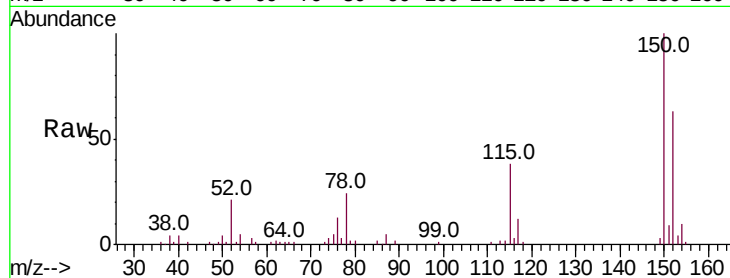


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

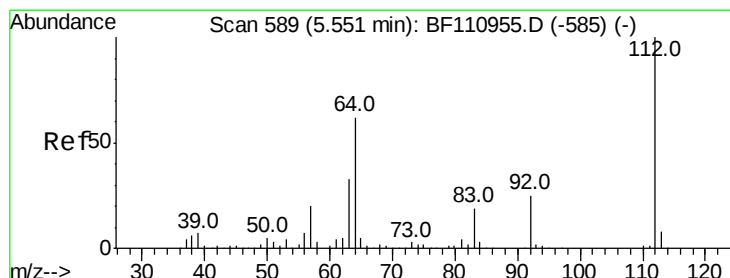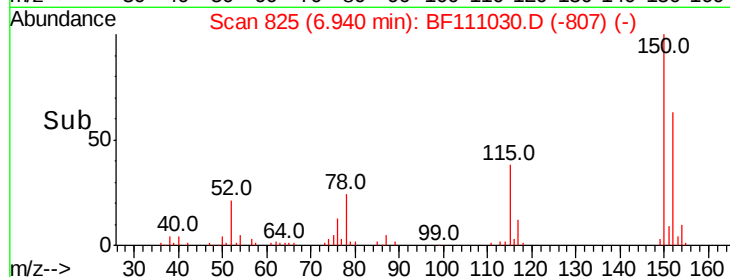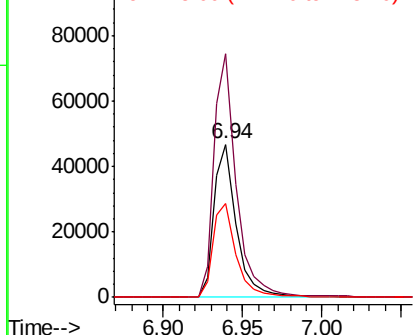



#5


2-Fluorophenol
Concen: 40.841 ng
RT: 5.56 min Scan# 591
Delta R.T. 0.01 min
Lab File: BF111030.D
Acq: 28 Nov 2018 1:36

Tgt Ion:112 Resp: 114872
Ion Ratio Lower Upper
112 100
64 60.9 44.1 66.1
63 31.4 23.7 35.5

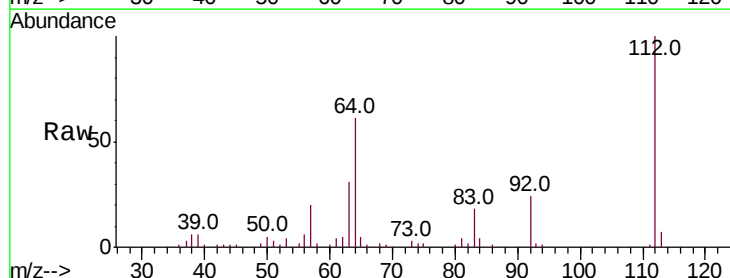

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

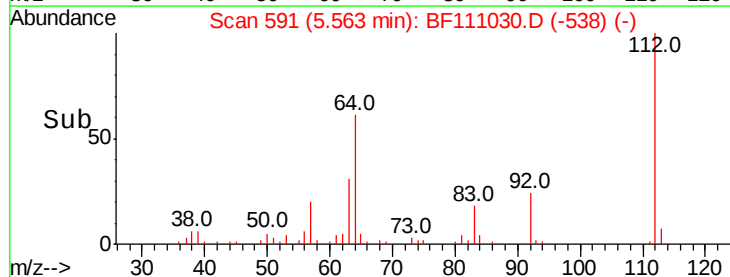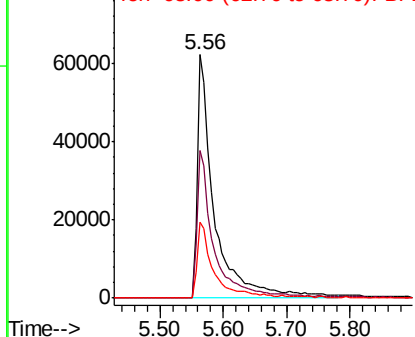

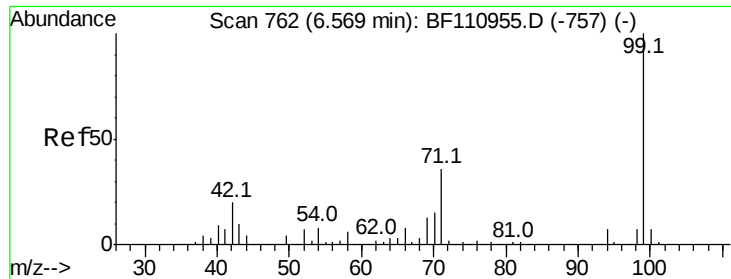

#7

Phenol-d6

Concen: 21.733 ng

RT: 6.57 min Scan# 763

Delta R.T. 0.01 min

Lab File: BF111030.D

Acq: 28 Nov 2018 1:36

Instrument :

BNA_F

ClientSampleId :

112118-CHDE-E-U-S


Tot Ion: 99 Resp: 79658

Ion Ratio Lower Upper




99 100

42 19.4 15.8 23.6

71 34.7 28.0 42.0

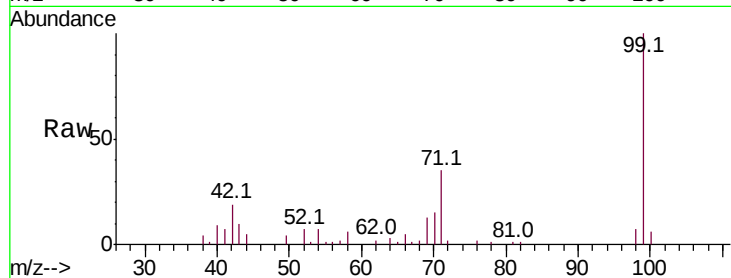

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

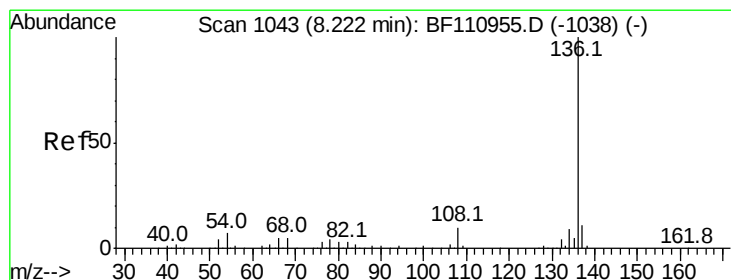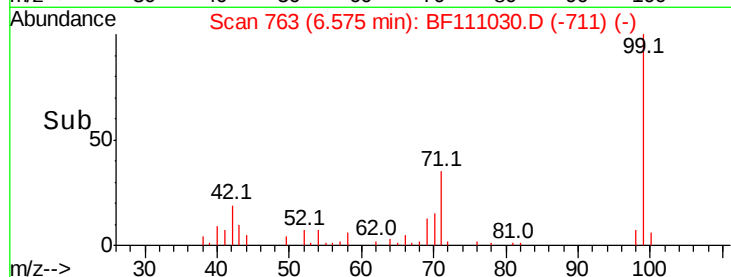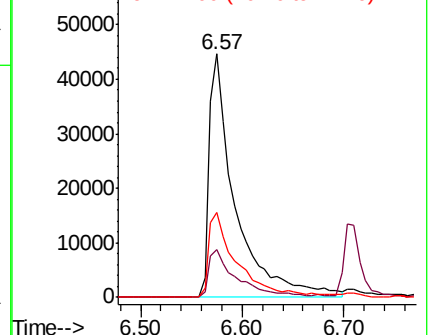

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.22 min Scan# 1043

Delta R.T. -0.00 min

Lab File: BF111030.D

Acq: 28 Nov 2018 1:36

Tgt Ion: 136 Resp: 169783


Ion Ratio Lower Upper

136 100



137 11.0 8.8 13.2


54 7.9 5.4 8.2

68 5.0 4.2 6.2

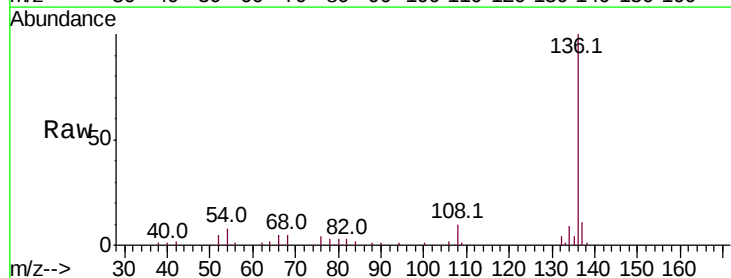

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

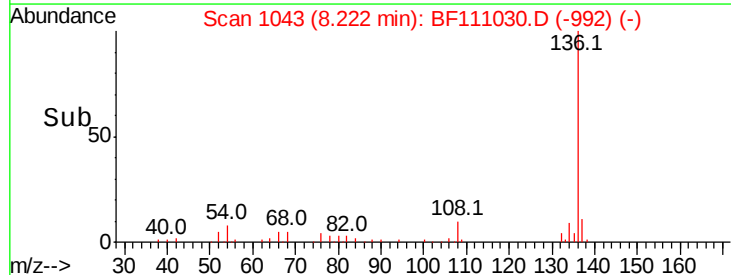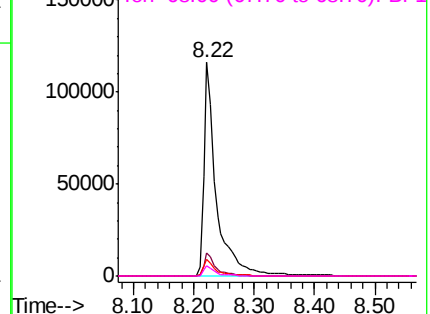


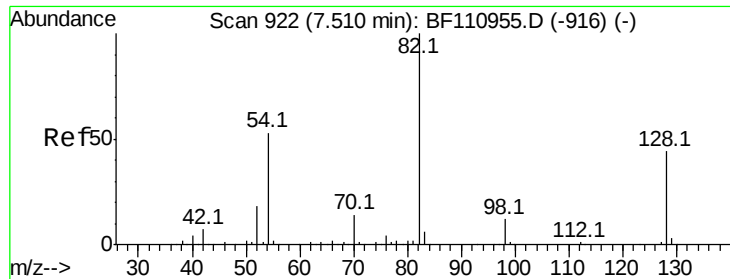




#23
Nitrobenzene-d5
Concen: 94.829 ng
RT: 7.50 min Scan# 921
Delta R.T. -0.01 min
Lab File: BF111030.D
Acq: 28 Nov 2018 1:36

Instrument :
BNA_F
ClientSampleId :
112118-CHDE-E-U-S

Tot Ion: 82 Resp: 281323
Ion Ratio Lower Upper
82 100
128 43.7 34.2 51.2
54 53.0 38.6 58.0

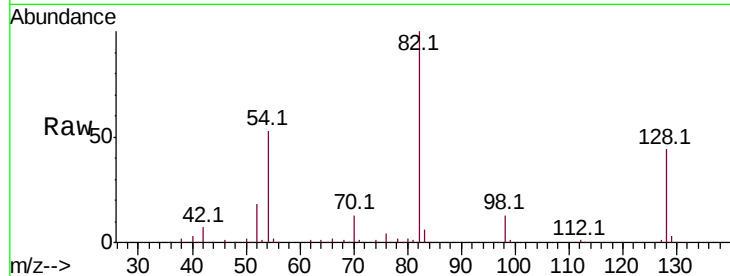


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

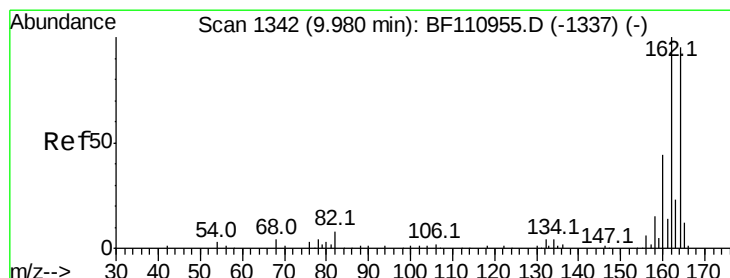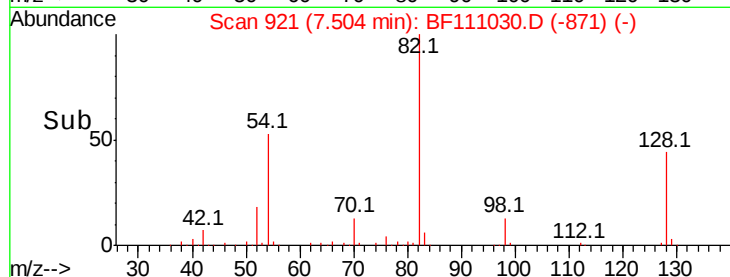
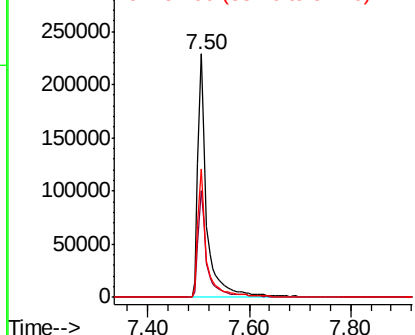



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.98 min Scan# 1342
Delta R.T. -0.00 min
Lab File: BF111030.D
Acq: 28 Nov 2018 1:36

Tgt Ion:164 Resp: 68694
Ion Ratio Lower Upper
164 100
162 101.0 83.0 124.6
160 45.3 37.0 55.6

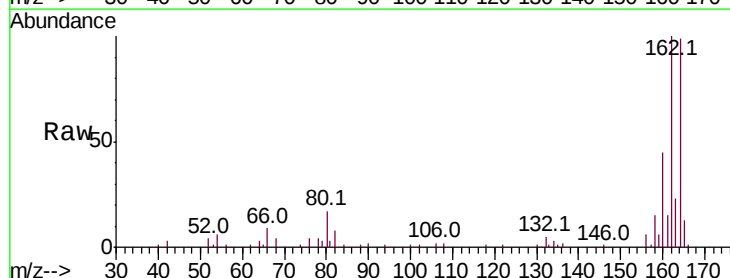

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

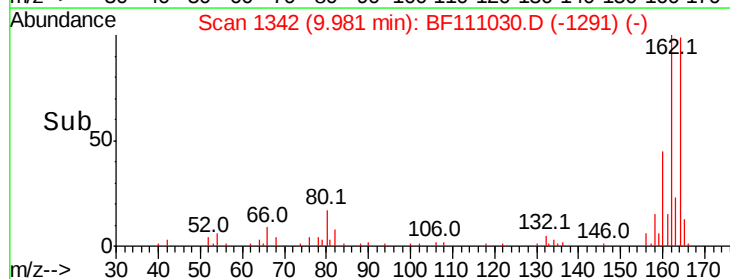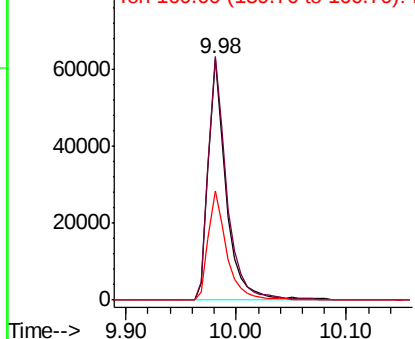


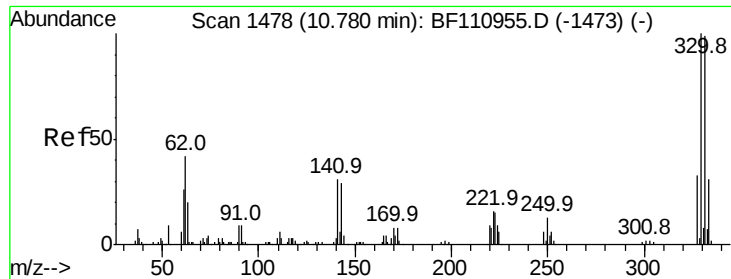




#42
 2,4,6-Tribromophenol
 Concen: 88.412 ng
 RT: 10.78 min Scan# 1478
 Delta R.T. -0.00 min
 Lab File: BF111030.D
 Acq: 28 Nov 2018 1:36

Instrument :
 BNA_F
 ClientSampleId :
 112118-CHDE-E-U-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	77.1	115.7
141	38.8	27.0	40.4

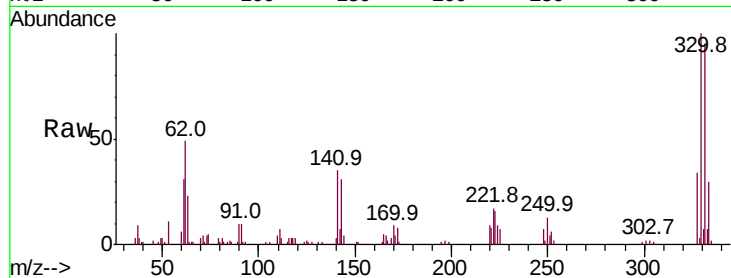


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

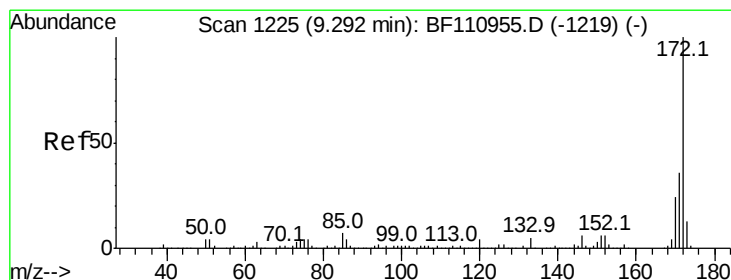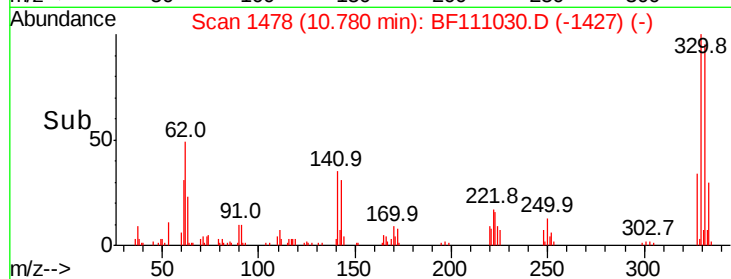
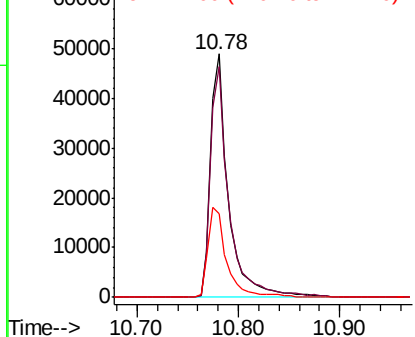



#45
 2-Fluorobiphenyl
 Concen: 98.443 ng
 RT: 9.29 min Scan# 1225
 Delta R.T. -0.00 min
 Lab File: BF111030.D
 Acq: 28 Nov 2018 1:36

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.6	28.6	43.0
170	23.1	19.7	29.5

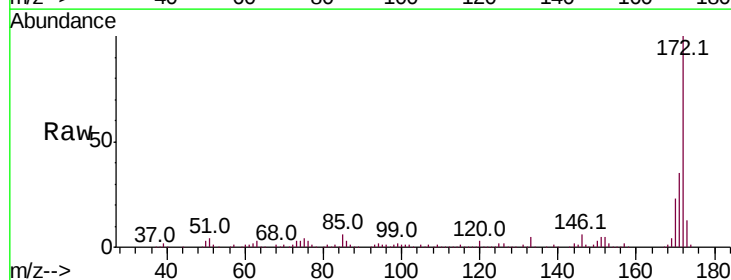

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

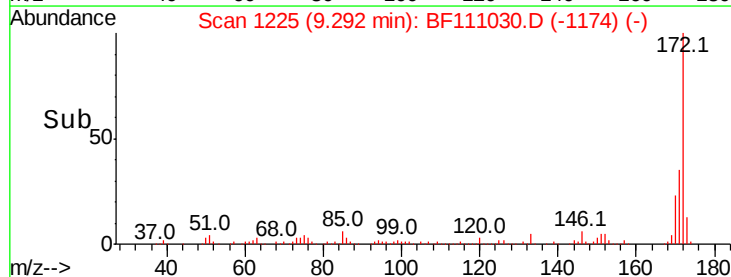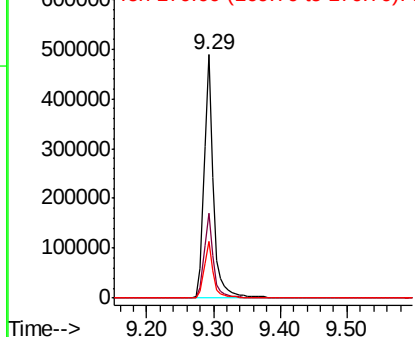

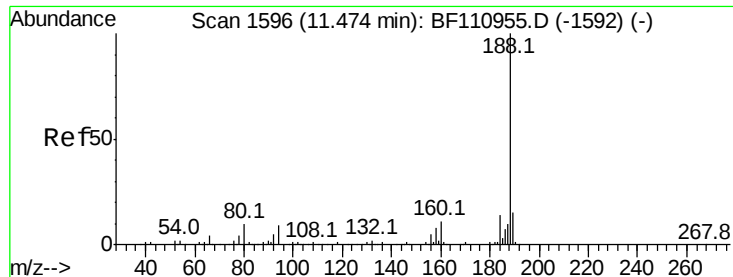

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.48 min Scan# 1597

Delta R.T. 0.01 min

Lab File: BF111030.D

Acq: 28 Nov 2018 1:36

Instrument :

BNA_F

ClientSampleId :

112118-CHDE-E-U-S


Tot Ion:188 Resp: 134956

Ion Ratio Lower Upper

188 100

94 8.5 7.2 10.8




80 9.3 7.9 11.9

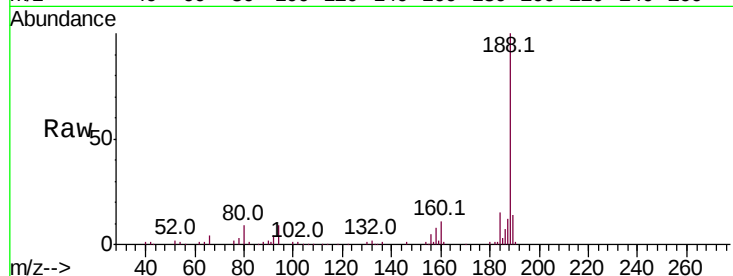

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

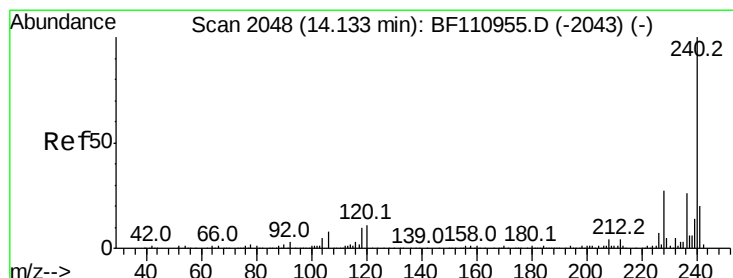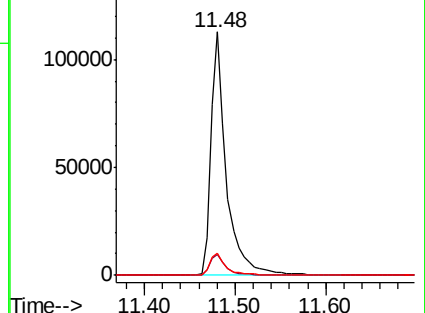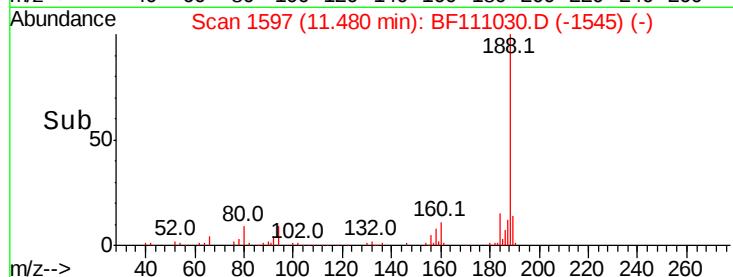

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.13 min Scan# 2048

Delta R.T. -0.00 min

Lab File: BF111030.D

Acq: 28 Nov 2018 1:36


Tgt Ion:240 Resp: 112907

Ion Ratio Lower Upper

240 100

120 12.3 8.3 12.5



236 25.7 21.2 31.8

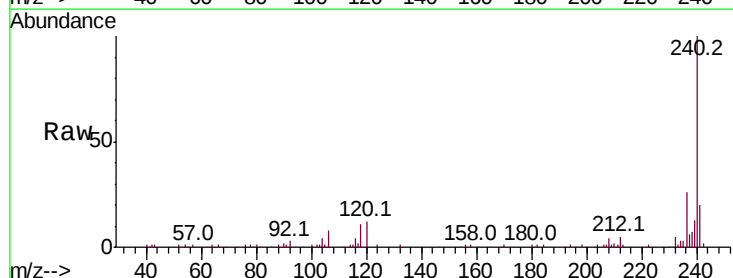


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

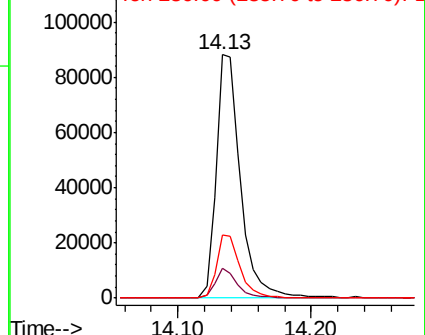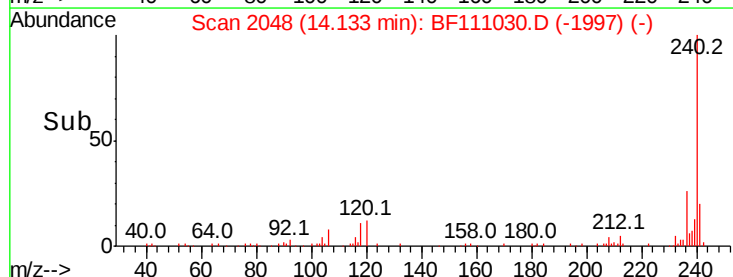

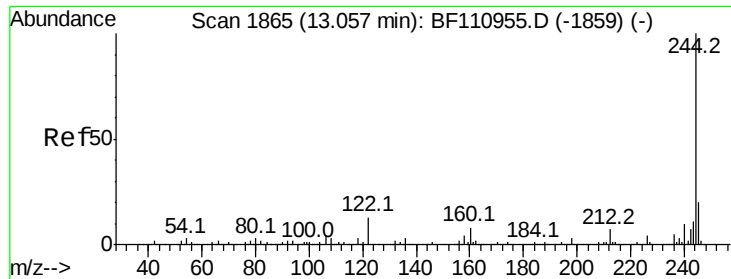

#79

Terphenyl-d14

Concen: 88.642 ng

RT: 13.06 min Scan# 1865

Delta R.T. -0.00 min

Lab File: BF111030.D

Acq: 28 Nov 2018 1:36

Instrument :

BNA_F

ClientSampleId :

112118-CHDE-E-U-S


Tot Ion:244 Resp: 514130

Ion Ratio Lower Upper

244 100

212 7.1 5.8 8.8




122 12.9 8.7 13.1

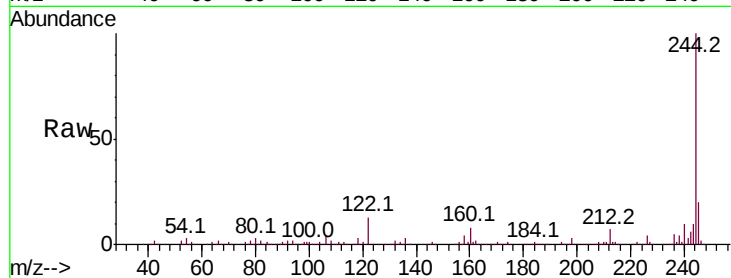

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

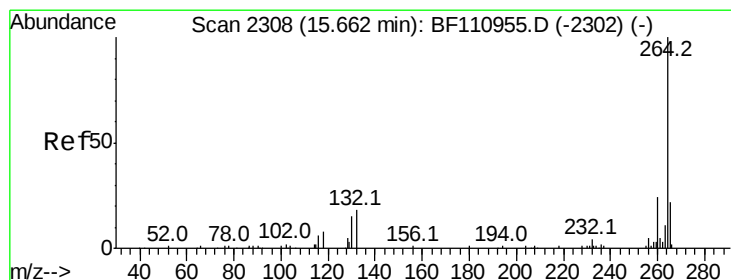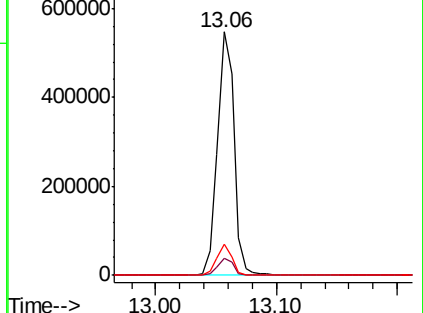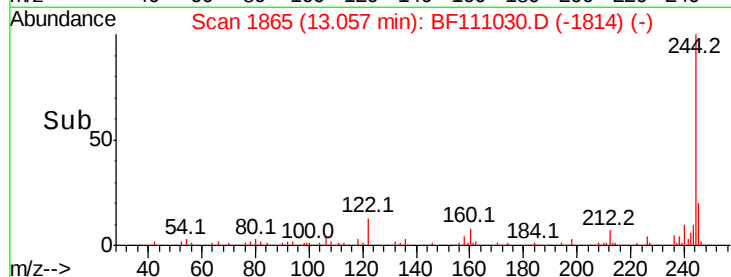

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.67 min Scan# 2310

Delta R.T. 0.01 min

Lab File: BF111030.D

Acq: 28 Nov 2018 1:36


Tgt Ion:264 Resp: 71506

Ion Ratio Lower Upper

264 100

260 22.3 18.7 28.1

265 21.3 16.7 25.1

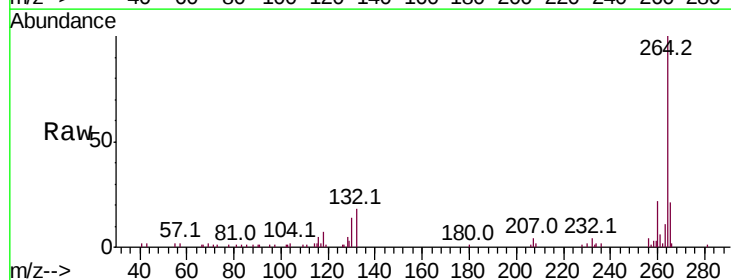

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

