


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112718\
 Data File : BF110996.D
 Acq On : 27 Nov 2018 9:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF112618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 27 15:32:10 2018

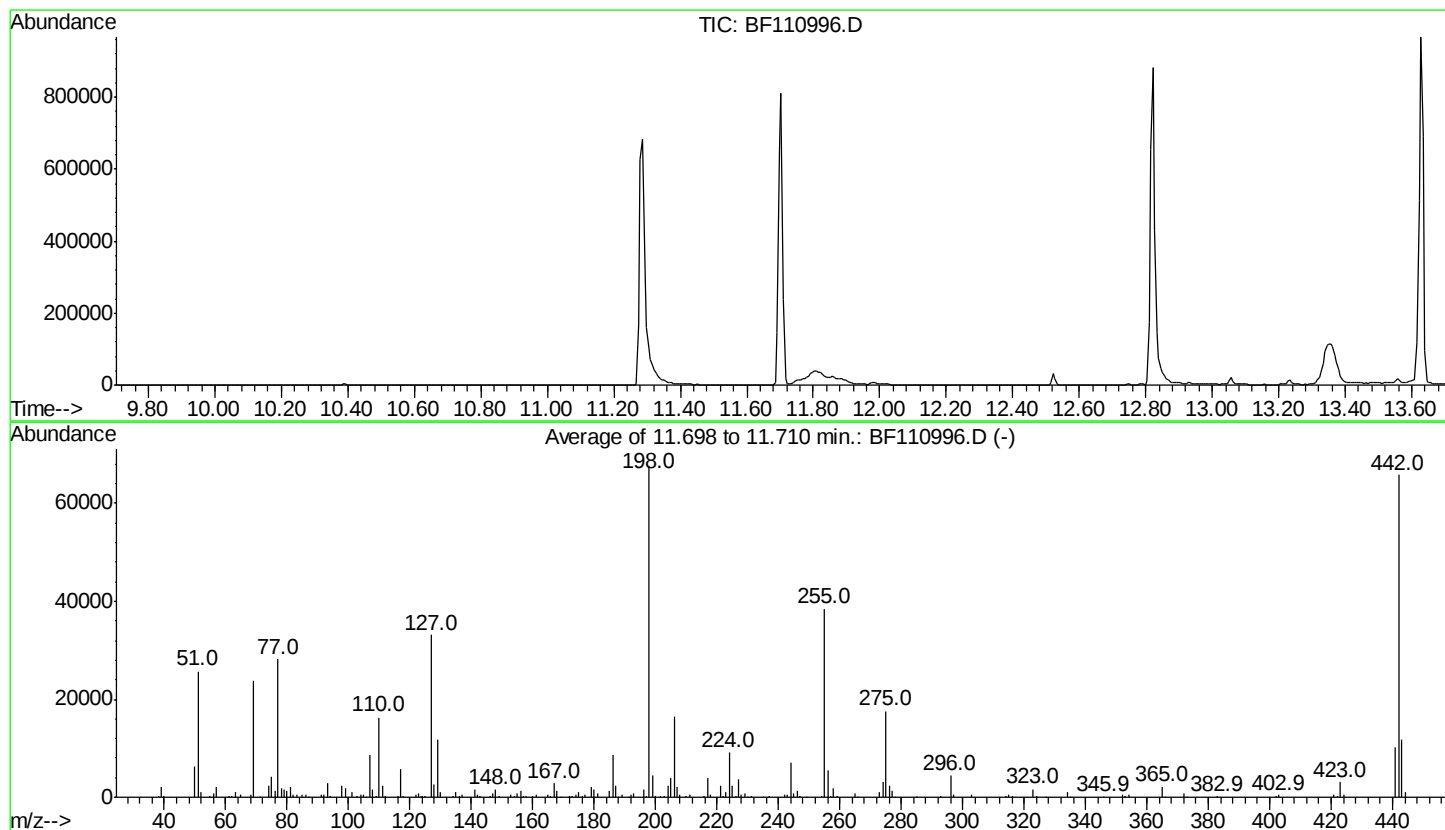

AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	25650	PASS
68	69	0.00	2	1.7	405	PASS
69	198	0.00	100	35.1	23800	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	33149	PASS
197	198	0.00	2	0.5	317	PASS
198	198	100	100	100.0	67717	PASS
199	198	5	9	6.6	4460	PASS
275	198	10	60	25.9	17528	PASS
365	198	1	100	3.1	2113	PASS
441	198	0.01	100	14.9	10104	PASS
442	198	50	100	97.2	65821	PASS
443	442	15	24	17.8	11695	PASS