
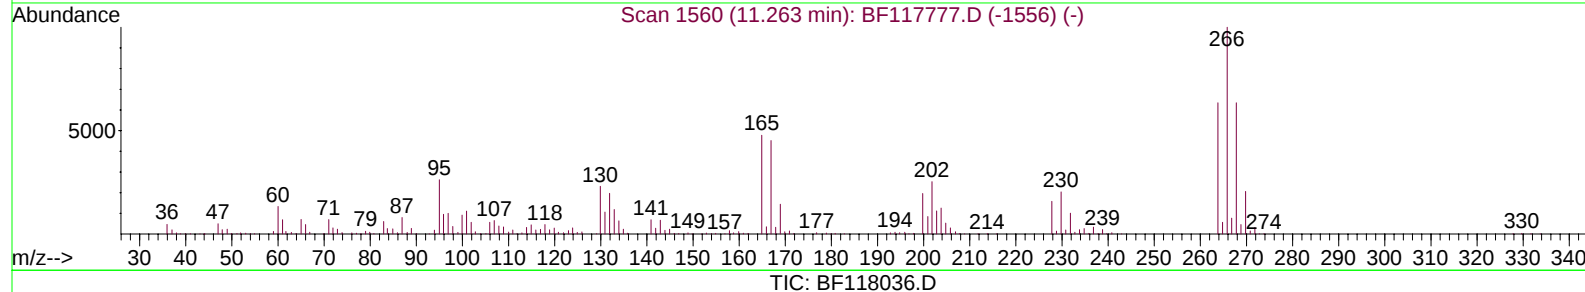
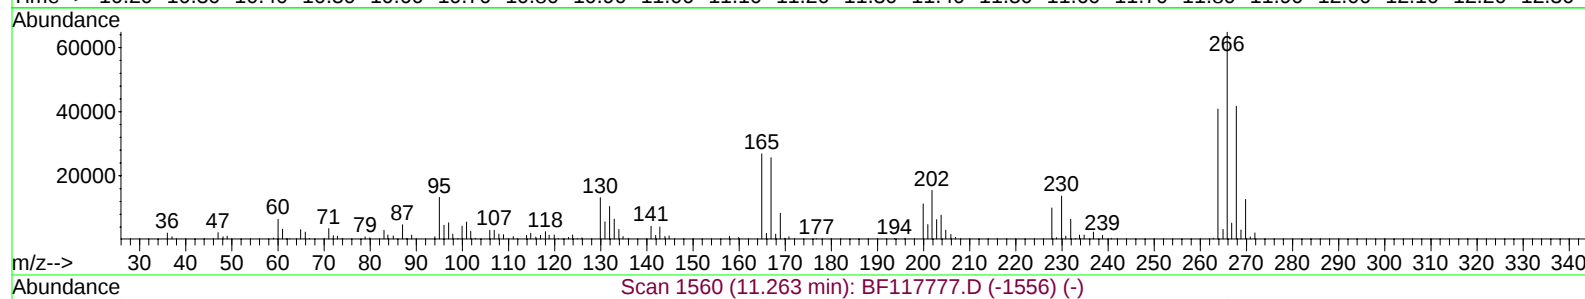


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112719\
Data File : BF118036.D
Acq On : 27 Nov 2019 11:51
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 14:23:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:38:20 2019
Response via : Initial Calibration

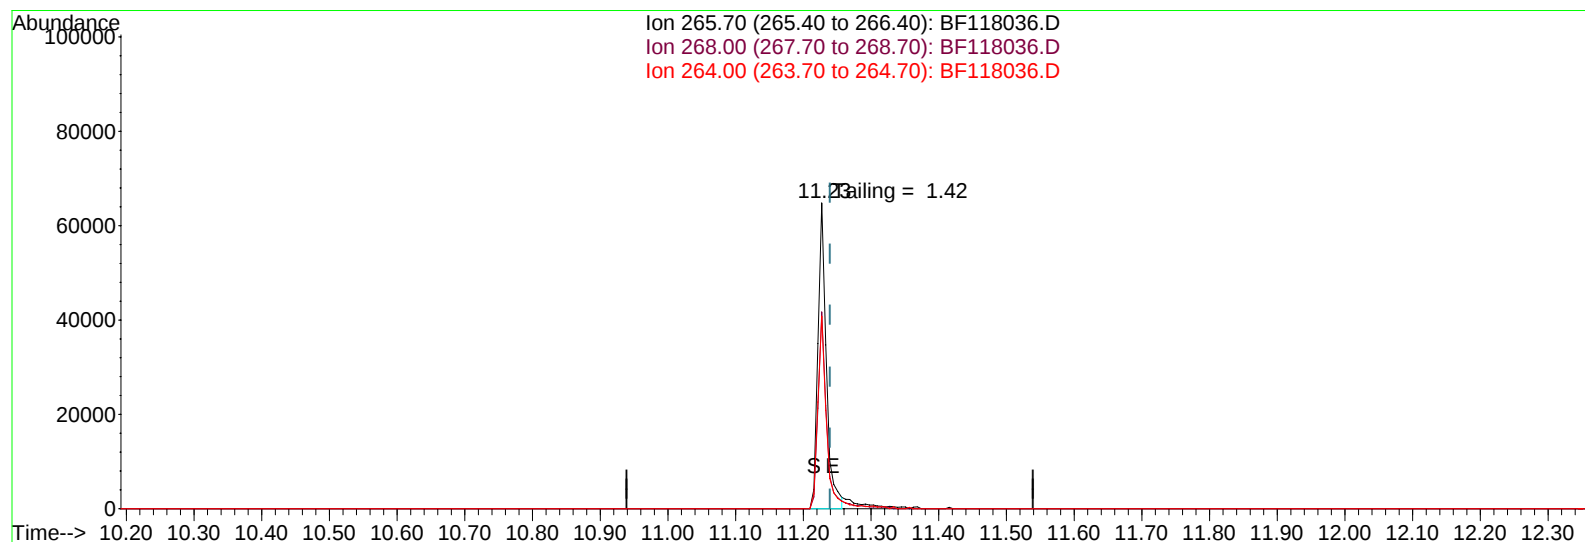

(70) Pentachlorophenol (C)




11.227min (-0.012) 23887.59ng

response 61104

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	64.35
264.00	63.40	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112719\
 Data File : BF118036.D
 Acq On : 27 Nov 2019 11:51
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 14:23:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 05:38:20 2019
 Response via : Initial Calibration

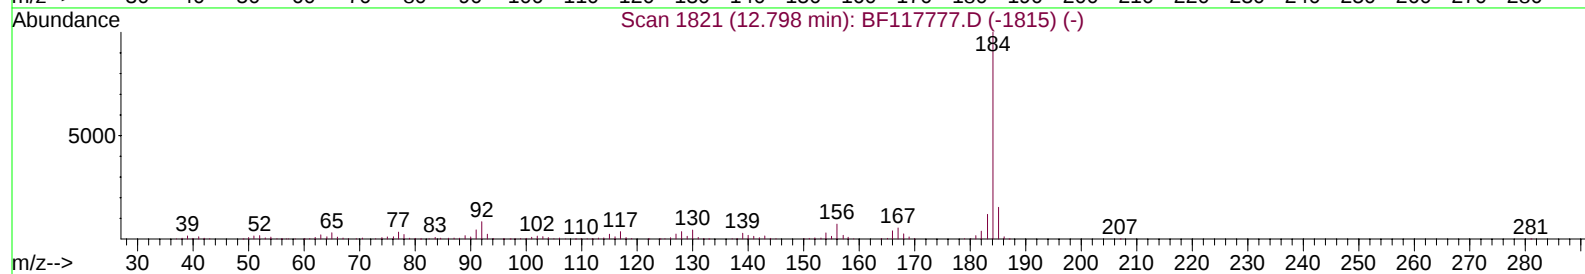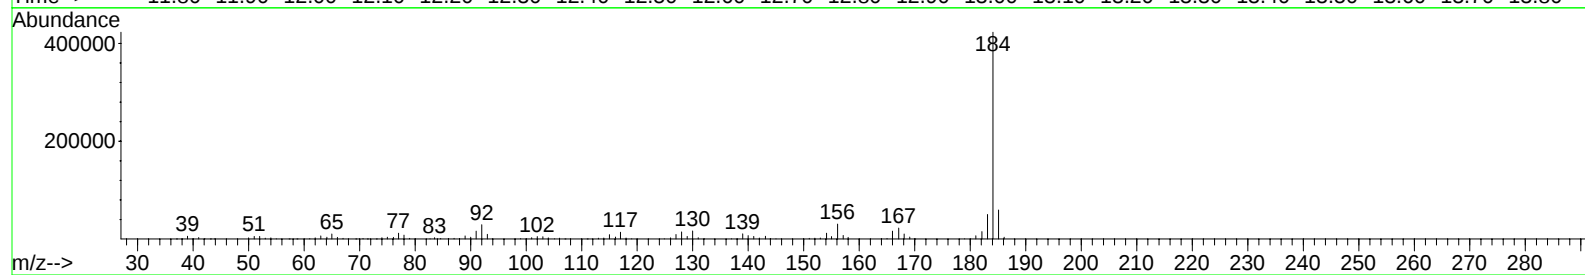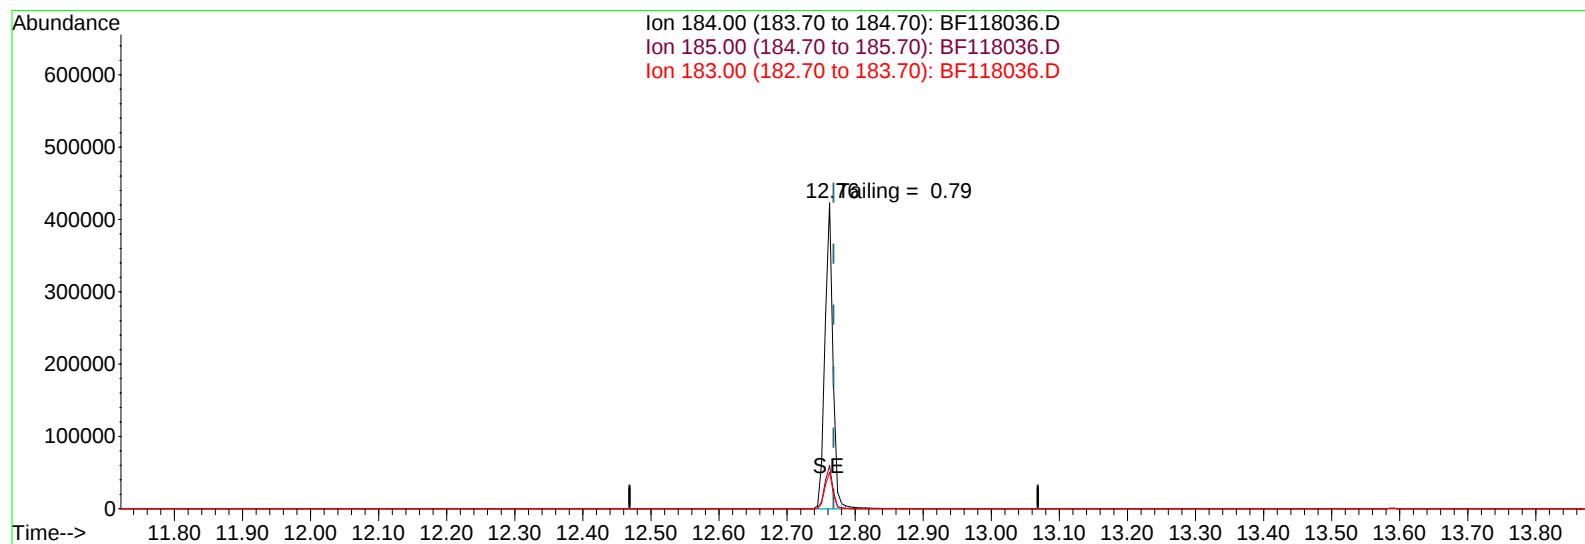

TIC: BF118036.D

(77) Benzidine

12.762min (-0.006) 0.00ng

response 343726

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.09
183.00	11.90	11.91
0.00	0.00	0.00