

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112719\
 Data File : BF118053.D
 Acq On : 27 Nov 2019 20:55
 Operator : JU
 Sample : K5999-02 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 IDLEWILD-BH-01B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	504	508	513	rBV	47704	46902	4.74%	0.592%
2	5.487	575	578	589	rBV	269795	263664	26.65%	3.329%
3	6.504	747	751	763	rBV	306163	294249	29.75%	3.715%
4	6.645	772	775	779	rBV	340429	309002	31.24%	3.901%
5	6.887	812	816	819	rBV	790585	709809	71.75%	8.962%
6	7.040	838	842	850	rBV	294810	229996	23.25%	2.904%
7	7.439	907	910	916	rBV	188164	166446	16.83%	2.101%
8	8.169	1031	1034	1038	rBV	1071023	904574	91.44%	11.421%
9	9.245	1214	1217	1228	rBV	421800	329455	33.30%	4.160%
10	9.639	1282	1284	1288	rBV	52947	47853	4.84%	0.604%
11	9.933	1330	1334	1338	rBV	1257906	989236	100.00%	12.490%
12	10.480	1424	1427	1434	rVB3	9270	14957	1.51%	0.189%
13	10.586	1440	1445	1450	rVB3	8505	13423	1.36%	0.169%
14	10.722	1465	1468	1475	rBV	209033	183740	18.57%	2.320%
15	10.851	1485	1490	1493	rVB	22196	20714	2.09%	0.262%
16	11.316	1566	1569	1575	rVB3	19054	22102	2.23%	0.279%
17	11.427	1584	1588	1591	rBV	1118776	908985	91.89%	11.476%
18	11.451	1591	1592	1596	rVB	50264	29364	2.97%	0.371%
19	11.539	1603	1607	1610	rBV4	9076	12708	1.28%	0.160%
20	11.663	1625	1628	1632	rBV4	11263	13953	1.41%	0.176%
21	11.945	1671	1676	1683	rBV5	46984	73172	7.40%	0.924%
22	12.357	1744	1746	1748	rBV2	13554	14373	1.45%	0.181%
23	12.404	1752	1754	1756	rBV3	11674	12663	1.28%	0.160%
24	12.645	1792	1795	1799	rBV	47778	42599	4.31%	0.538%
25	12.739	1808	1811	1814	rBV4	28454	35502	3.59%	0.448%
26	12.874	1831	1834	1841	rBV	52402	67215	6.79%	0.849%
27	13.016	1854	1858	1861	rBV	366630	315715	31.92%	3.986%
28	13.204	1888	1890	1893	rVB2	24985	19983	2.02%	0.252%
29	14.080	2035	2039	2042	rBV	1058572	905106	91.50%	11.427%
30	15.586	2290	2295	2305	rVB	618649	923078	93.31%	11.654%


Sum of corrected areas: 7920538

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112719\
Data File : BF118053.D
Acq On : 27 Nov 2019 20:55
Operator : JU
Sample : K5999-02 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IDLEWILD-BH-01B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

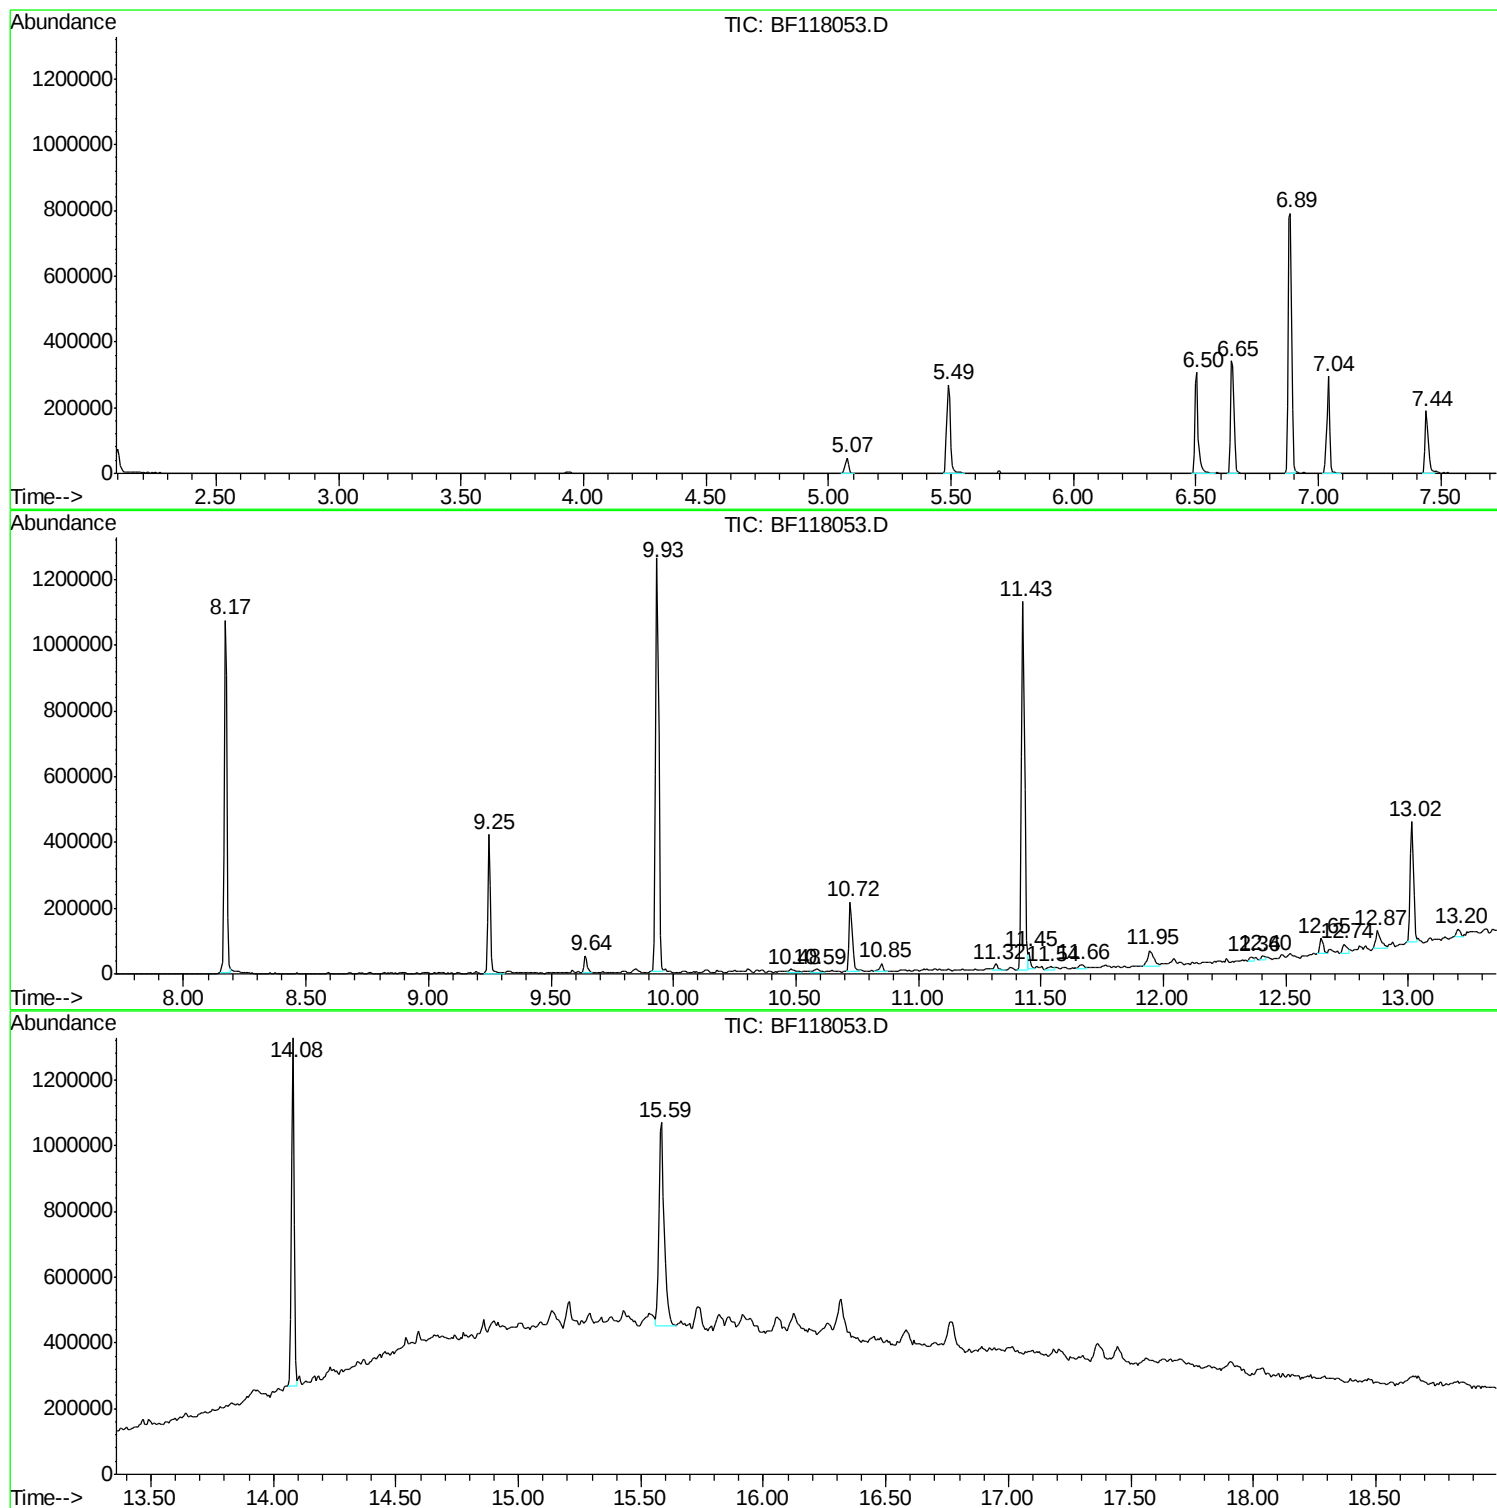

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112719\
Data File : BF118053.D
Acq On : 27 Nov 2019 20:55
Operator : JU
Sample : K5999-02 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IDLEWILD-BH-01B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	8.71 ng	309002	1,4-Dichlorobenzene-d4	6.89

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3			1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

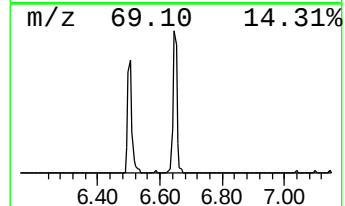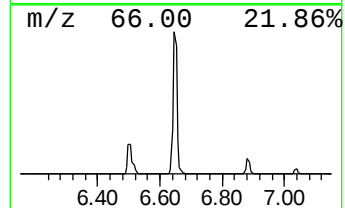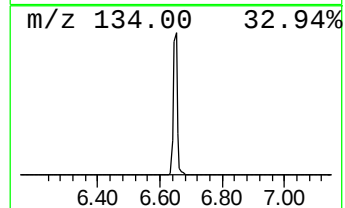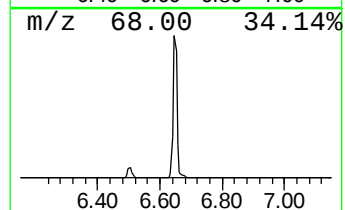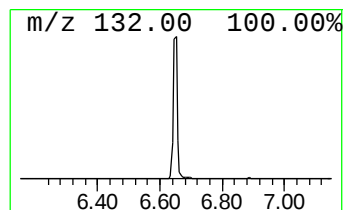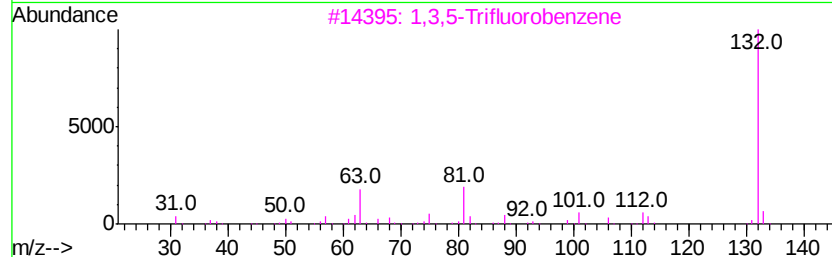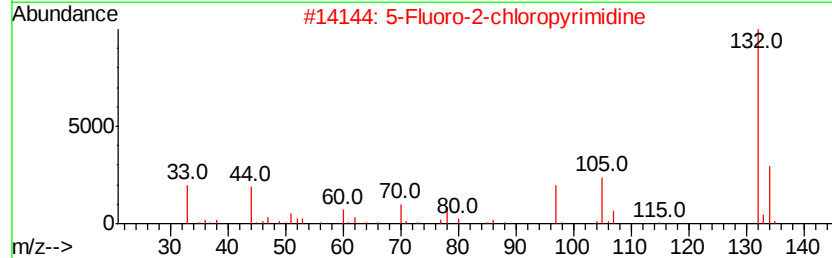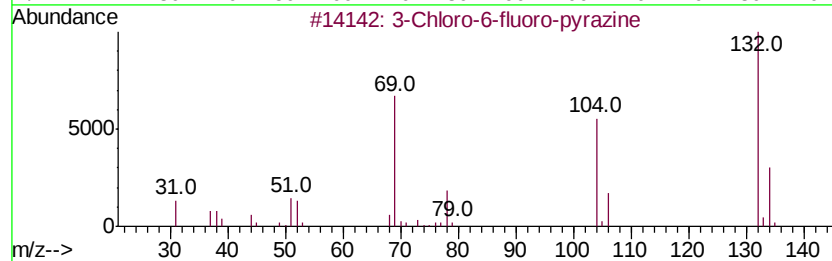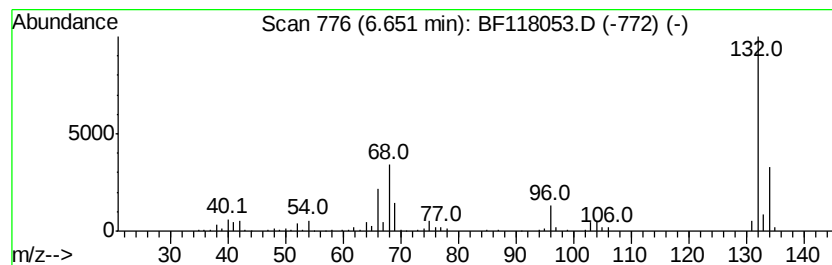

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112719\
Data File : BF118053.D
Acq On : 27 Nov 2019 20:55
Operator : JU
Sample : K5999-02 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
IDLEWILD-BH-01B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.65	6.65	8.7	ng	309002	1	6.89	709809	20.0