


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112719\
 Data File : BF118036.D
 Acq On : 27 Nov 2019 11:51
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 26 05:38:20 2019

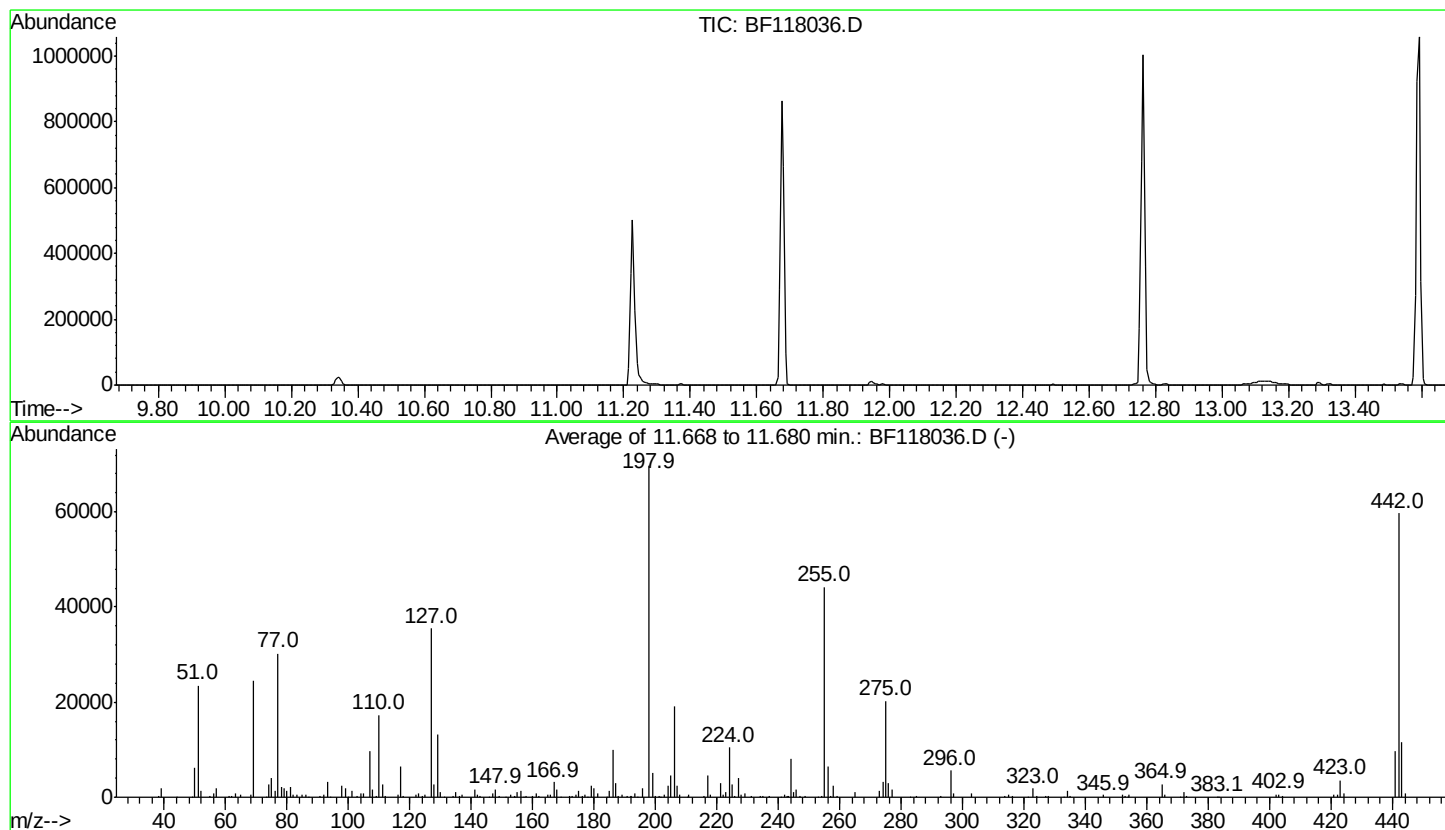

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	23424	PASS
68	69	0.00	2	2.0	490	PASS
69	198	0.00	100	35.2	24520	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	35426	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69728	PASS
199	198	5	9	7.3	5066	PASS
275	198	10	60	29.0	20218	PASS
365	198	1	100	4.0	2819	PASS
441	198	0.01	100	13.8	9629	PASS
442	198	50	100	85.6	59704	PASS
443	442	15	24	19.2	11491	PASS