
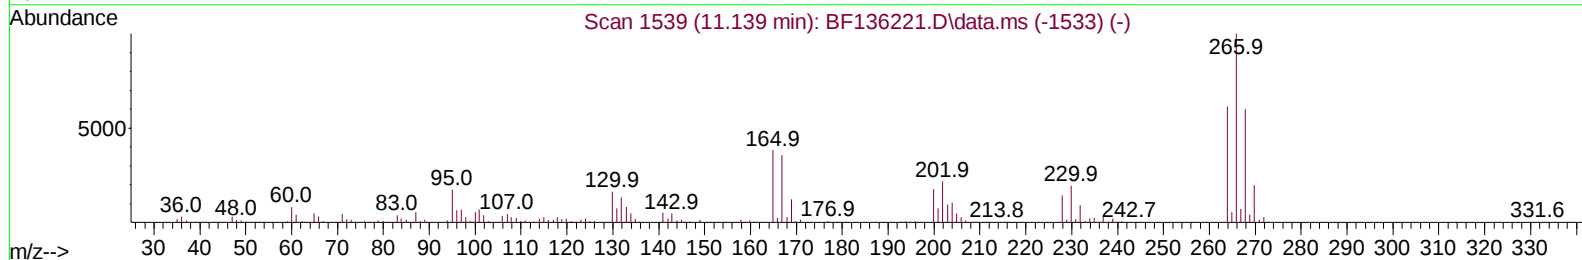
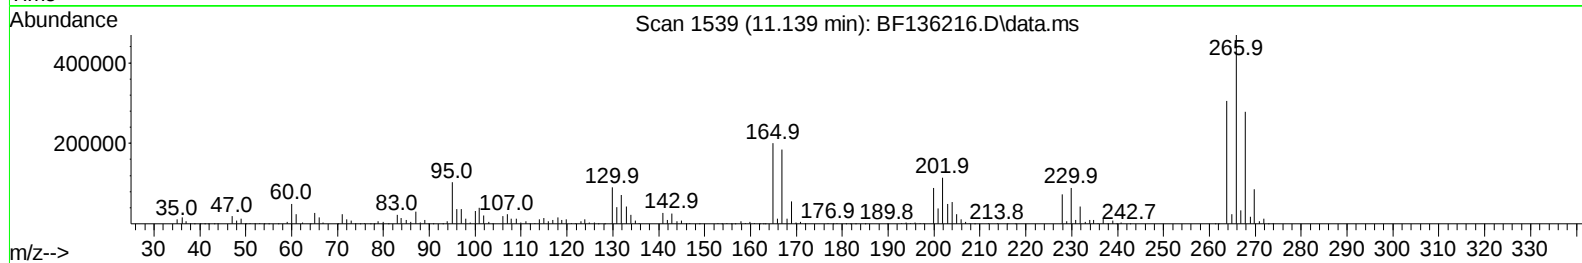


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112723\
Data File : BF136216.D
Acq On : 27 Nov 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 04:45:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

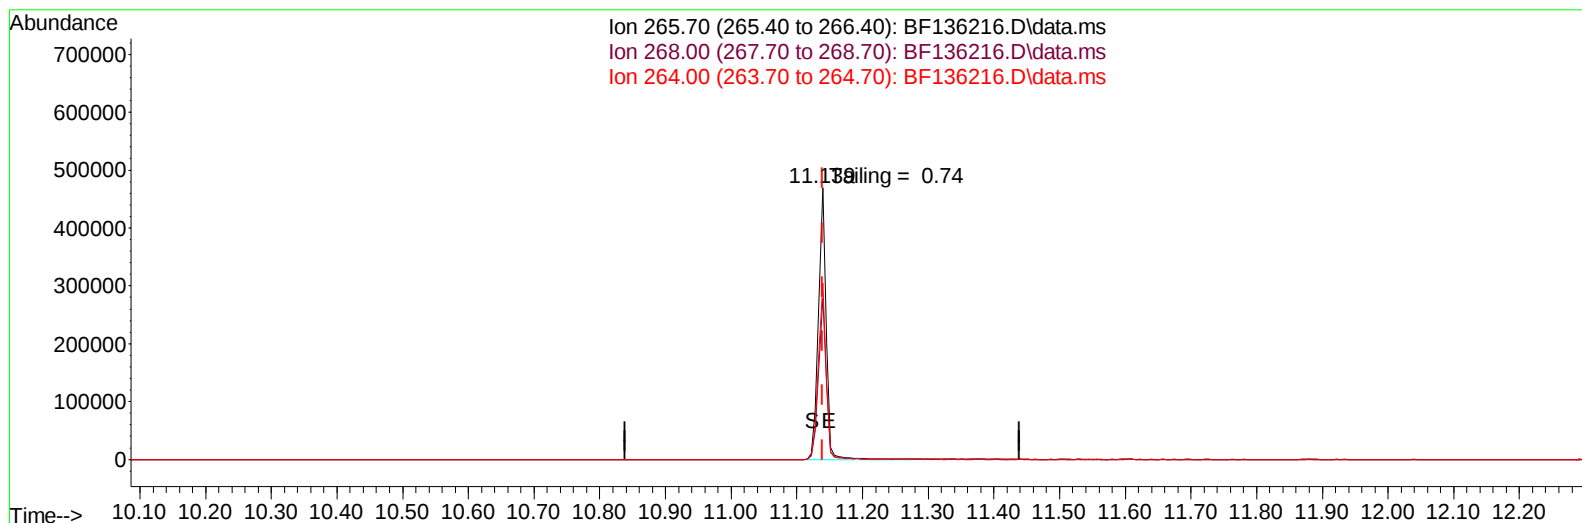

TIC: BF136216.D\data.ms

(70) Pentachlorophenol (C)




11.139min (+ 0.000) 86719.19 ng

response 391169

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	59.41
264.00	61.40	65.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112723\
Data File : BF136216.D
Acq On : 27 Nov 2023 11:17
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 04:45:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

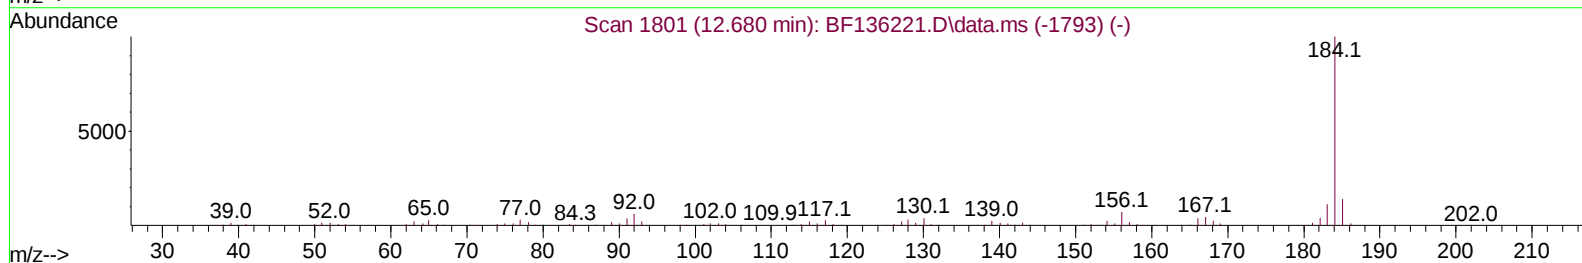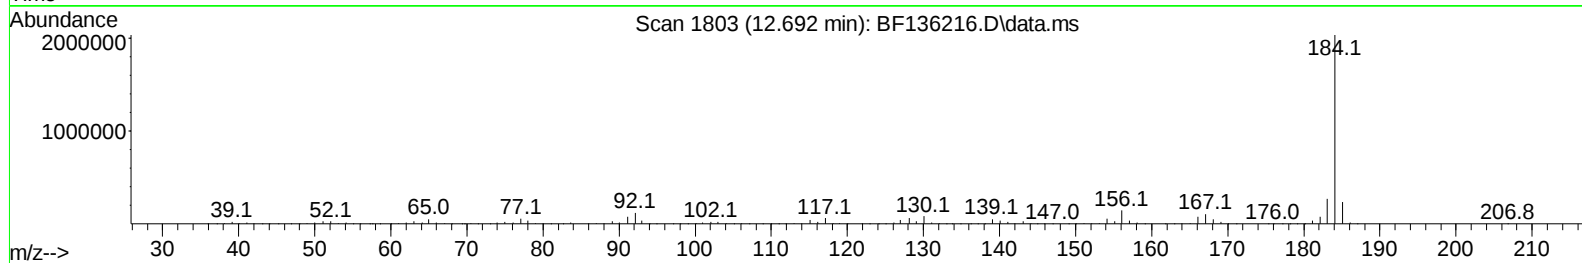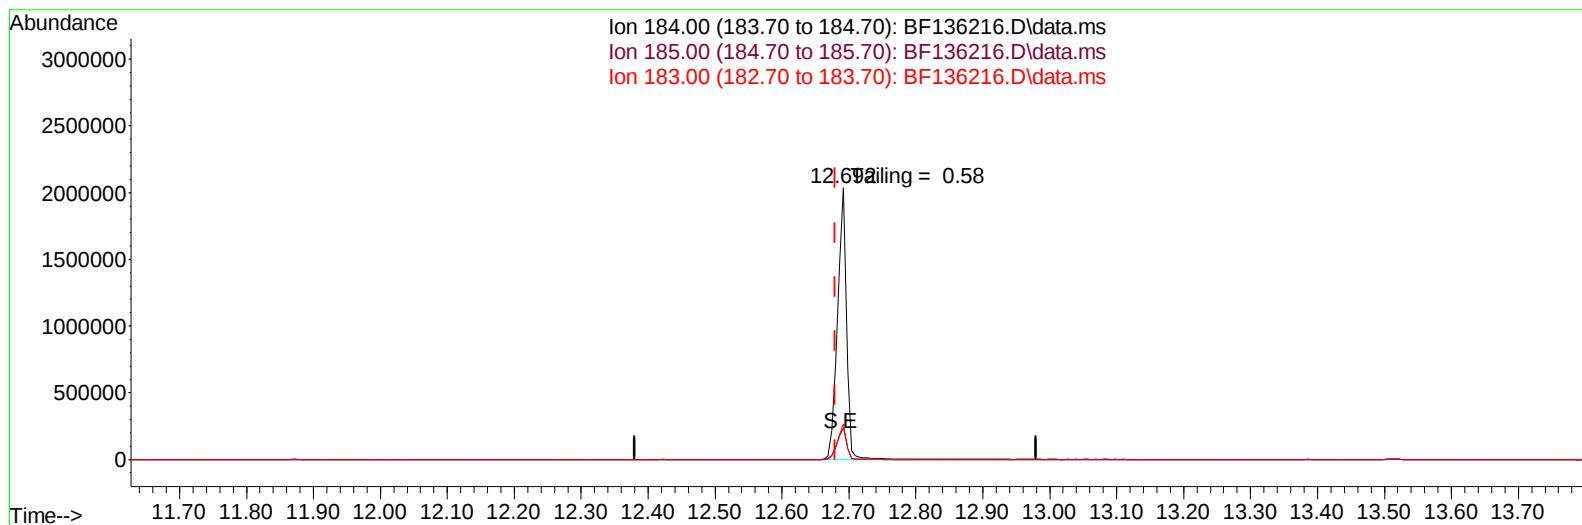

TIC: BF136216.D\data.ms

(77) Benzidine**12.692min (+ 0.012) 16125.67 ng****response 1873836**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	11.70
183.00	11.20	13.22
0.00	0.00	0.00