


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112723\
Data File : BF136216.D
Acq On : 27 Nov 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 28 03:04:20 2023

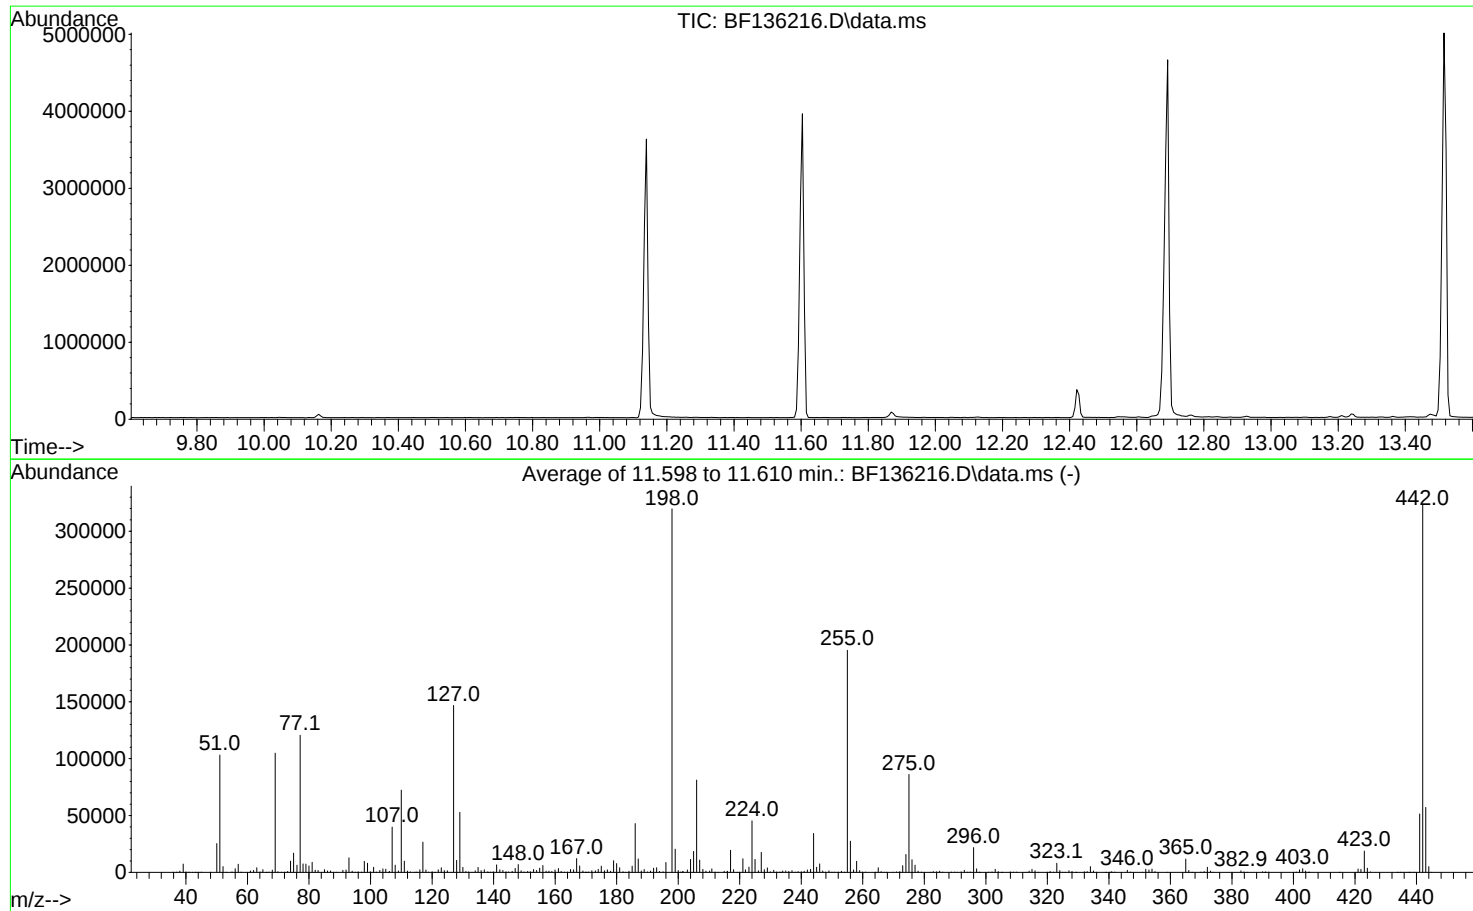




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	103120	PASS
68	69	0.00	2	1.9	2042	PASS
69	198	0.00	100	32.8	104896	PASS
70	69	0.00	2	0.5	547	PASS
127	198	10	80	45.9	146720	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	319701	PASS
199	198	5	9	6.4	20460	PASS
275	198	10	60	26.9	86067	PASS
365	198	1	100	3.6	11629	PASS
441	198	0.01	100	16.1	51331	PASS
442	442	50	100	100.0	323541	PASS
443	442	15	24	17.7	57149	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112723\
Data File : BF136216.D
Acq On : 27 Nov 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 28 04:45:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

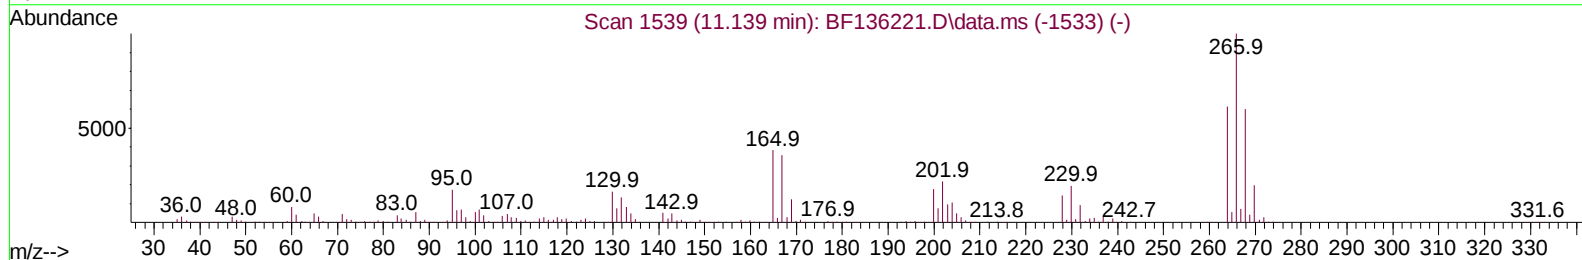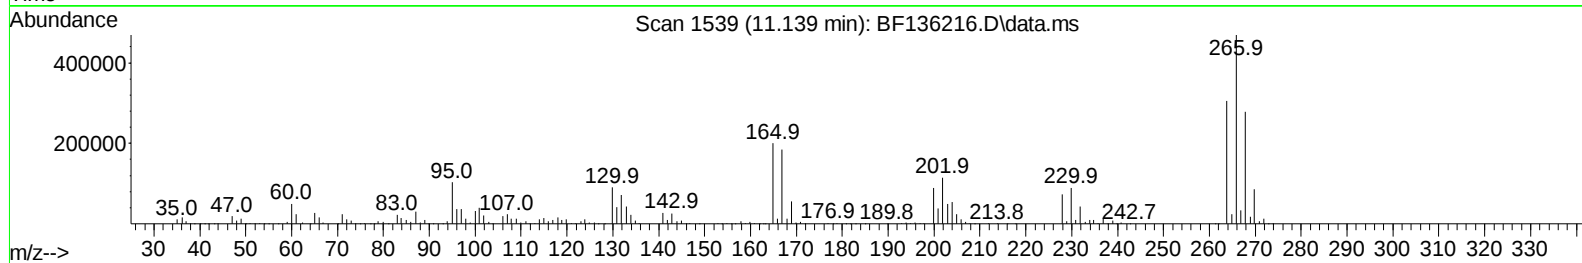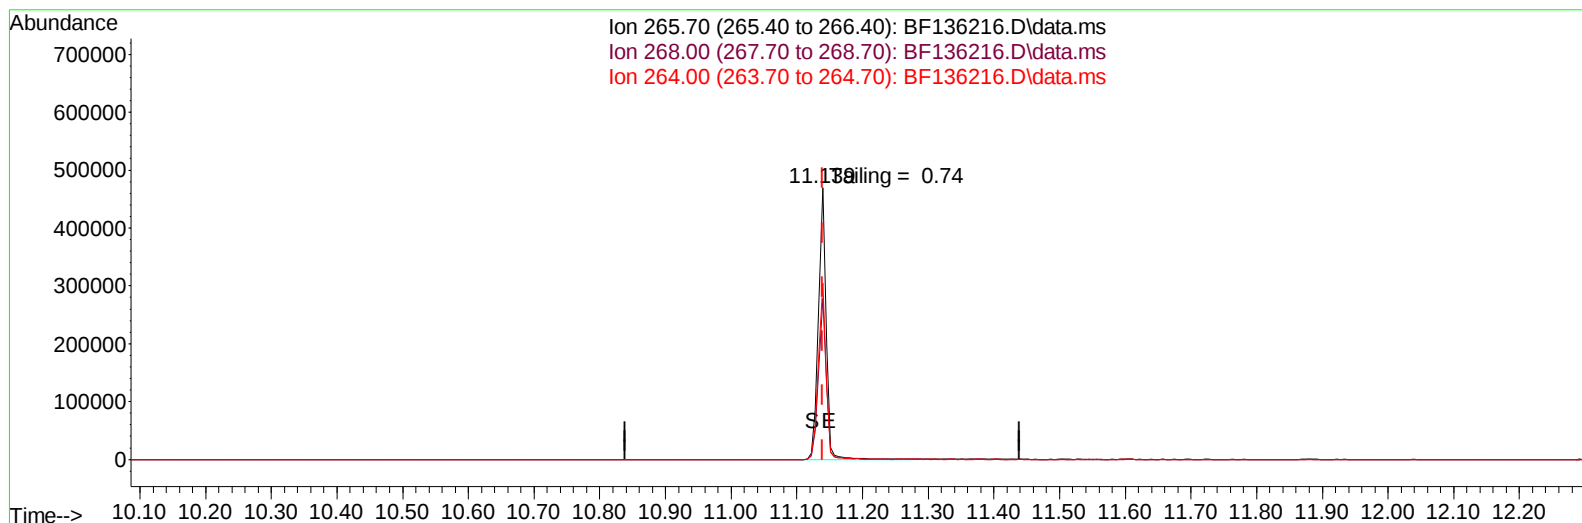

TIC: BF136216.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 86719.19 ng




response 391169

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	59.41
264.00	61.40	65.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112723\
 Data File : BF136216.D
 Acq On : 27 Nov 2023 11:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 28 04:45:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 28 03:04:20 2023
 Response via : Initial Calibration

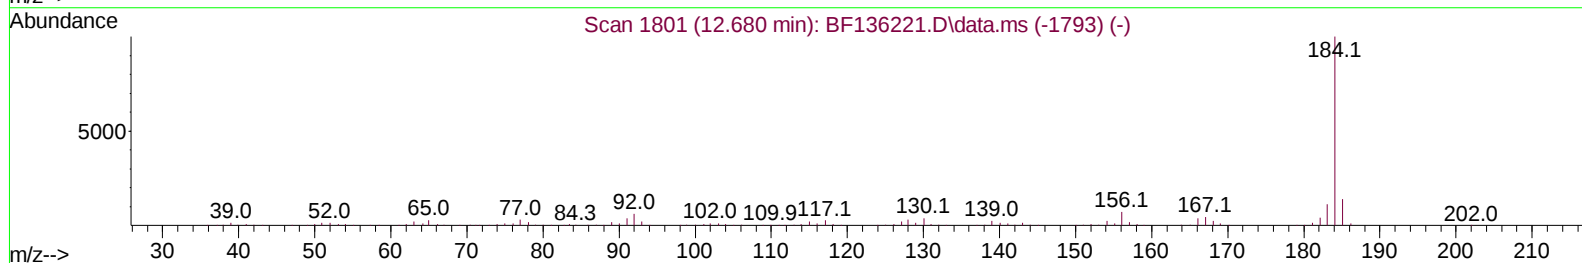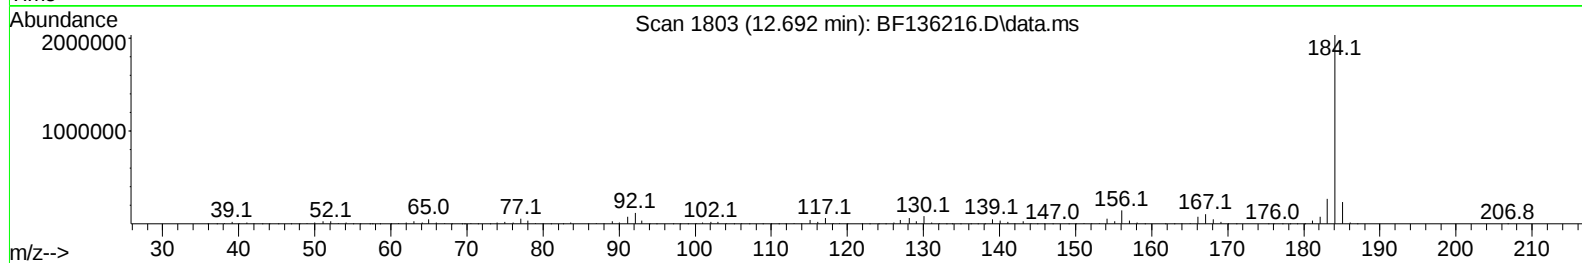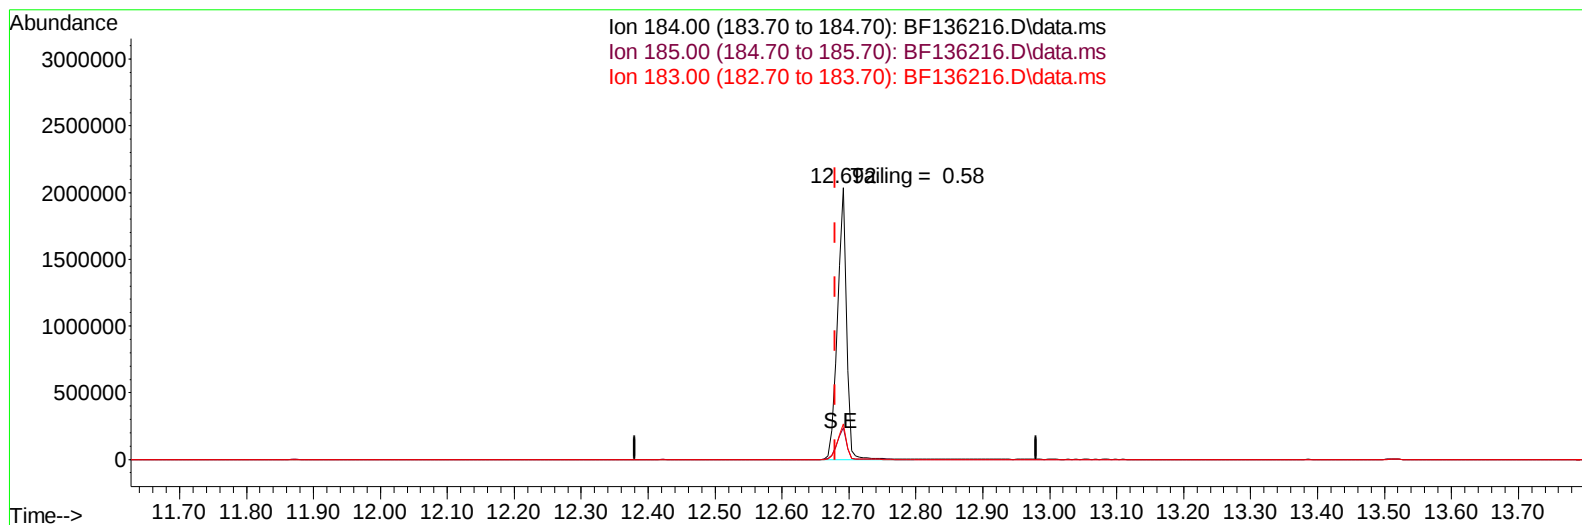

TIC: BF136216.D\data.ms

(77) Benzidine

12.692min (+ 0.012) 16125.67 ng

response 1873836

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	11.70
183.00	11.20	13.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/27/2023	BNA_F	<u>BF136216.D</u>
Compound Name	Response	Retention Time
DDT	949180	13.515
DDD	10991	13.245
DDE	538	12.421
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11529	960709	1.20

Instrument :
BNA_F
ClientSampleId :
DFTPP