
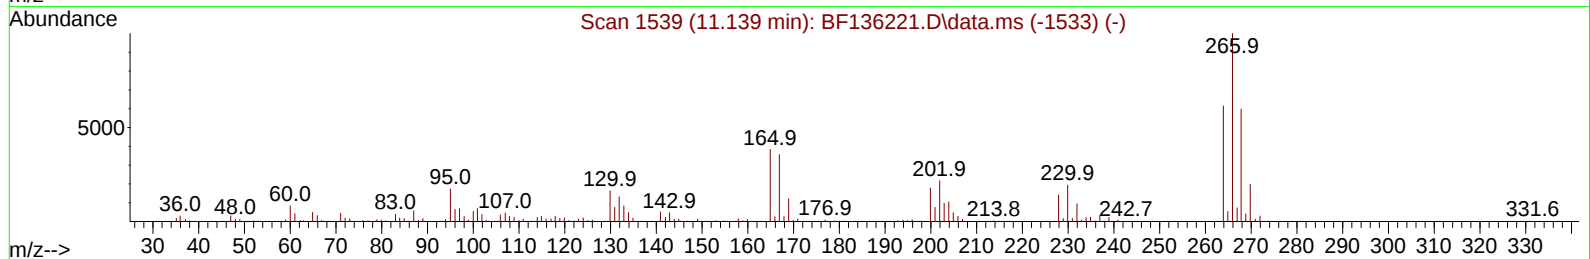
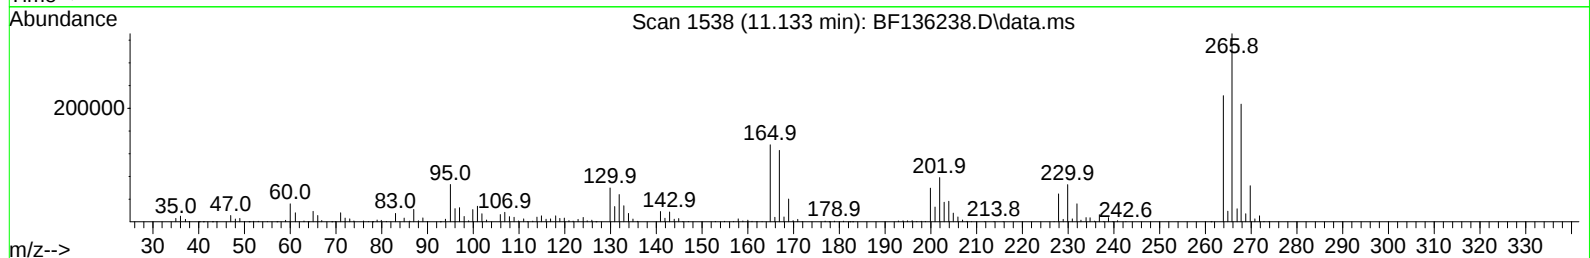


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136238.D
Acq On : 28 Nov 2023 09:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 12:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

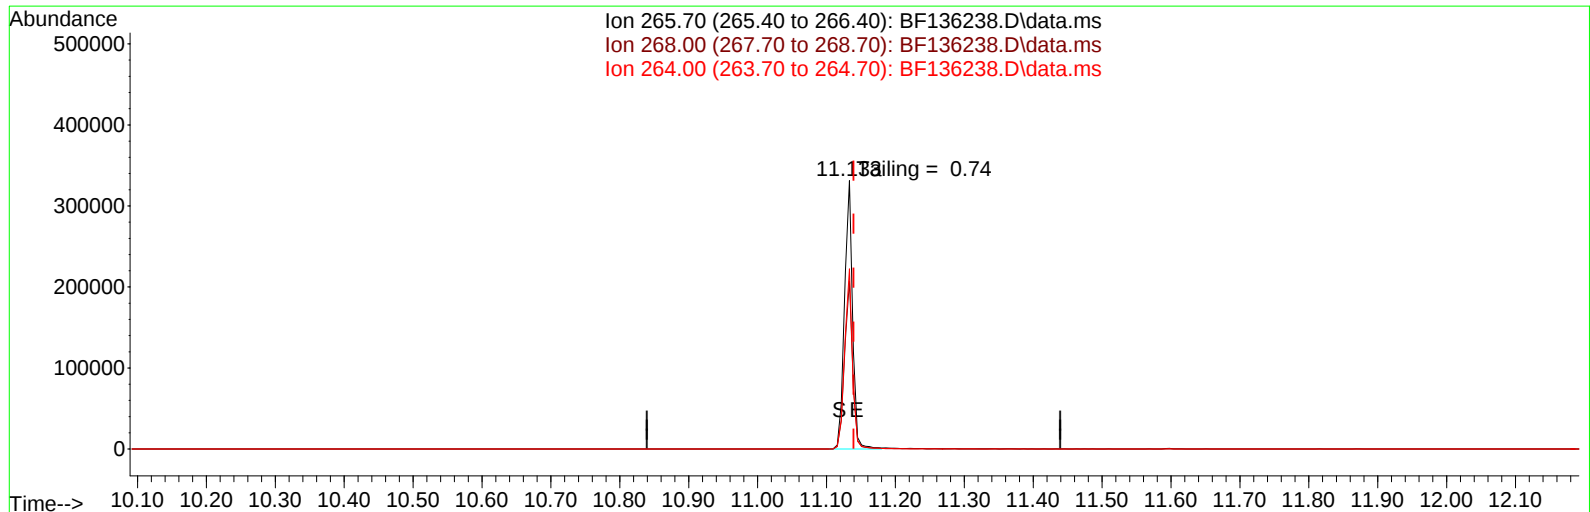

TIC: BF136238.D\data.ms

(70) Pentachlorophenol (C)




11.133min (-0.006) 52867.34 ng m

response 269138

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	62.60
264.00	61.40	67.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136238.D
Acq On : 28 Nov 2023 09:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 12:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

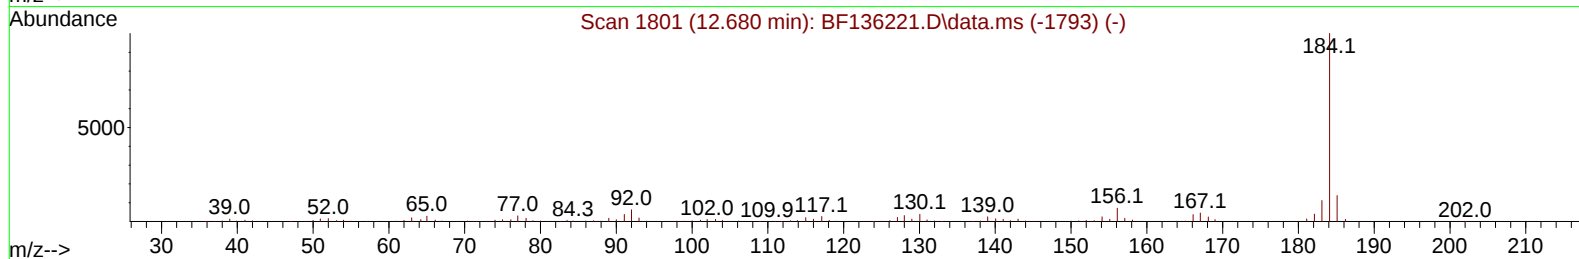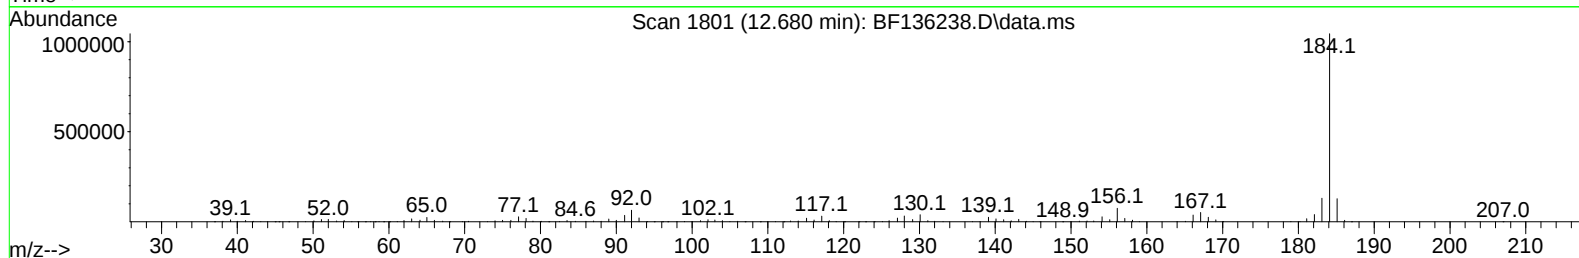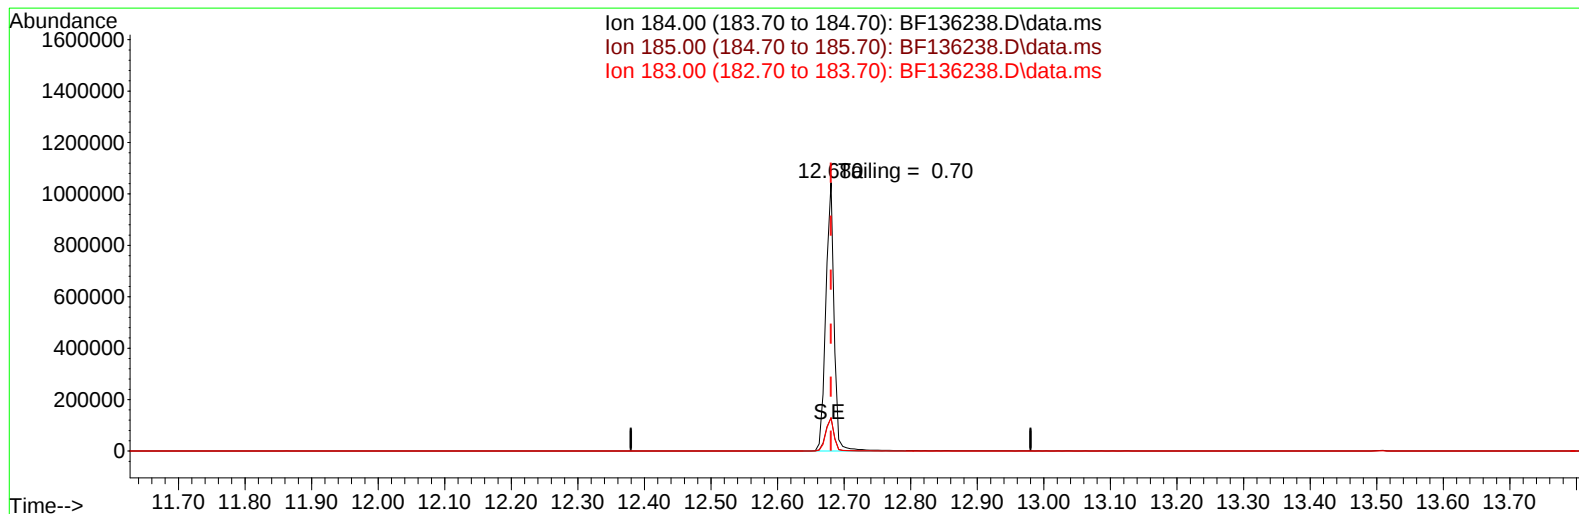

TIC: BF136238.D\data.ms

(77) Benzidine

12.680min (+ 0.000) 97737.15 ng

response 899712

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	12.29
183.00	11.20	12.50
0.00	0.00	0.00