

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
 Data File : BF136247.D
 Acq On : 28 Nov 2023 14:04
 Operator : CG\JU
 Sample : PB156974BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156974BL

Quant Time: Nov 28 15:01:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 28 03:04:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.804	152	145196	20.000	ng	0.00
21) Naphthalene-d8	8.081	136	615427	20.000	ng	0.00
39) Acenaphthene-d10	9.839	164	316787	20.000	ng	0.00
64) Phenanthrene-d10	11.327	188	606907	20.000	ng	0.00
76) Chrysene-d12	13.980	240	332436	20.000	ng	-0.01
86) Perylene-d12	15.463	264	262932	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.451	112	1390184	133.263	ng	0.01
7) Phenol-d6	6.440	99	1712135	131.262	ng	0.00
23) Nitrobenzene-d5	7.363	82	1041979	89.469	ng	-0.01
42) 2,4,6-Tribromophenol	10.633	330	519179	134.051	ng	0.00
45) 2-Fluorobiphenyl	9.163	172	2158478	87.031	ng	0.00
79) Terphenyl-d14	12.933	244	2495742	86.597	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136247.D
Acq On : 28 Nov 2023 14:04
Operator : CG\JU
Sample : PB156974BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156974BL

Quant Time: Nov 28 15:01:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration




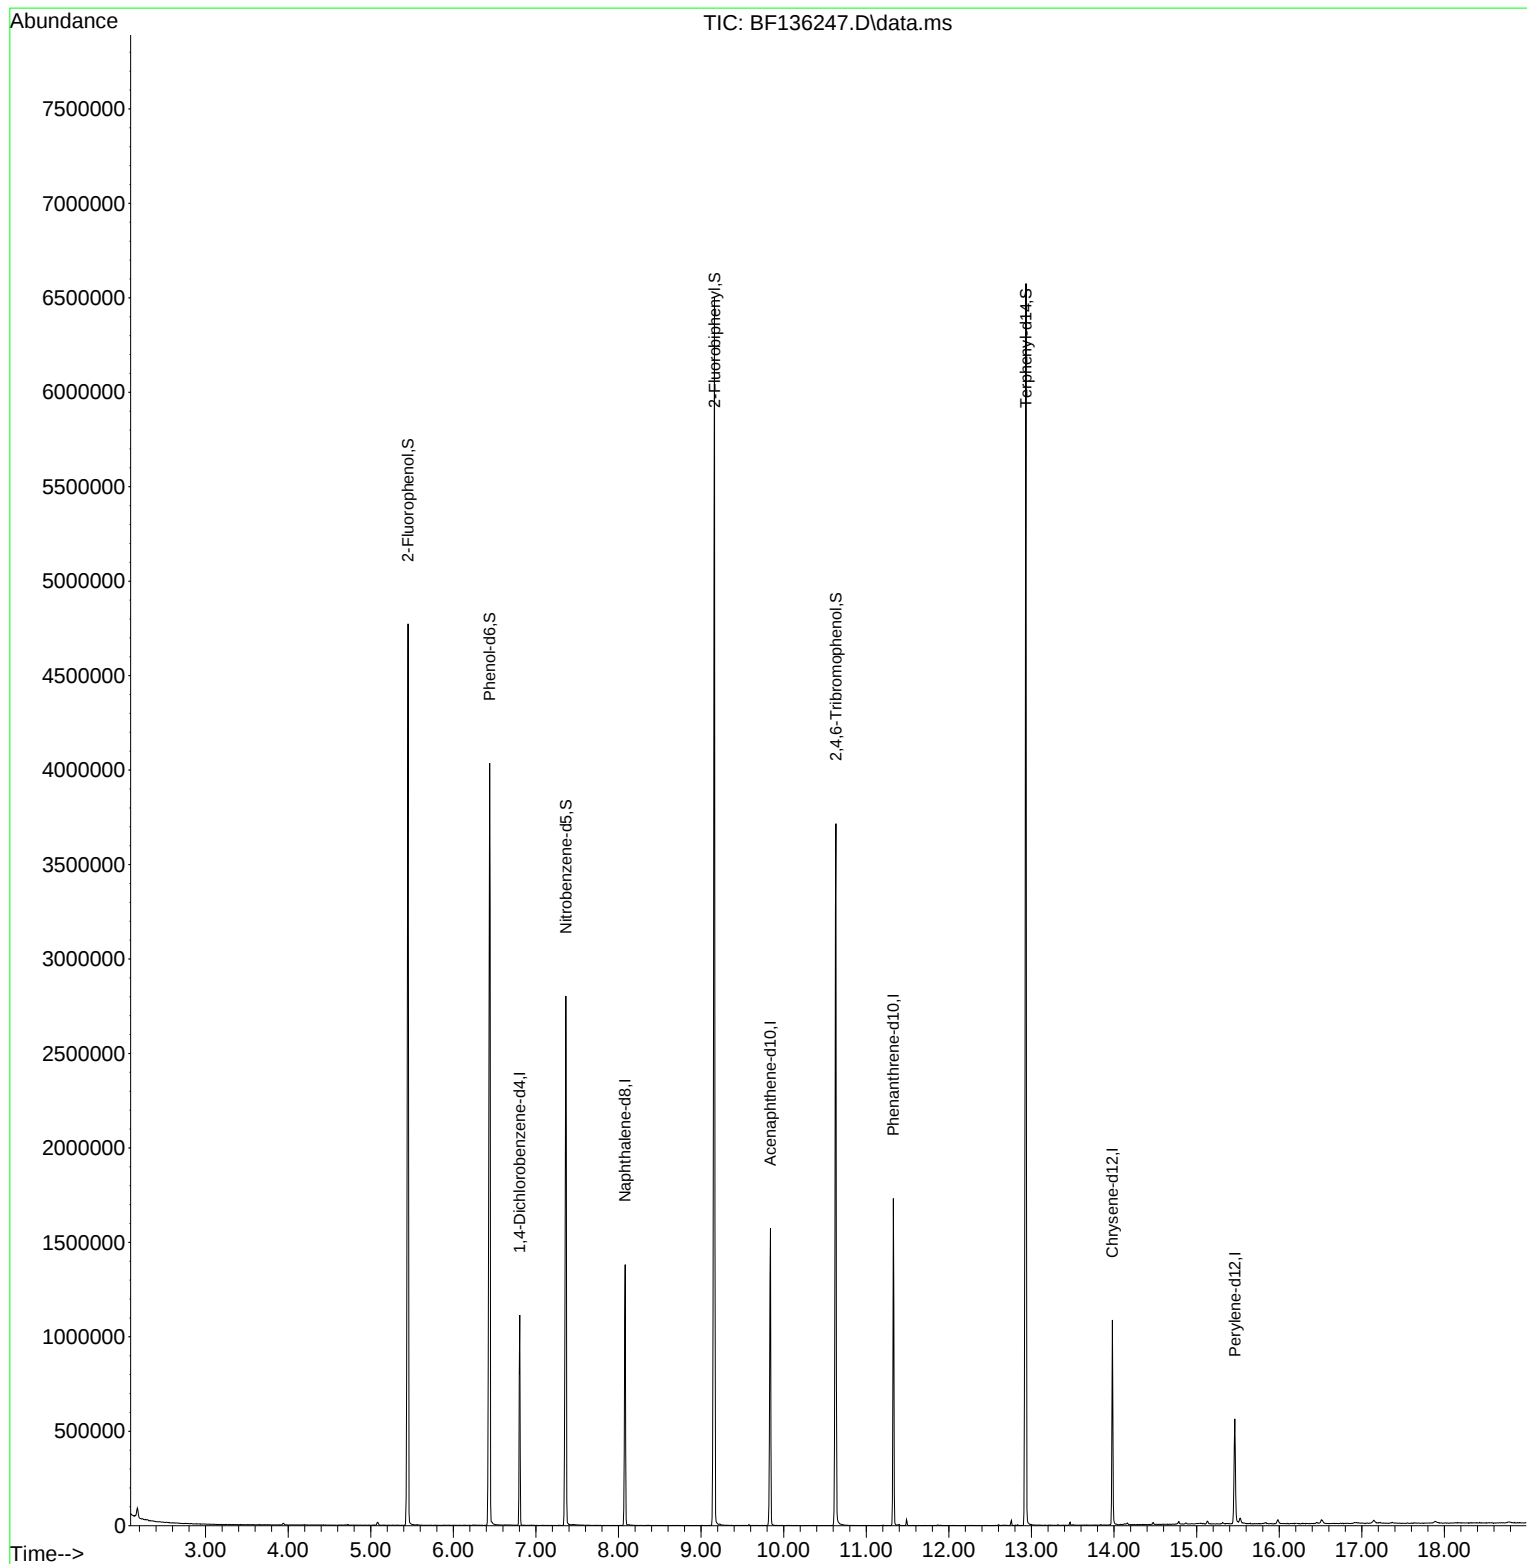


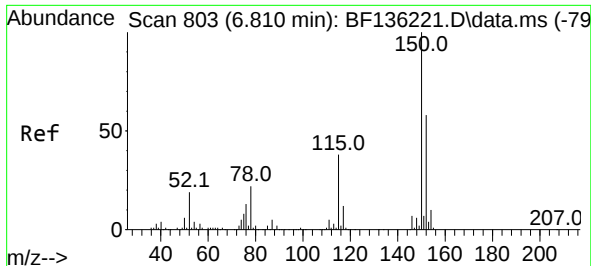

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.804 min Scan# 803
Delta R.T. -0.006 min
Lab File: BF136247.D
Acq: 28 Nov 2023 14:04




Instrument :
BNA_F
ClientSampleId :
PB156974BL


Tgt Ion:152 Resp: 145196
Ion Ratio Lower Upper
152 100
150 167.8 137.8 206.8
115 65.0 52.7 79.1

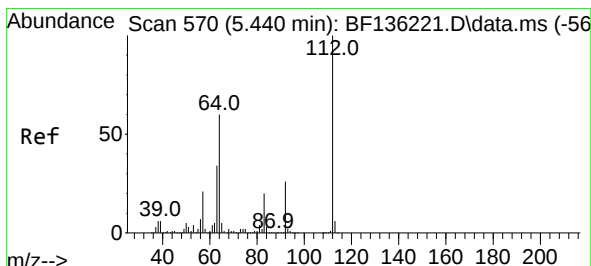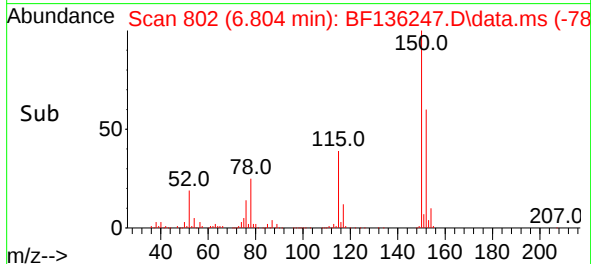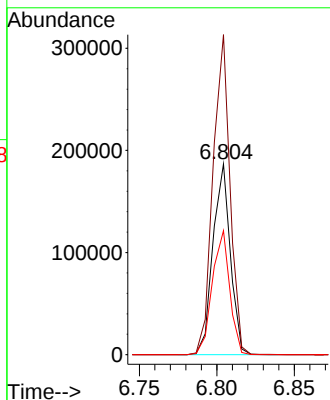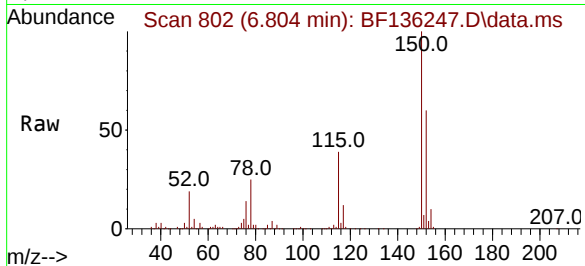

#5
2-Fluorophenol
Concen: 133.263 ng
RT: 5.451 min Scan# 572
Delta R.T. 0.012 min
Lab File: BF136247.D
Acq: 28 Nov 2023 14:04

Tgt Ion:112 Resp: 1390184
Ion Ratio Lower Upper
112 100
64 61.4 48.2 72.4
63 34.3 27.0 40.6


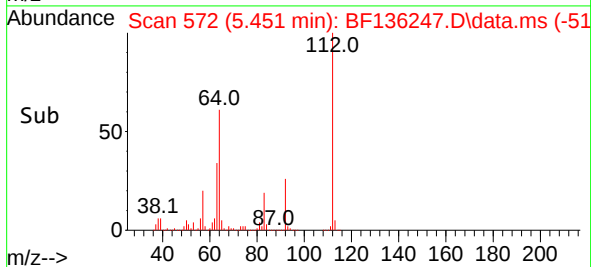
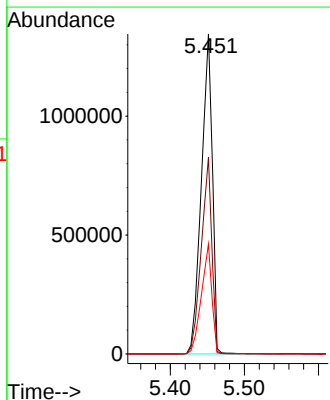
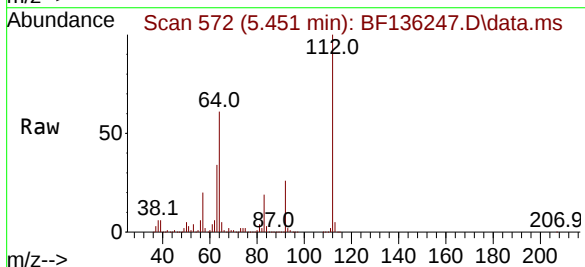


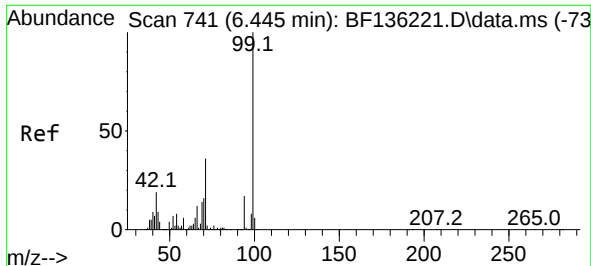

#7
Phenol-d6
Concen: 131.262 ng
RT: 6.440 min Scan# 741
Delta R.T. -0.006 min
Lab File: BF136247.D
Acq: 28 Nov 2023 14:04




Instrument :
BNA_F
ClientSampleId :
PB156974BL


Tgt Ion: 99 Resp: 1712135
Ion Ratio Lower Upper
99 100
42 17.9 15.0 22.6
71 35.5 28.9 43.3

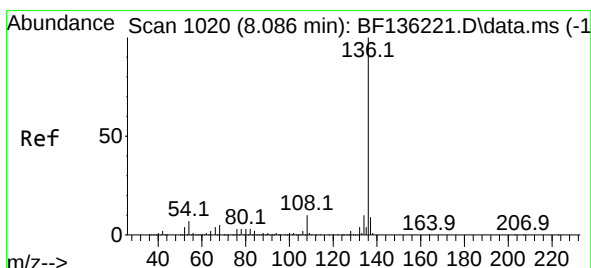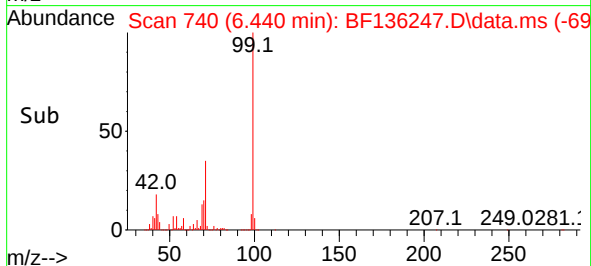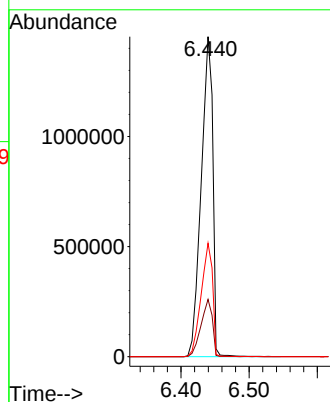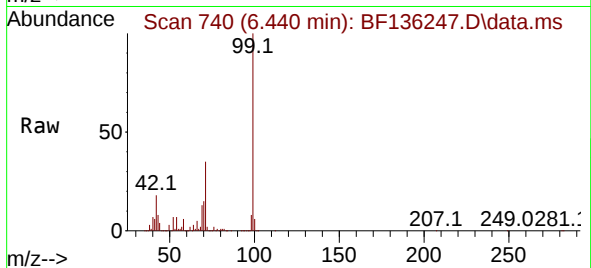

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.081 min Scan# 1019
Delta R.T. -0.006 min
Lab File: BF136247.D
Acq: 28 Nov 2023 14:04

Tgt Ion: 136 Resp: 615427
Ion Ratio Lower Upper
136 100
137 10.0 7.4 11.2
54 7.1 5.5 8.3
68 4.7 3.7 5.5

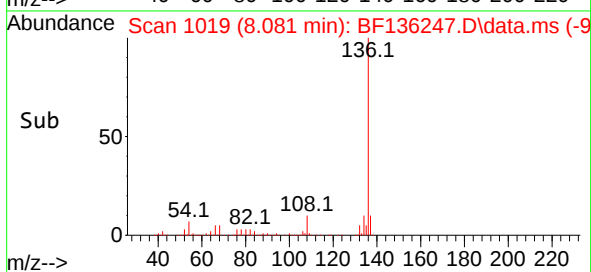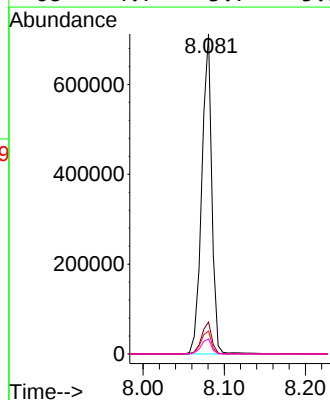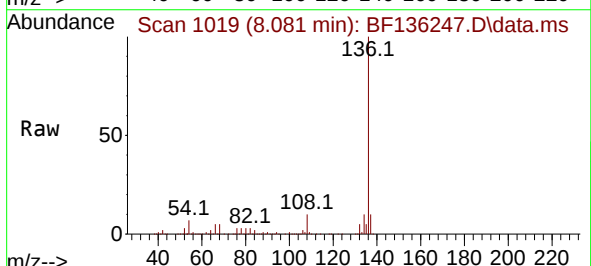

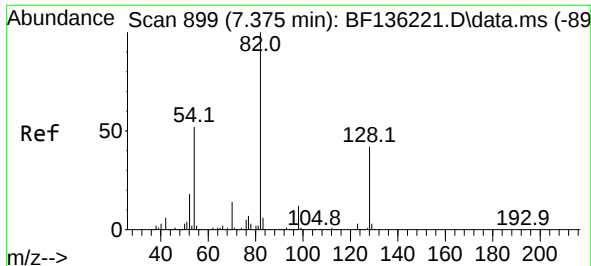

#23

Nitrobenzene-d5

Concen: 89.469 ng

RT: 7.363 min Scan# 89

Delta R.T. -0.012 min

Lab File: BF136247.D


Acq: 28 Nov 2023 14:04

Instrument :

BNA_F

ClientSampleId :

PB156974BL

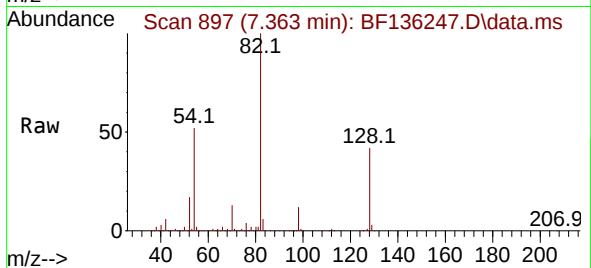




Tgt Ion: 82 Resp: 1041979

Ion Ratio Lower Upper

82 100

128 41.7 33.4 50.2

54 52.0 41.7 62.5

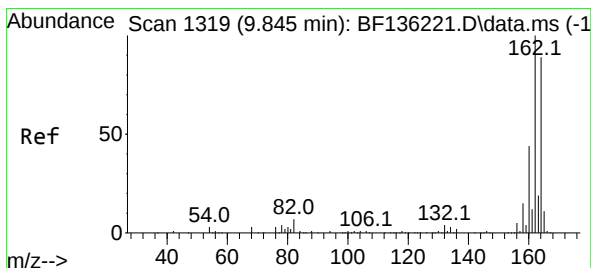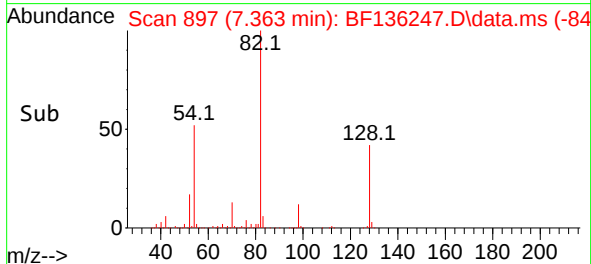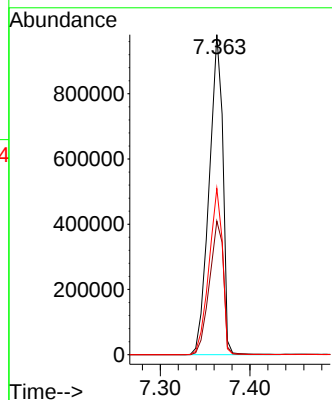

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.839 min Scan# 1318

Delta R.T. -0.006 min

Lab File: BF136247.D

Acq: 28 Nov 2023 14:04




Tgt Ion:164 Resp: 316787


Ion Ratio Lower Upper

164 100

162 110.8 89.5 134.3

160 51.4 39.6 59.4

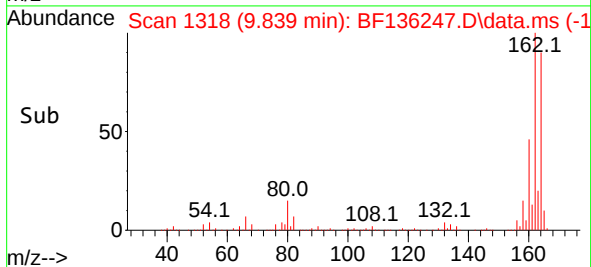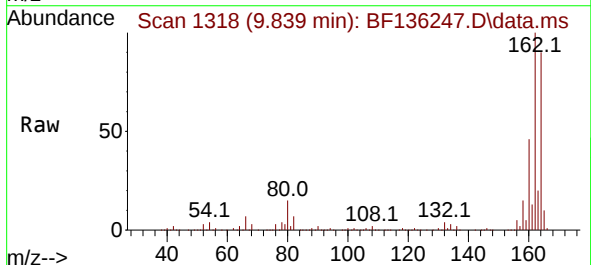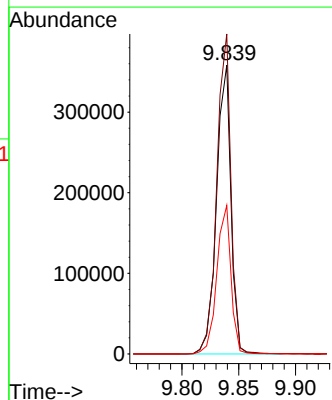

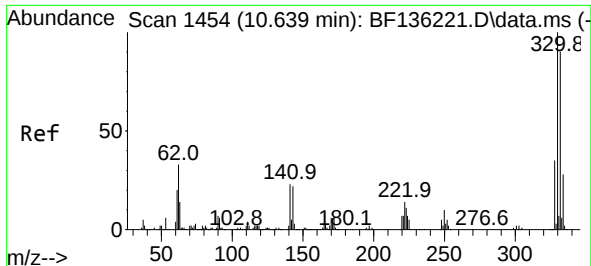

#42

2,4,6-Tribromophenol

Concen: 134.051 ng

RT: 10.633 min Scan# 1454

Delta R.T. -0.006 min

Lab File: BF136247.D

Acq: 28 Nov 2023 14:04

Instrument :

BNA_F

ClientSampleId :

PB156974BL





Tgt Ion:330 Resp: 519179

Ion Ratio Lower Upper

330 100

332 90.9 73.0 109.6

141 29.3 24.2 36.2

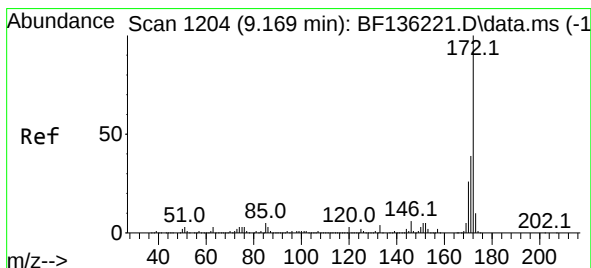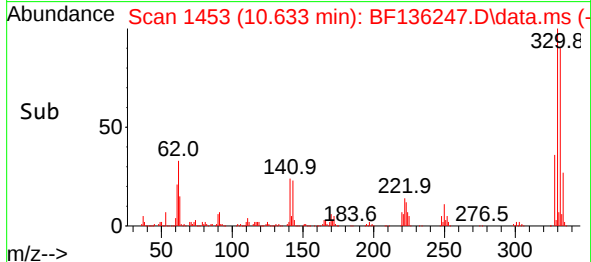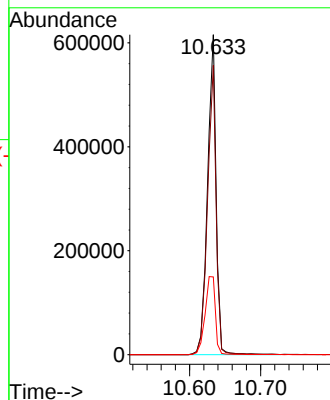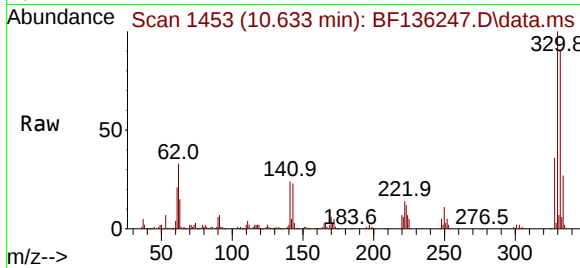

#45

2-Fluorobiphenyl

Concen: 87.031 ng

RT: 9.163 min Scan# 1203

Delta R.T. -0.006 min

Lab File: BF136247.D

Acq: 28 Nov 2023 14:04




Tgt Ion:172 Resp: 2158478


Ion Ratio Lower Upper

172 100

171 39.6 31.5 47.3

170 26.5 20.8 31.2


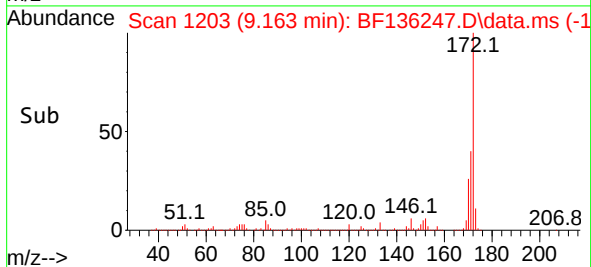
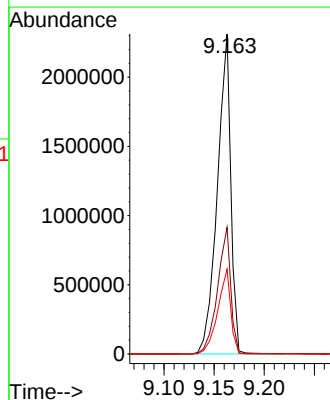
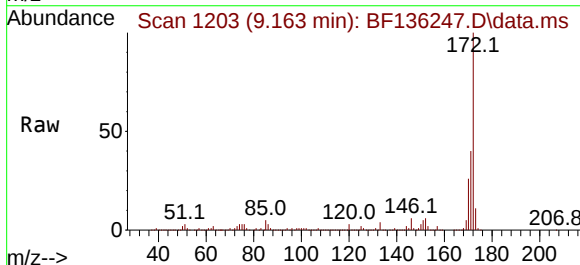


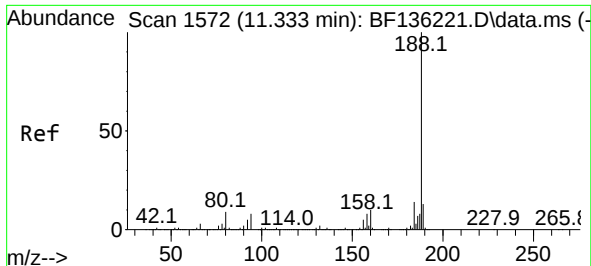

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.327 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF136247.D
Acq: 28 Nov 2023 14:04




Instrument :
BNA_F
ClientSampleId :
PB156974BL


Tgt Ion:188 Resp: 606907
Ion Ratio Lower Upper
188 100
94 8.1 6.7 10.1
80 9.1 7.2 10.8

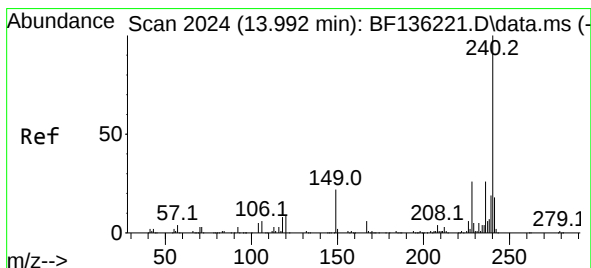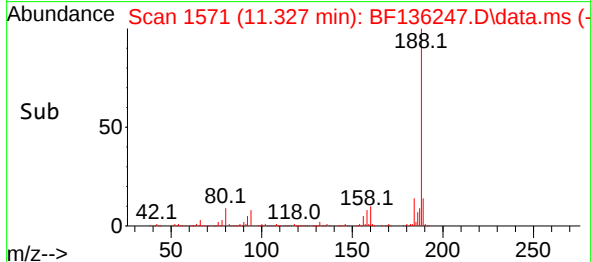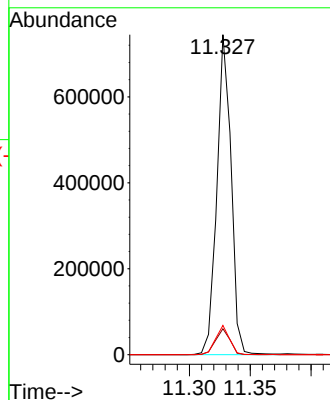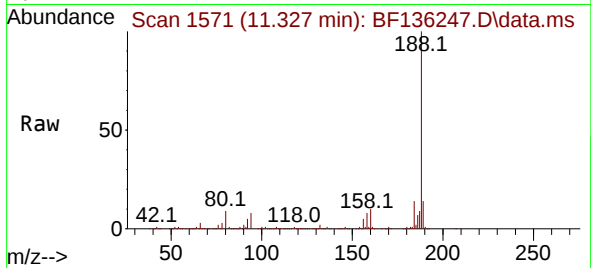

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.980 min Scan# 2022
Delta R.T. -0.012 min
Lab File: BF136247.D
Acq: 28 Nov 2023 14:04

Tgt Ion:240 Resp: 332436
Ion Ratio Lower Upper
240 100
120 9.9 7.4 11.2
236 26.2 21.1 31.7


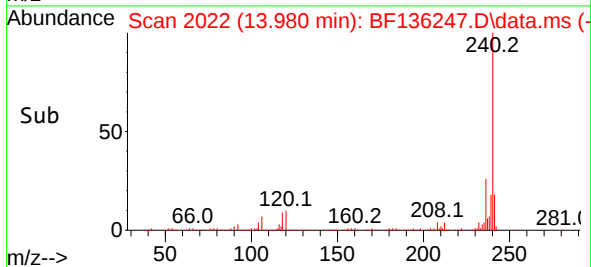
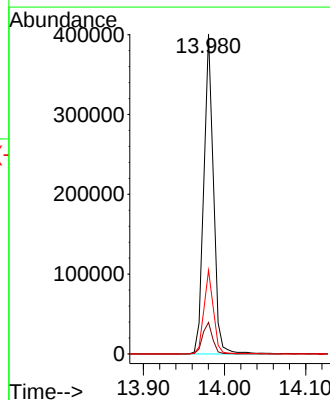
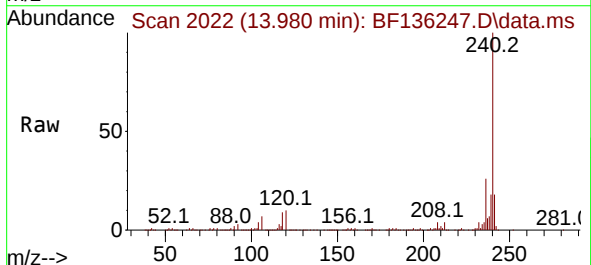


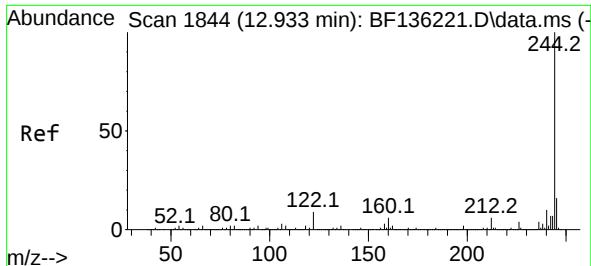

#79
 Terphenyl-d14
 Concen: 86.597 ng
 RT: 12.933 min Scan# 1844
 Delta R.T. 0.000 min
 Lab File: BF136247.D
 Acq: 28 Nov 2023 14:04

Instrument :
 BNA_F
 ClientSampleId :
 PB156974BL

Tgt Ion:244 Resp: 2495742
 Ion Ratio Lower Upper
 244 100
 212 5.7 4.6 7.0
 122 8.2 7.3 10.9

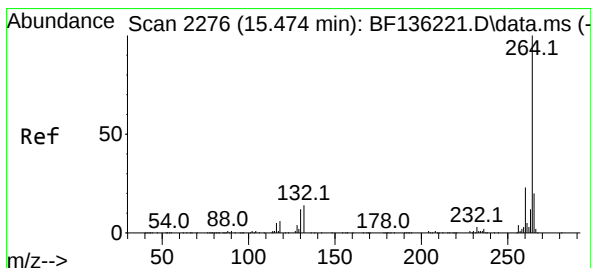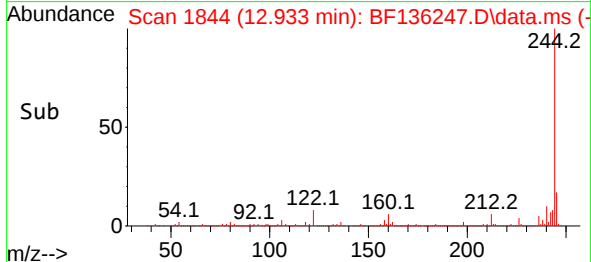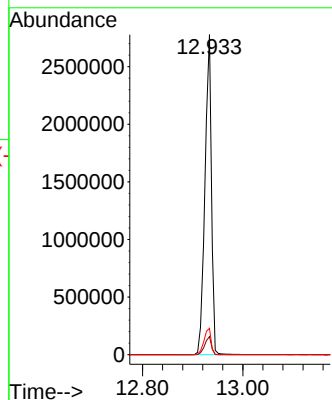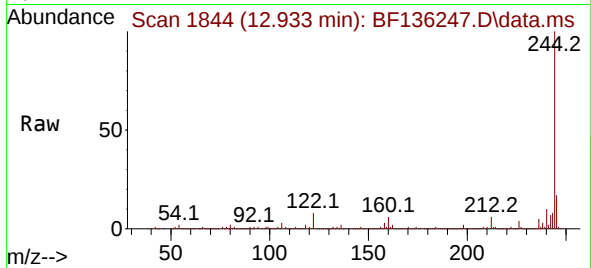

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.463 min Scan# 2274
 Delta R.T. -0.011 min
 Lab File: BF136247.D
 Acq: 28 Nov 2023 14:04

Tgt Ion:264 Resp: 262932
 Ion Ratio Lower Upper
 264 100
 260 23.1 18.6 27.8
 265 20.0 15.7 23.5

