

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
 Data File : BF136240.D
 Acq On : 28 Nov 2023 10:19
 Operator : CG\JU
 Sample : PB157023BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157023BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	11	15	19	rVB	81290	107293	1.65%	0.294%
2	5.451	566	572	575	rBV	5107337	5064250	77.88%	13.880%
3	6.439	734	740	743	rBV	4032949	5052313	77.70%	13.847%
4	6.804	798	802	805	rBV	1177602	897920	13.81%	2.461%
5	7.363	891	897	900	rBV	2768048	3193251	49.11%	8.752%
6	8.081	1014	1019	1022	rBV	1382429	1233559	18.97%	3.381%
7	9.163	1196	1203	1206	rBV	7243913	6502442	100.00%	17.822%
8	9.839	1312	1318	1321	rBV	1638503	1430544	22.00%	3.921%
9	10.633	1446	1453	1456	rBV	4075293	3730153	57.37%	10.224%
10	11.327	1567	1571	1574	rBV	1796873	1438075	22.12%	3.942%
11	12.933	1839	1844	1847	rBV	6876969	6260559	96.28%	17.159%
12	13.980	2018	2022	2026	rBV	1082303	926581	14.25%	2.540%
13	15.462	2268	2274	2281	rBV	545927	648447	9.97%	1.777%




Sum of corrected areas: 36485387

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136240.D
Acq On : 28 Nov 2023 10:19
Operator : CG\JU
Sample : PB157023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157023BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

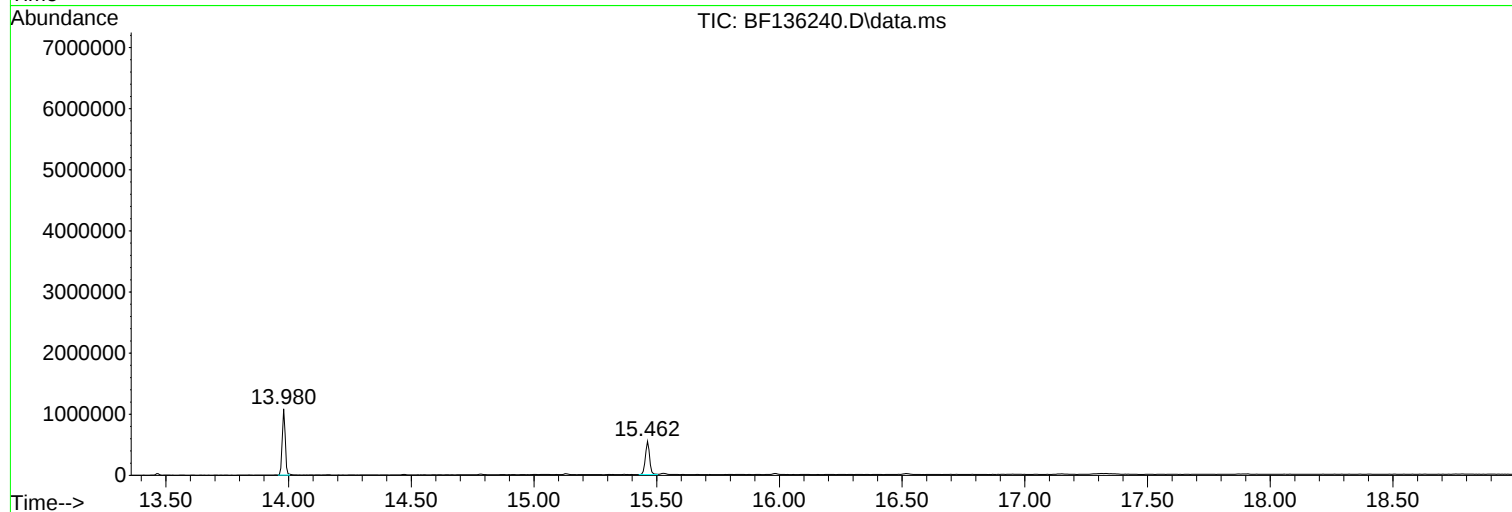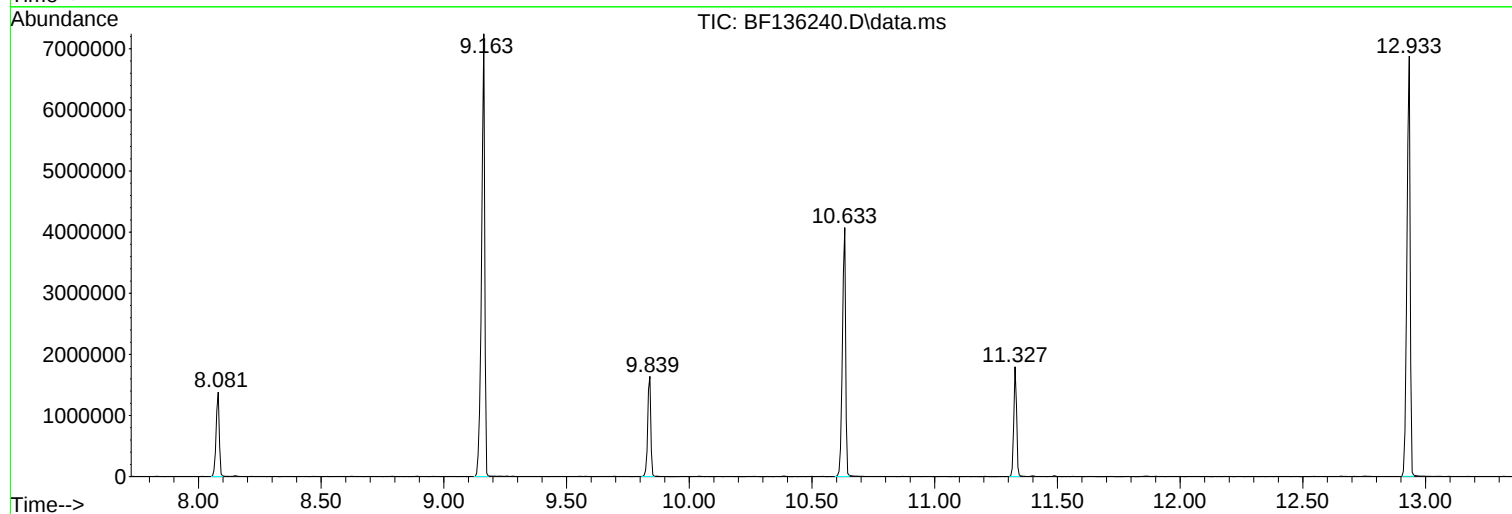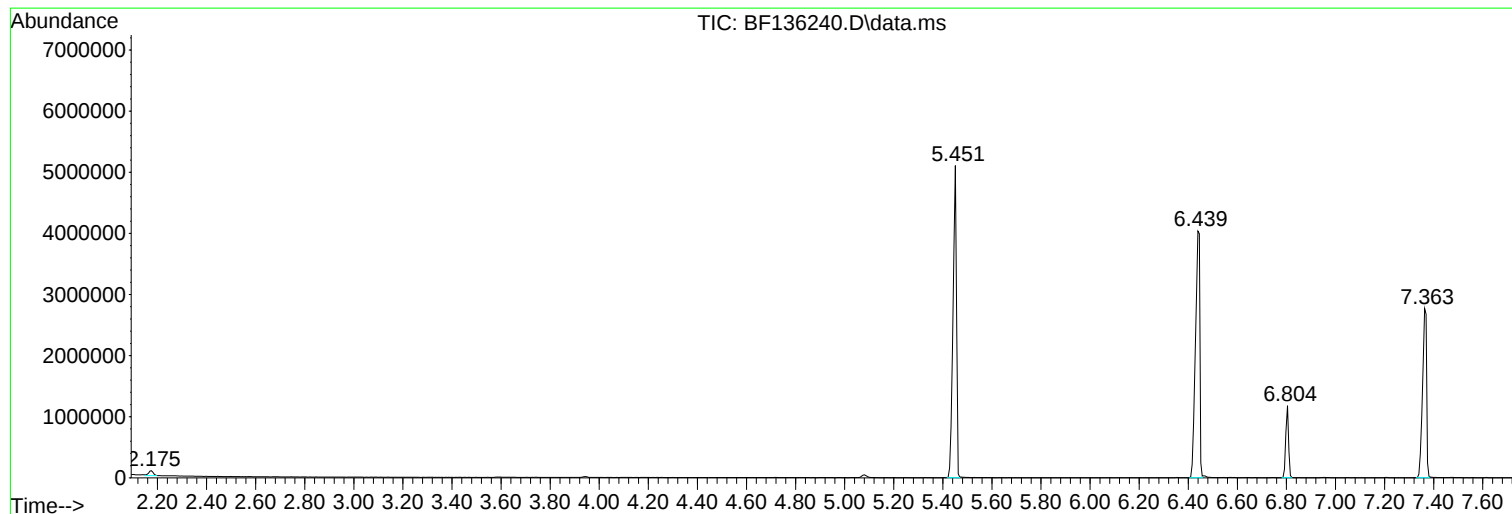

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136240.D
Acq On : 28 Nov 2023 10:19
Operator : CG\JU
Sample : PB157023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157023BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.175	2.39 ng	107293	1,4-Dichlorobenzene-d4	6.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	17
3			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	17
4			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	16
5			Boronic acid, ethyl-, dimethyl e...	102	C4H11BO2	007318-82-3	10

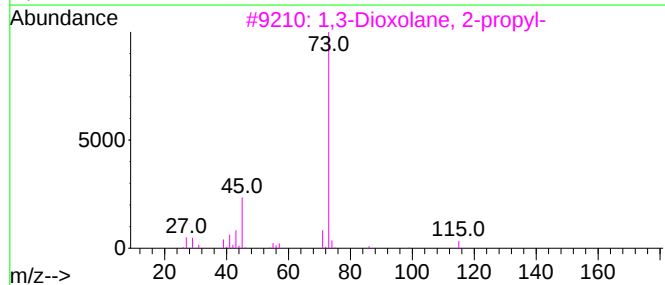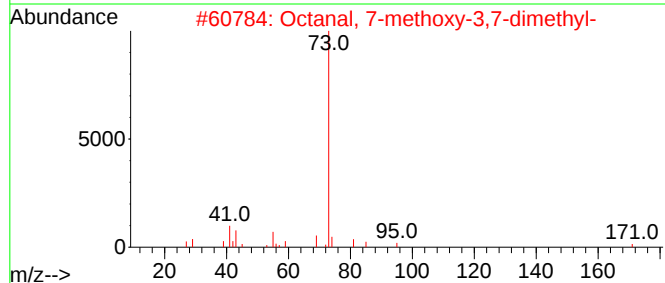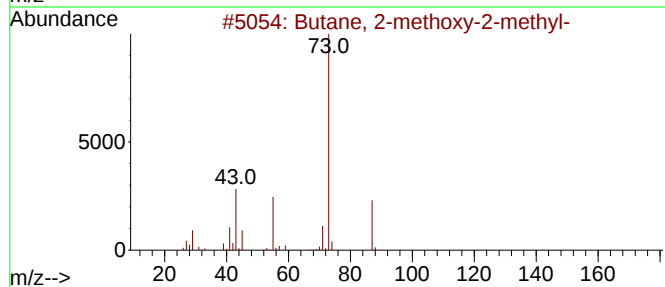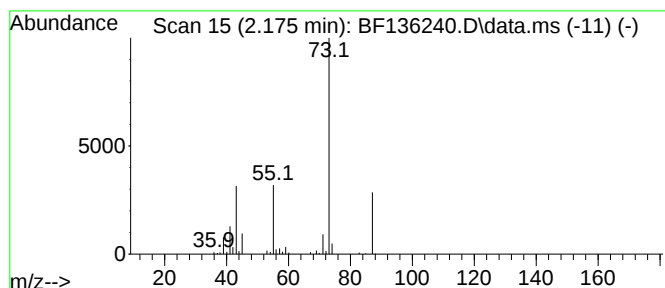

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136240.D
Acq On : 28 Nov 2023 10:19
Operator : CG\JU
Sample : PB157023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157023BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.175	2.4	ng	107293	1	6.804	897920	20.0