

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
 Data File : BF136242.D
 Acq On : 28 Nov 2023 11:23
 Operator : CG\JU
 Sample : PB157019BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157019BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	10	14	23	rVB	89273	133078	2.07%	0.372%
2	5.451	566	572	575	rBV	5018305	4974827	77.26%	13.901%
3	6.440	734	740	743	rBV	4028509	4942915	76.76%	13.812%
4	6.804	798	802	805	rBV	1148069	888556	13.80%	2.483%
5	7.363	891	897	900	rBV	2876762	3136850	48.71%	8.765%
6	8.081	1014	1019	1022	rBV	1339453	1211041	18.81%	3.384%
7	9.163	1197	1203	1206	rBV	6917646	6439318	100.00%	17.993%
8	9.839	1312	1318	1321	rBV	1628272	1409336	21.89%	3.938%
9	10.634	1446	1453	1456	rBV	3991477	3640361	56.53%	10.172%
10	11.328	1567	1571	1575	rBV	1753630	1410705	21.91%	3.942%
11	12.933	1839	1844	1847	rBV	6628465	6048145	93.93%	16.900%
12	13.980	2018	2022	2037	rBV	1024181	895603	13.91%	2.503%
13	15.463	2268	2274	2282	rBV	509067	656423	10.19%	1.834%




Sum of corrected areas: 35787158

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136242.D
Acq On : 28 Nov 2023 11:23
Operator : CG\JU
Sample : PB157019BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157019BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

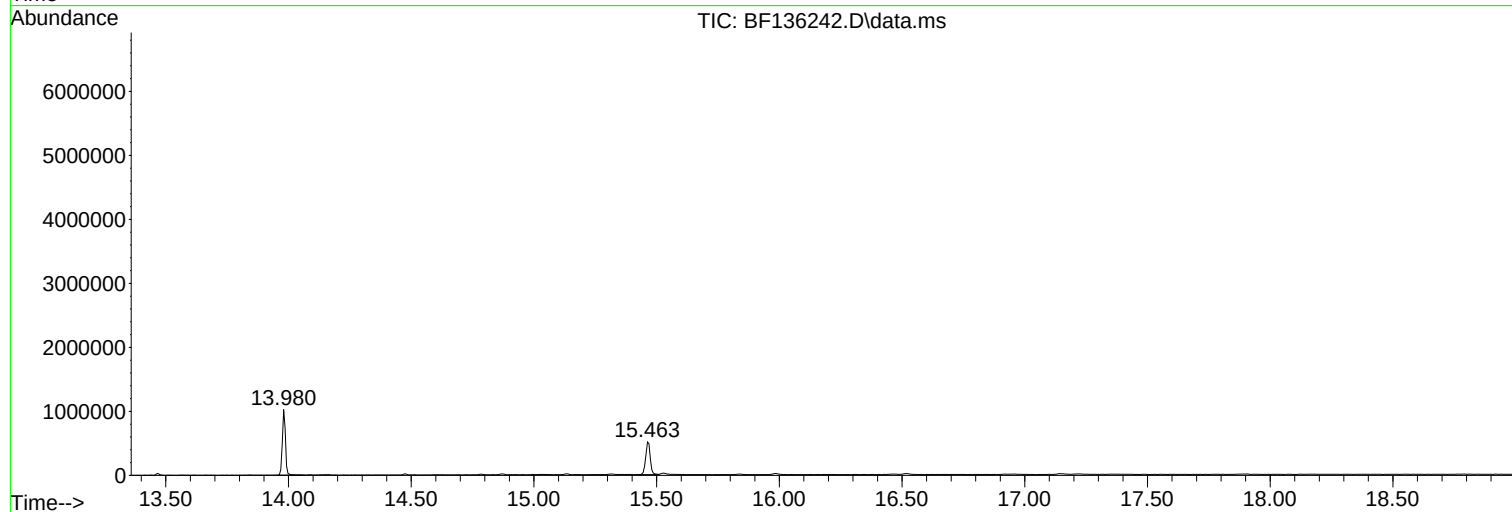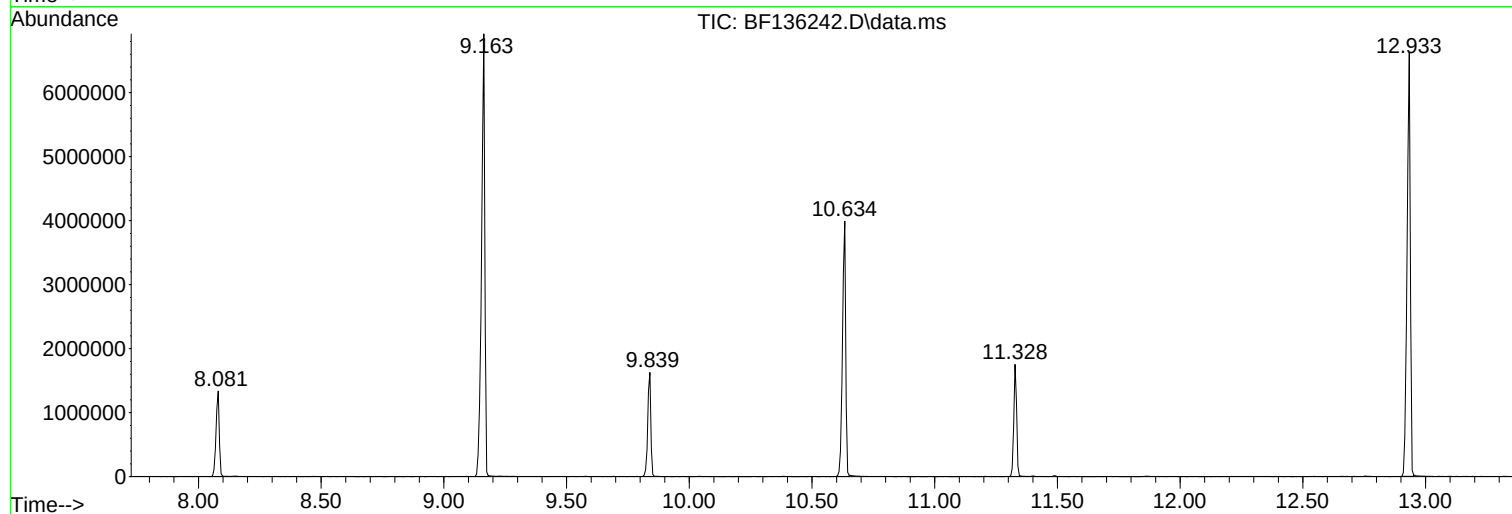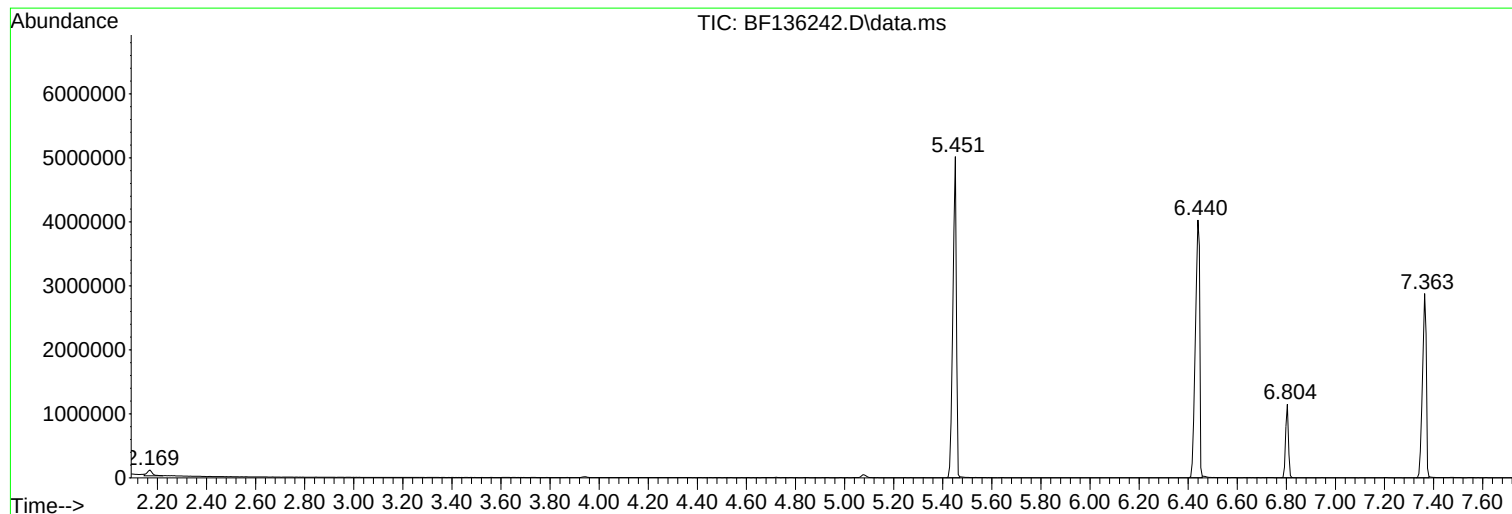

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136242.D
Acq On : 28 Nov 2023 11:23
Operator : CG\JU
Sample : PB157019BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157019BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.169	3.00 ng	133078	1,4-Dichlorobenzene-d4	6.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	64
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	25
4			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	25
5			1-(2-Methoxyethoxy)-2-methyl-2-p...	162	C8H18O3	1000364-24-4	25

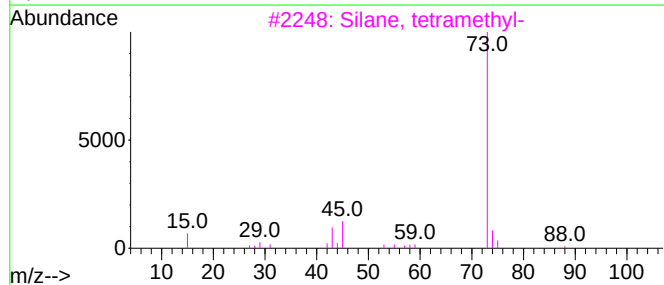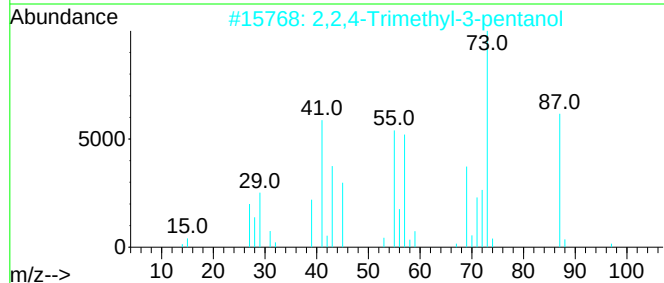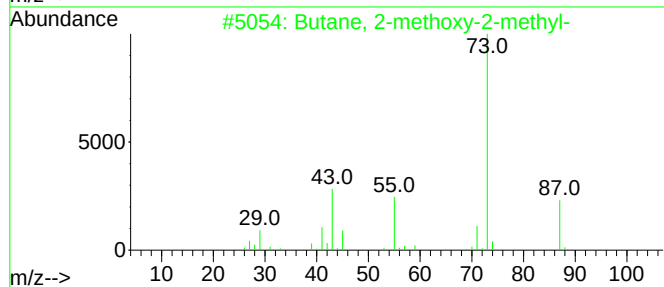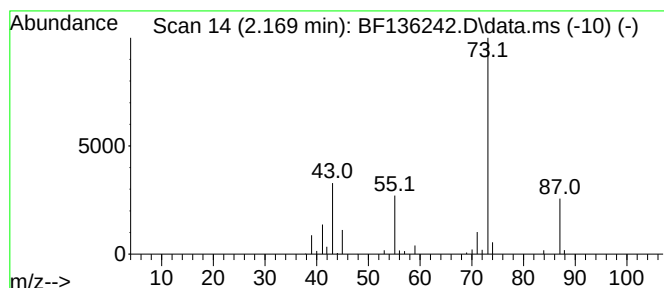

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136242.D
Acq On : 28 Nov 2023 11:23
Operator : CG\JU
Sample : PB157019BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157019BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.169	3.0	ng	133078	1	6.804	888556	20.0