

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136244.D
Acq On : 28 Nov 2023 12:27
Operator : CG\JU
Sample : PB156994TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156994TB

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	566	572	574	rBV	4251086	4596686	76.13%	13.844%
2	6.440	734	740	743	rBV	4026570	4492713	74.41%	13.531%
3	6.804	798	802	805	rBV	1121065	874015	14.48%	2.632%
4	7.363	891	897	900	rBV	2641618	2895503	47.96%	8.721%
5	8.081	1014	1019	1022	rBV	1351888	1201425	19.90%	3.618%
6	9.163	1196	1203	1206	rBV	6617393	6037798	100.00%	18.185%
7	9.839	1312	1318	1321	rBV	1614423	1400239	23.19%	4.217%
8	10.633	1446	1453	1456	rBV	3423124	3329466	55.14%	10.028%
9	11.328	1567	1571	1575	rBV	1645221	1390145	23.02%	4.187%
10	12.933	1839	1844	1847	rBV	6127421	5514344	91.33%	16.608%
11	13.980	2018	2022	2026	rBV	957426	829560	13.74%	2.498%
12	15.463	2268	2274	2281	rBV	518348	641043	10.62%	1.931%




Sum of corrected areas: 33202937

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136244.D
Acq On : 28 Nov 2023 12:27
Operator : CG\JU
Sample : PB156994TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156994TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

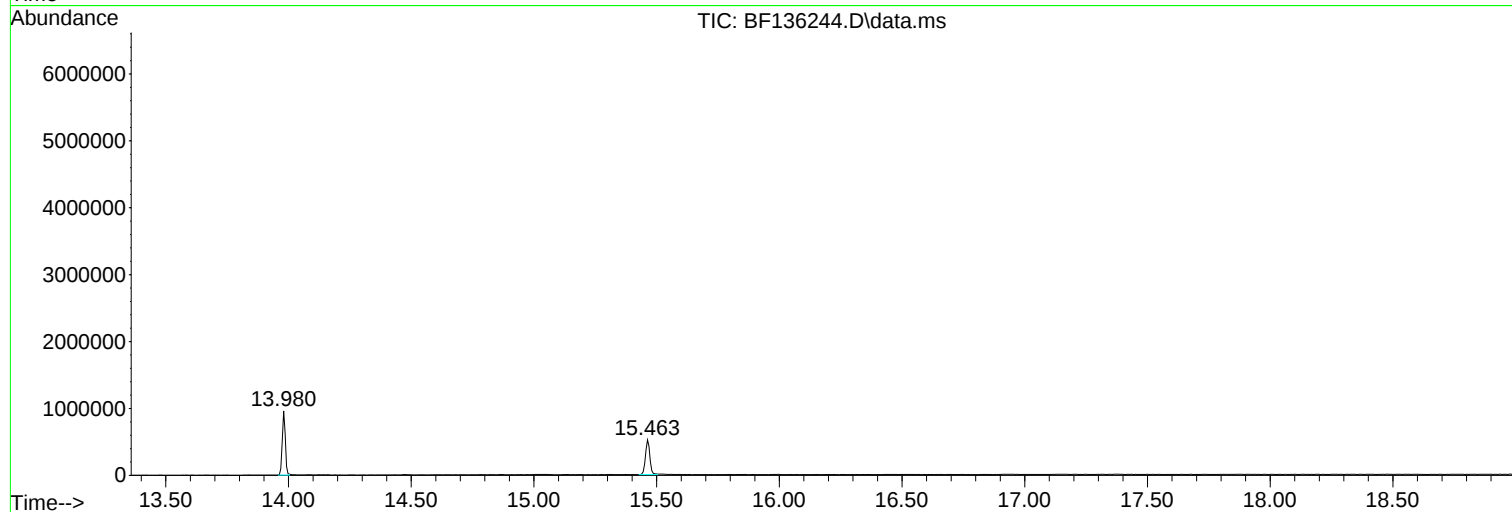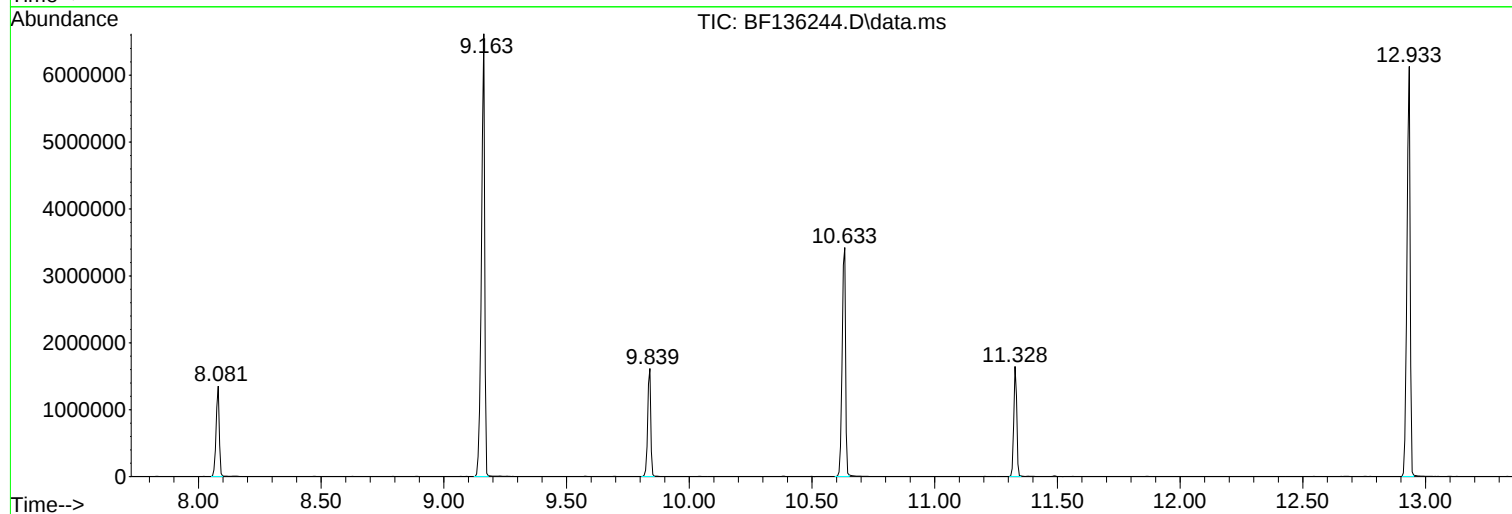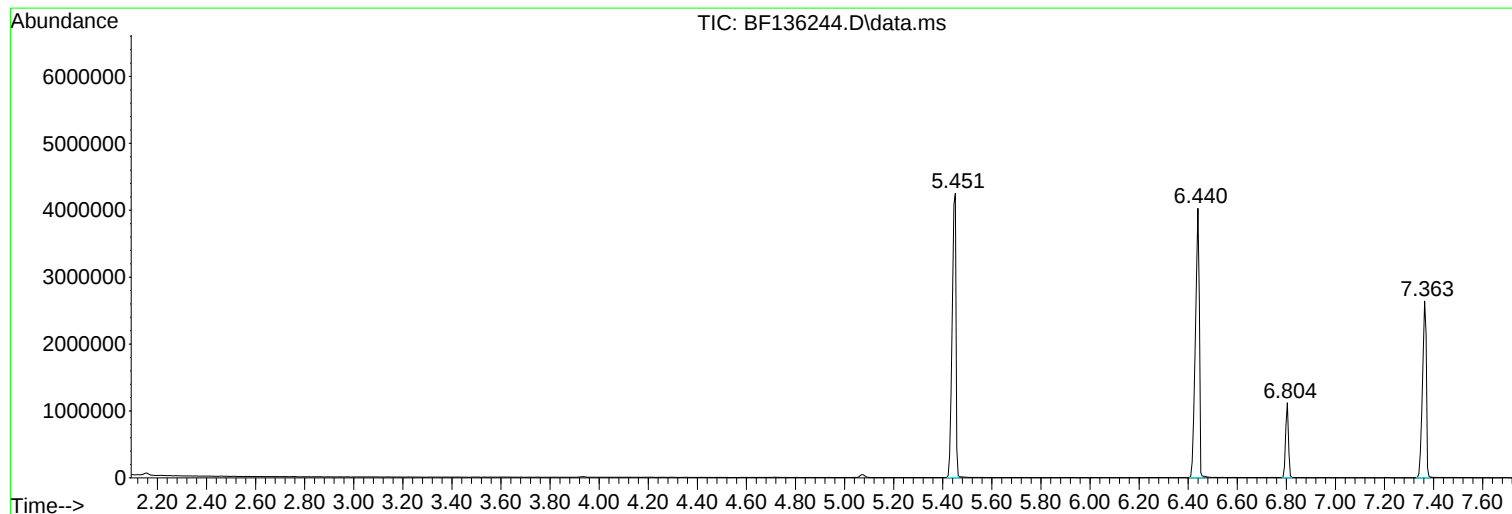

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136244.D
Acq On : 28 Nov 2023 12:27
Operator : CG\JU
Sample : PB156994TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156994TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136244.D
Acq On : 28 Nov 2023 12:27
Operator : CG\JU
Sample : PB156994TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156994TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------