

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
 Data File : BF136245.D
 Acq On : 28 Nov 2023 12:59
 Operator : CG\JU
 Sample : PB157271BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157271BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	504	508	516	rVB	49823	67430	1.11%	0.200%
2	5.451	566	572	575	rBV	4821535	4615179	75.78%	13.690%
3	6.439	734	740	743	rBV	3985522	4535271	74.47%	13.453%
4	6.804	798	802	805	rBV	1093457	844527	13.87%	2.505%
5	7.363	891	897	900	rBV	2621150	2948408	48.41%	8.746%
6	8.081	1014	1019	1022	rBV	1331898	1163828	19.11%	3.452%
7	9.163	1196	1203	1206	rBV	6608995	6090248	100.00%	18.066%
8	9.839	1312	1318	1321	rBV	1562127	1359011	22.31%	4.031%
9	10.633	1445	1453	1456	rBV	3751487	3416881	56.10%	10.136%
10	11.327	1567	1571	1575	rBV	1668232	1354652	22.24%	4.018%
11	12.933	1839	1844	1847	rBV	6690123	5822602	95.61%	17.272%
12	13.980	2018	2022	2026	rBV	981541	856815	14.07%	2.542%
13	15.462	2269	2274	2282	rBV	535298	636695	10.45%	1.889%




Sum of corrected areas: 33711547

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136245.D
Acq On : 28 Nov 2023 12:59
Operator : CG\JU
Sample : PB157271BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157271BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

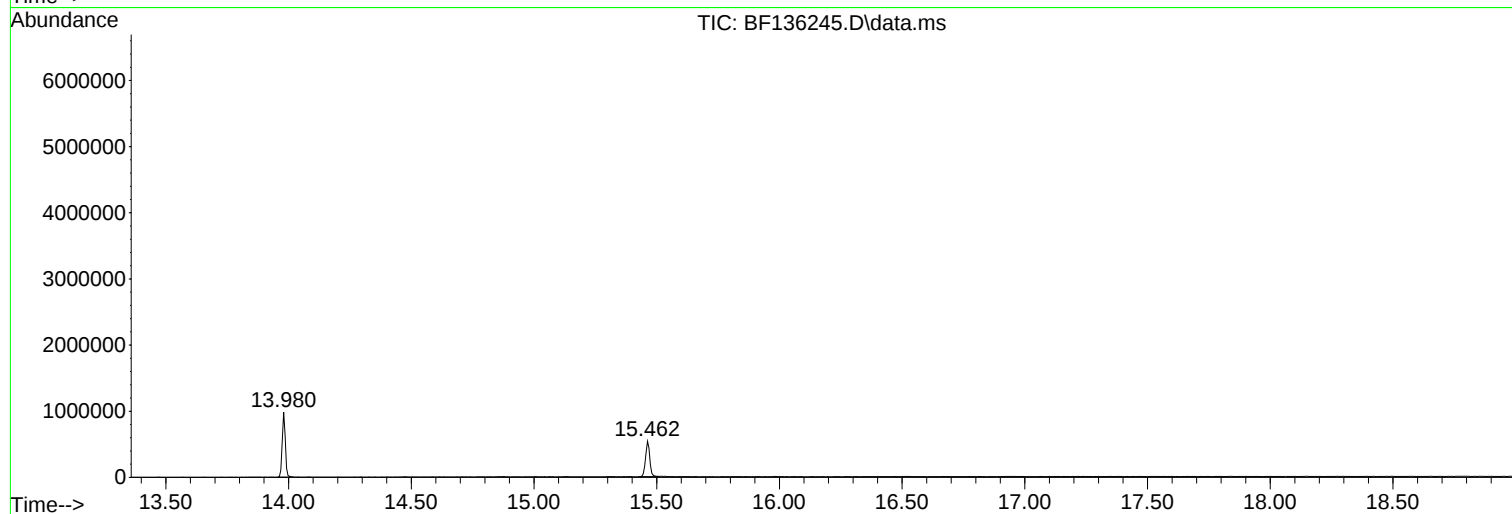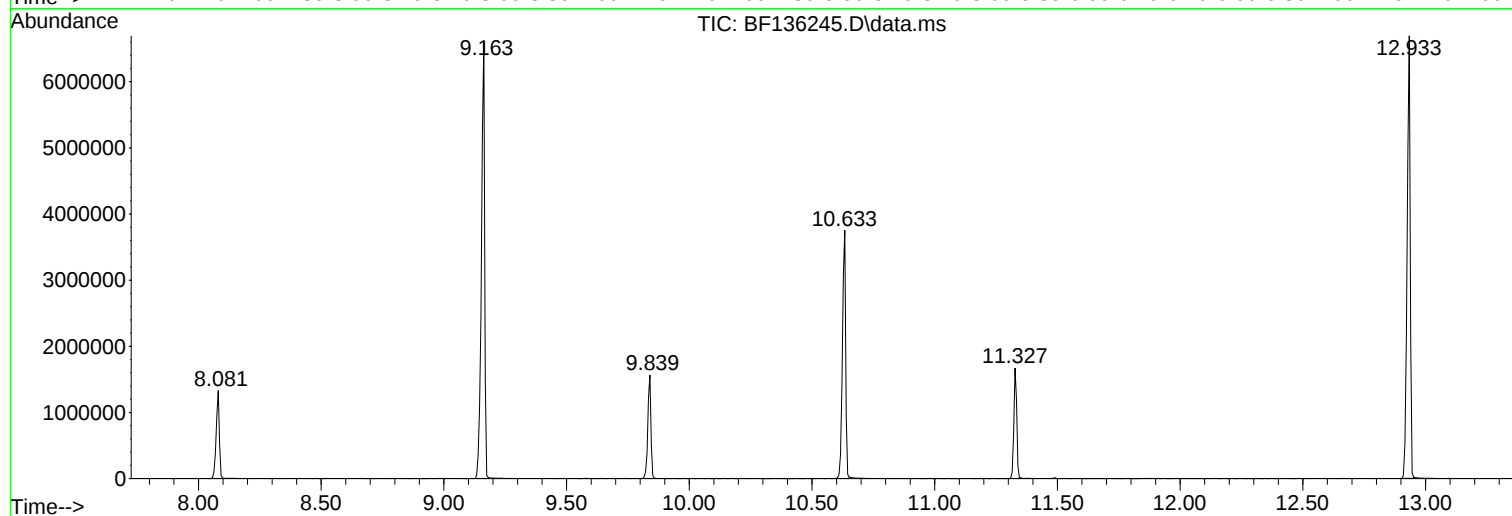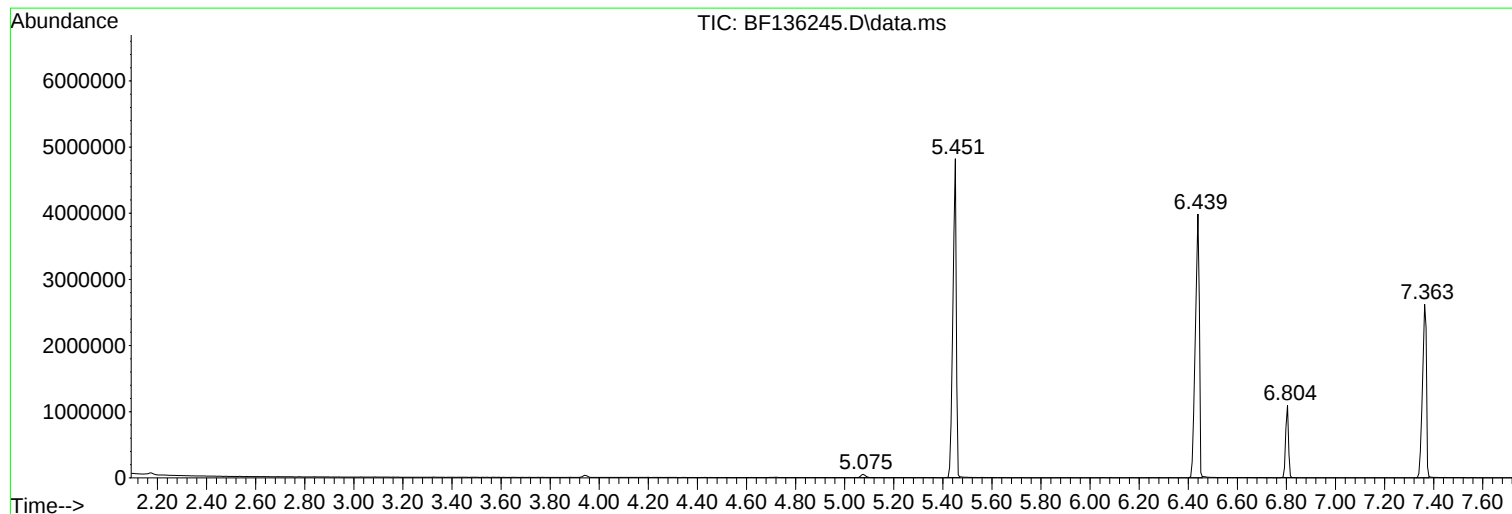

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136245.D
Acq On : 28 Nov 2023 12:59
Operator : CG\JU
Sample : PB157271BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157271BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136245.D
Acq On : 28 Nov 2023 12:59
Operator : CG\JU
Sample : PB157271BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157271BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------