

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
 Data File : BF136247.D
 Acq On : 28 Nov 2023 14:04
 Operator : CG\JU
 Sample : PB156974BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB156974BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	12	15	23	rVB	58361	82826	1.35%	0.239%
2	5.451	566	572	575	rBV	4772137	4807875	78.41%	13.866%
3	6.440	734	740	743	rBV	4034921	4738973	77.29%	13.667%
4	6.804	798	802	805	rBV	1113107	871480	14.21%	2.513%
5	7.363	891	897	900	rBV	2802246	2976612	48.54%	8.584%
6	8.081	1014	1019	1022	rBV	1380806	1198292	19.54%	3.456%
7	9.163	1197	1203	1206	rBV	6499912	6131683	100.00%	17.683%
8	9.839	1312	1318	1321	rBV	1573057	1393131	22.72%	4.018%
9	10.633	1446	1453	1456	rBV	3715379	3503874	57.14%	10.105%
10	11.327	1567	1571	1575	rBV	1729763	1416348	23.10%	4.085%
11	12.933	1839	1844	1847	rBV	6571249	5966761	97.31%	17.208%
12	13.980	2018	2022	2034	rBV	1084680	910728	14.85%	2.626%
13	15.463	2268	2274	2281	rBV	555300	676339	11.03%	1.951%




Sum of corrected areas: 34674922

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136247.D
Acq On : 28 Nov 2023 14:04
Operator : CG\JU
Sample : PB156974BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156974BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

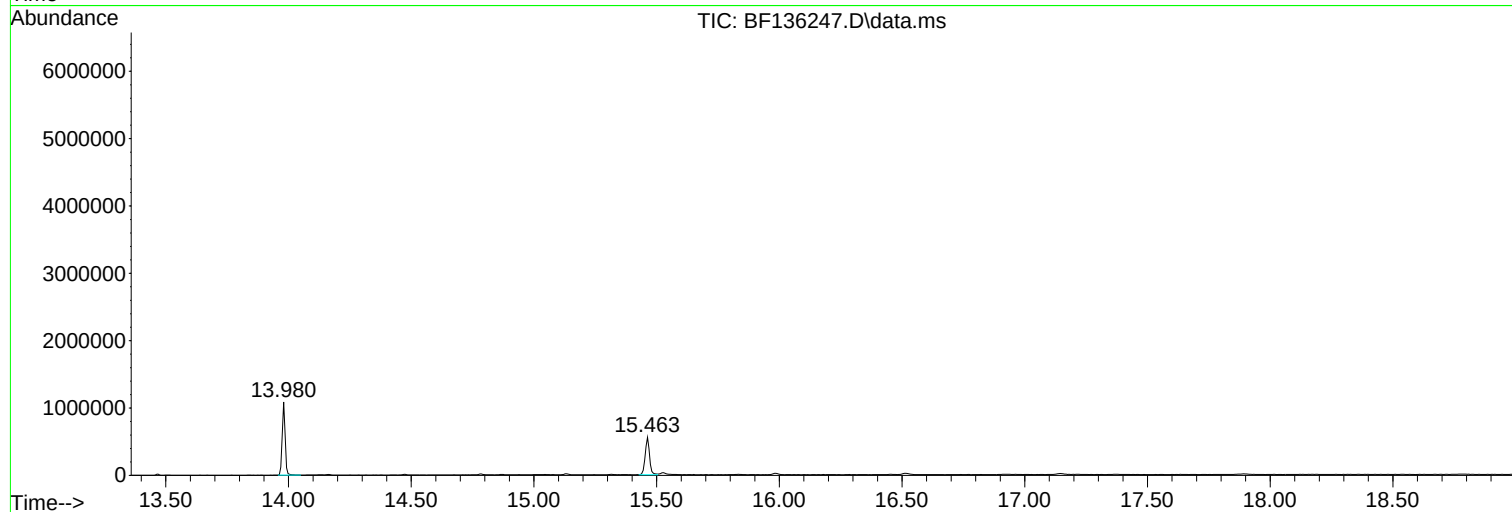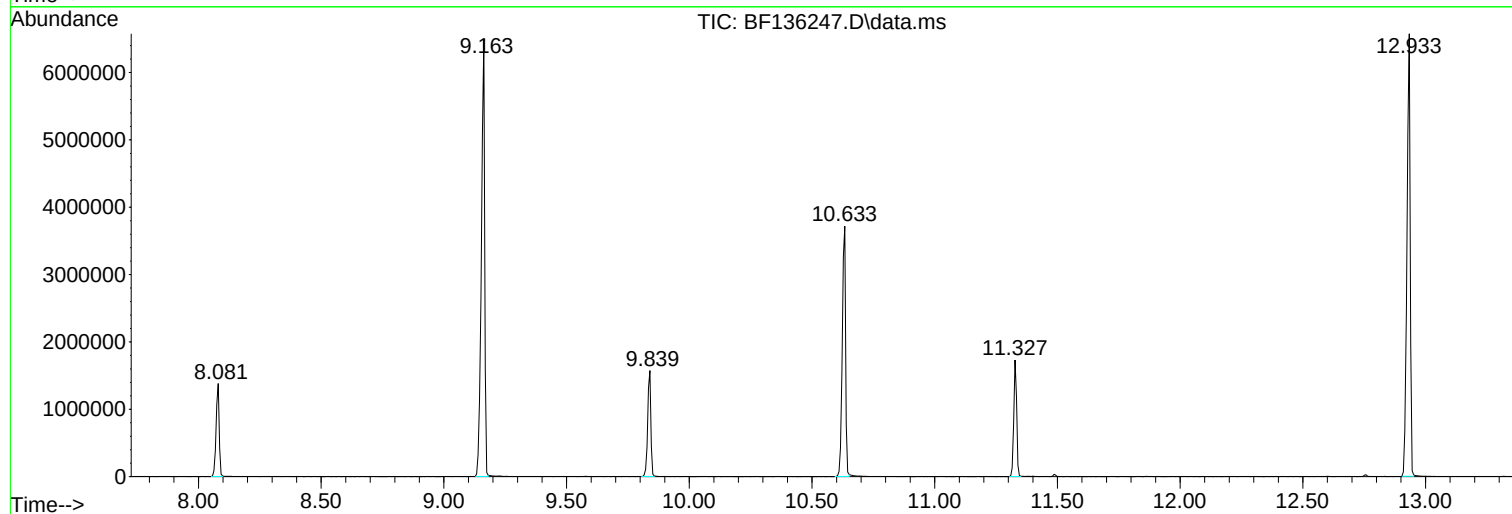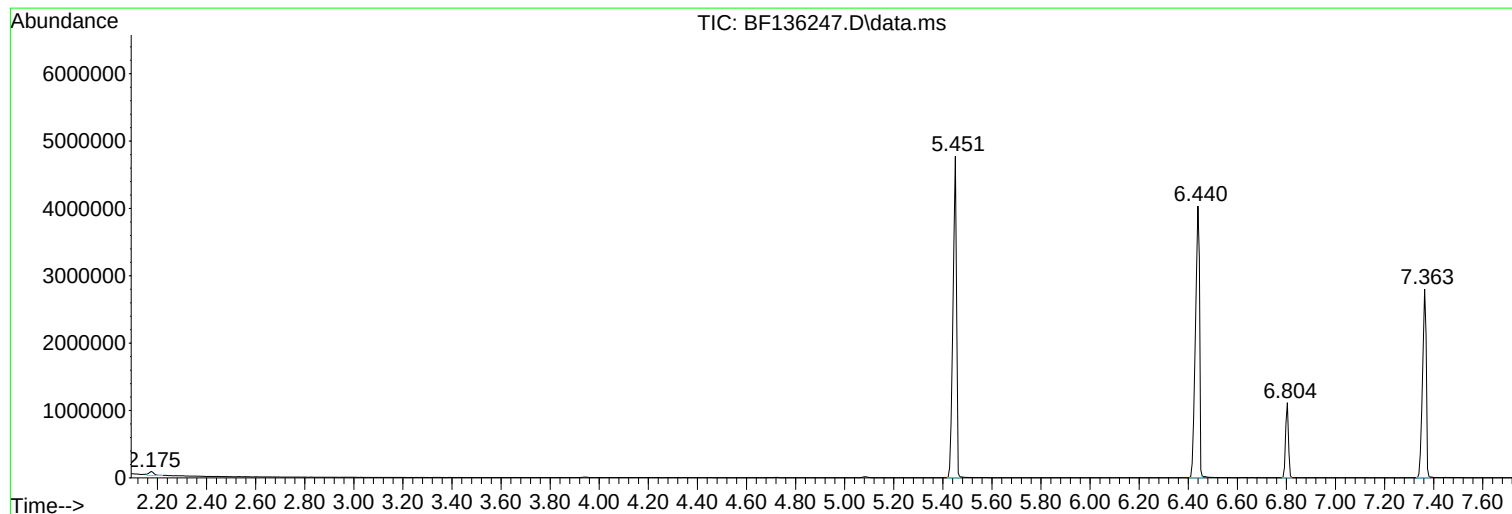

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136247.D
Acq On : 28 Nov 2023 14:04
Operator : CG\JU
Sample : PB156974BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156974BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112823\
Data File : BF136247.D
Acq On : 28 Nov 2023 14:04
Operator : CG\JU
Sample : PB156974BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156974BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------