


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112823\  
Data File : BF136238.D  
Acq On : 28 Nov 2023 09:15  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112723.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Nov 28 03:04:20 2023

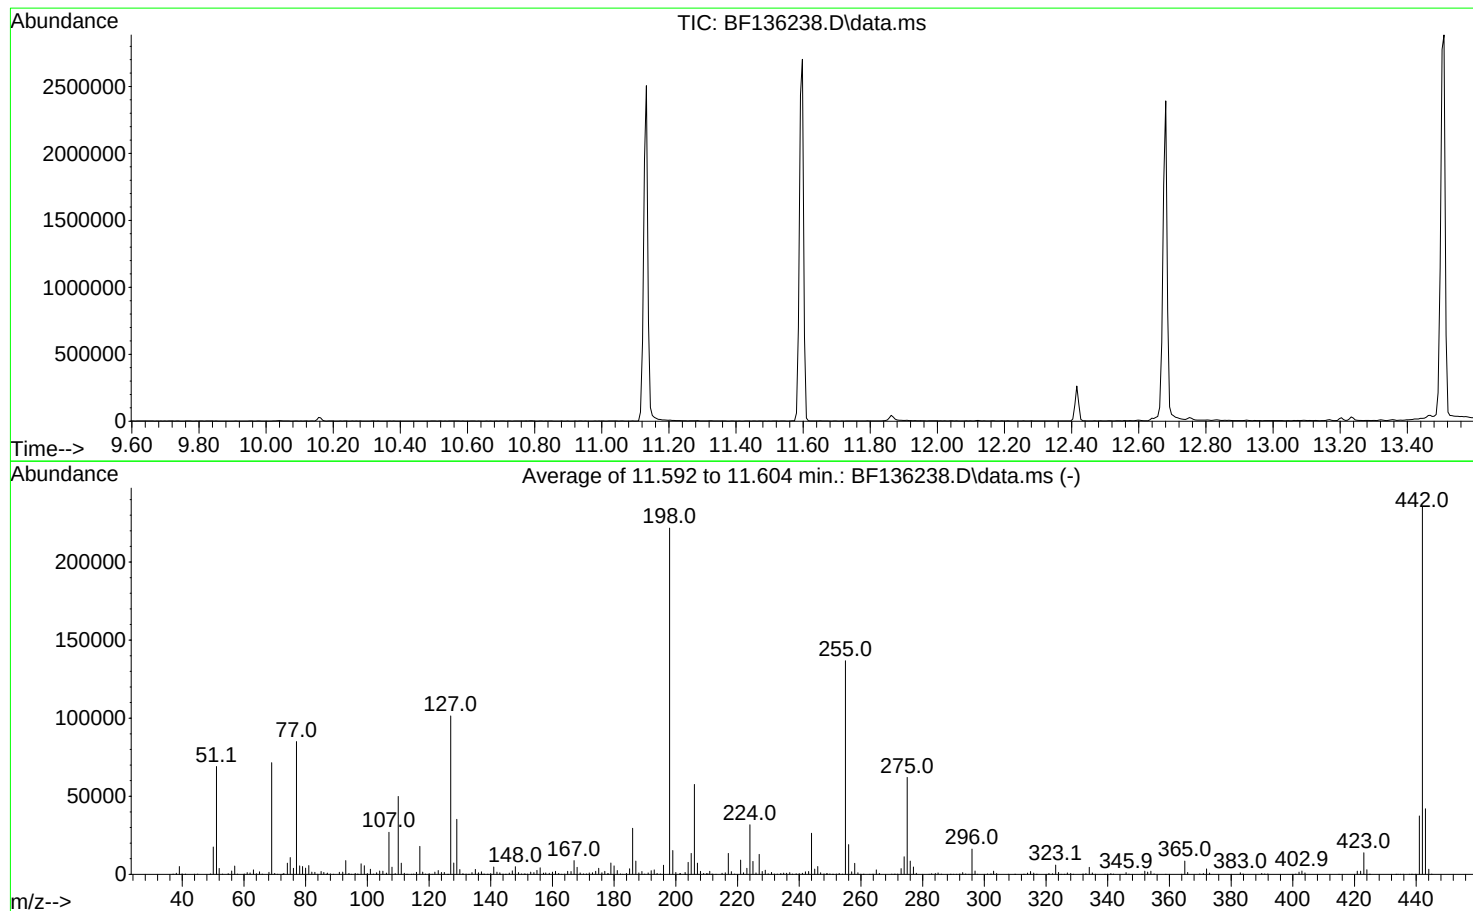




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 31.2         | 69108      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 1357       | PASS                |
| 69             | 198             | 0.00            | 100             | 32.2         | 71508      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.8          | 589        | PASS                |
| 127            | 198             | 10              | 80              | 45.7         | 101419     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 221744     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 15227      | PASS                |
| 275            | 198             | 10              | 60              | 28.0         | 62085      | PASS                |
| 365            | 198             | 1               | 100             | 3.8          | 8537       | PASS                |
| 441            | 198             | 0.01            | 100             | 16.8         | 37355      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 235563     | PASS                |
| 443            | 442             | 15              | 24              | 17.8         | 42035      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112823\  
 Data File : BF136238.D  
 Acq On : 28 Nov 2023 09:15  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Nov 28 12:27:18 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112723.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Nov 28 03:04:20 2023  
 Response via : Initial Calibration

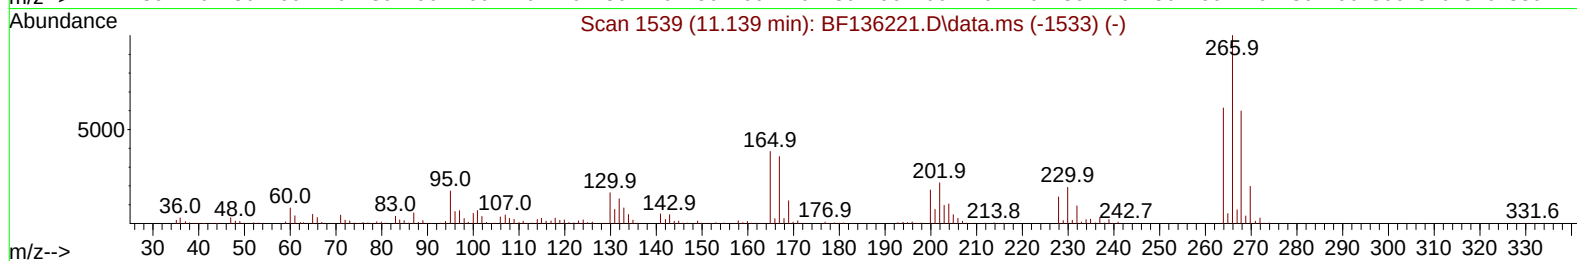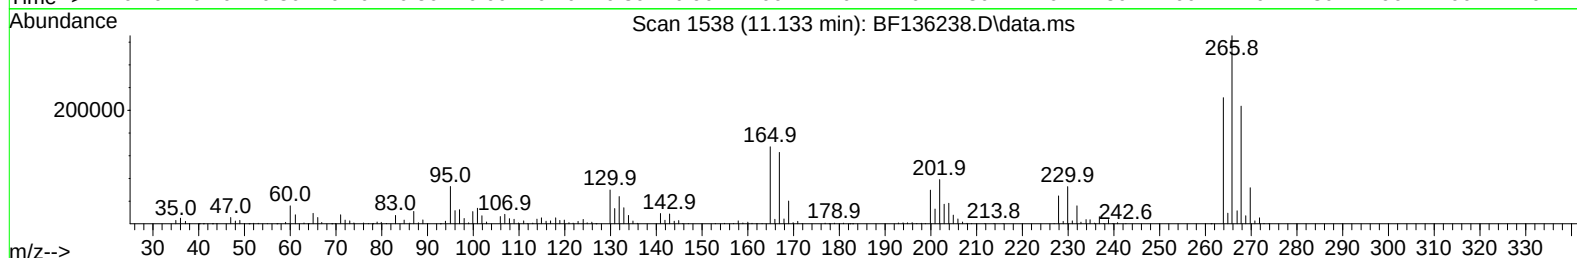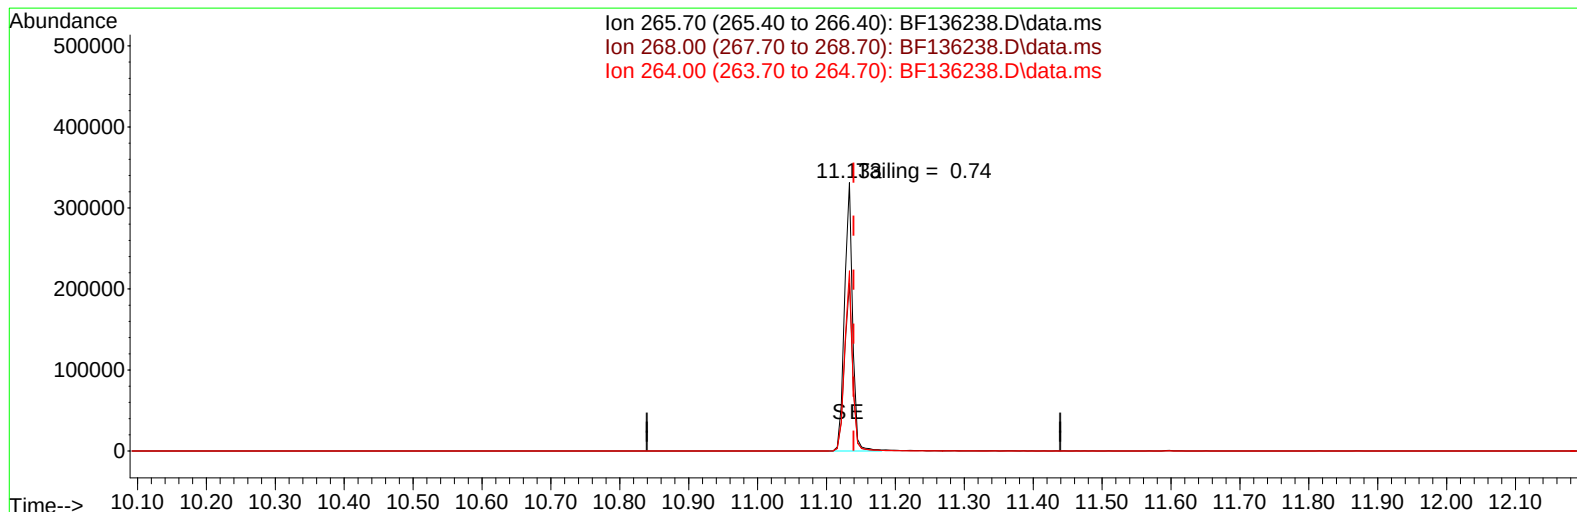

TIC: BF136238.D\data.ms

**(70) Pentachlorophenol (C)**

11.133min (-0.006) 52867.34 ng m




response 269138

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 59.90  | 62.60  |
| 264.00 | 61.40  | 67.12  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112823\  
Data File : BF136238.D  
Acq On : 28 Nov 2023 09:15  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 28 12:27:18 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 28 03:04:20 2023  
Response via : Initial Calibration

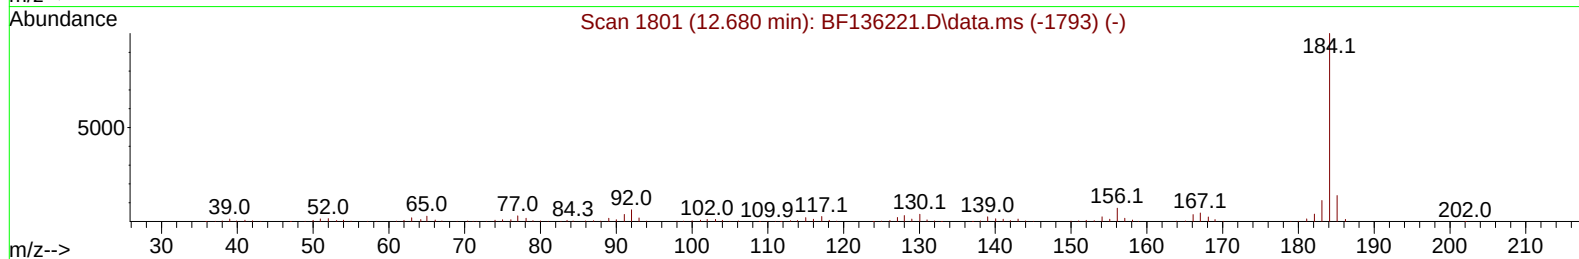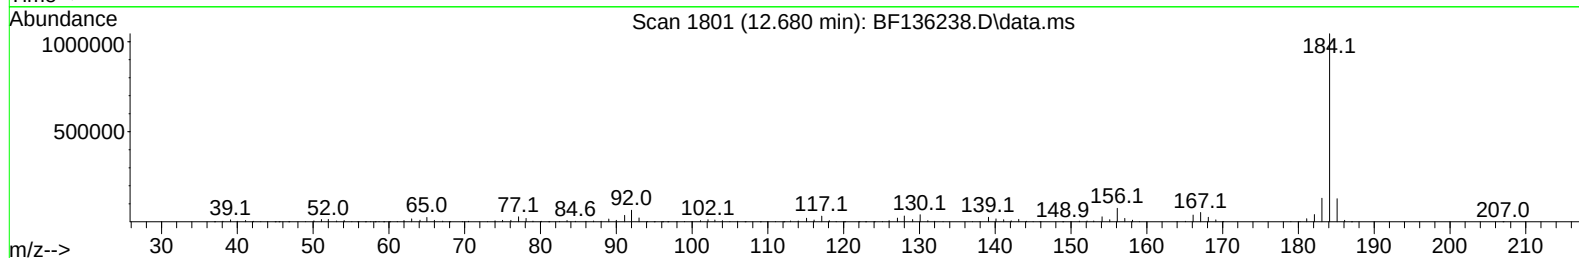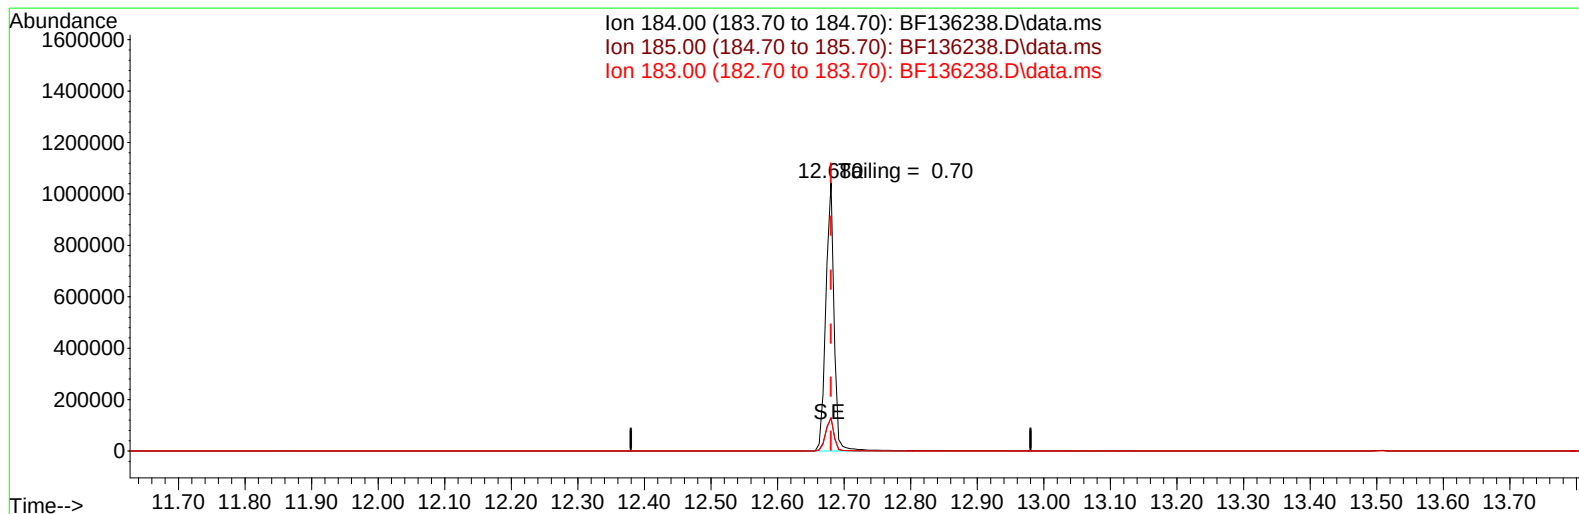

TIC: BF136238.D\data.ms

**(77) Benzidine**

**12.680min (+ 0.000) 97737.15 ng**

**response 899712**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 12.29  |
| 183.00 | 11.20  | 12.50  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/28/2023    | BNA_F            | <u>BF136238.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 577547           | 13.509             |
| DDD           | 8155             | 13.233             |
| DDE           | 464              | 12.415             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 8619          | 586166           | 1.47               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP