


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112823\  
Data File : BF136250.D  
Acq On : 28 Nov 2023 15:40  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112723.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Nov 28 03:04:20 2023

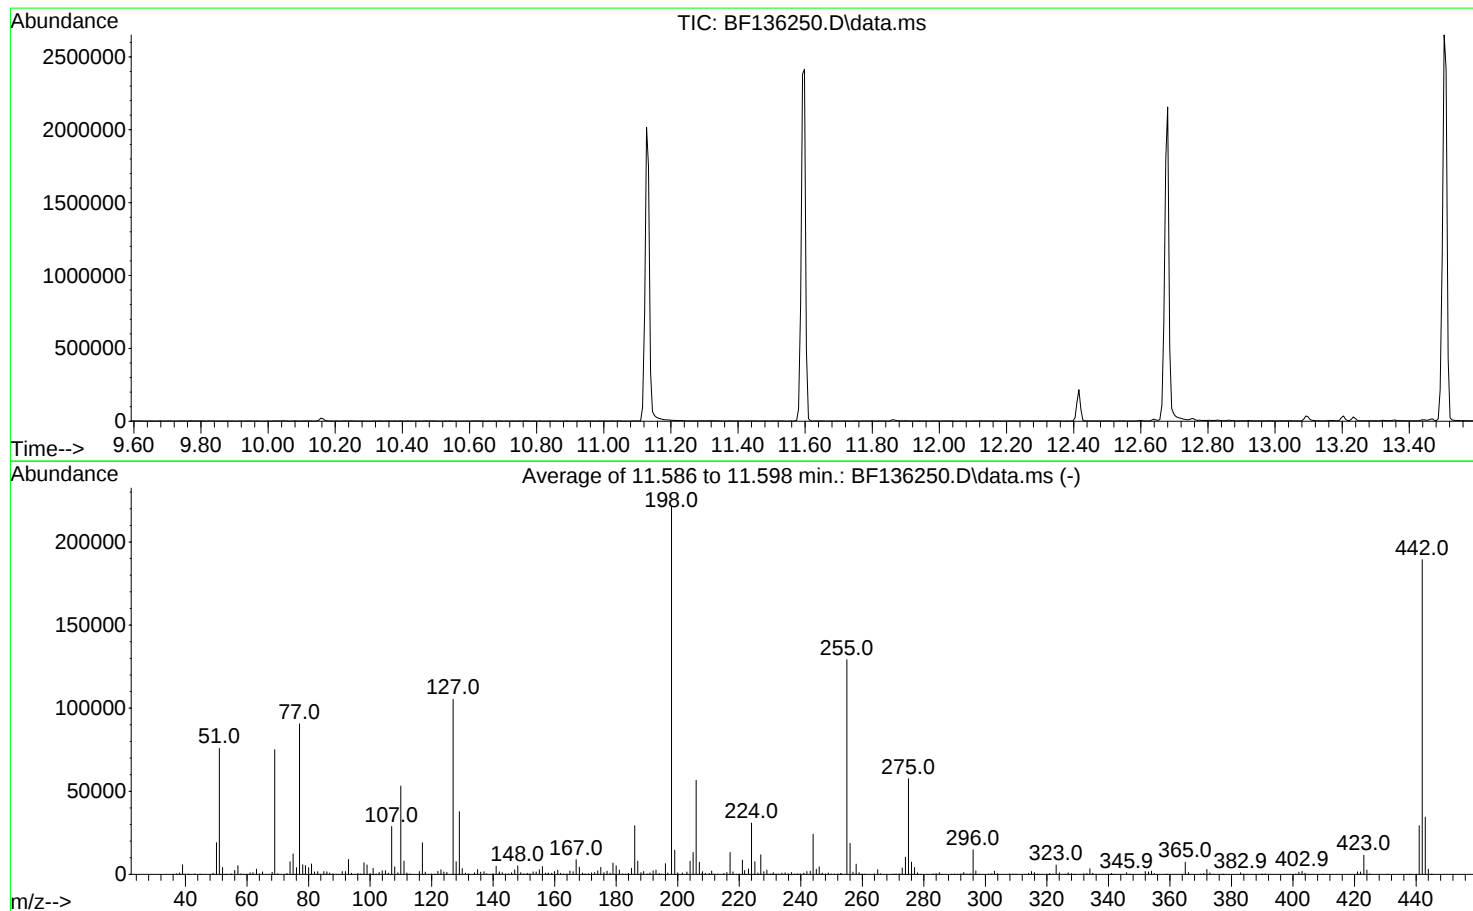




AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 34.2         | 75778      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 1302       | PASS                |
| 69             | 198             | 0.00            | 100             | 33.9         | 74992      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 283        | PASS                |
| 127            | 198             | 10              | 80              | 47.6         | 105368     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 785        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 221336     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 14590      | PASS                |
| 275            | 198             | 10              | 60              | 26.0         | 57533      | PASS                |
| 365            | 198             | 1               | 100             | 3.3          | 7330       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.2         | 29316      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 189331     | PASS                |
| 443            | 442             | 15              | 24              | 18.2         | 34465      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112823\  
Data File : BF136250.D  
Acq On : 28 Nov 2023 15:40  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 29 00:33:41 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 28 03:04:20 2023  
Response via : Initial Calibration

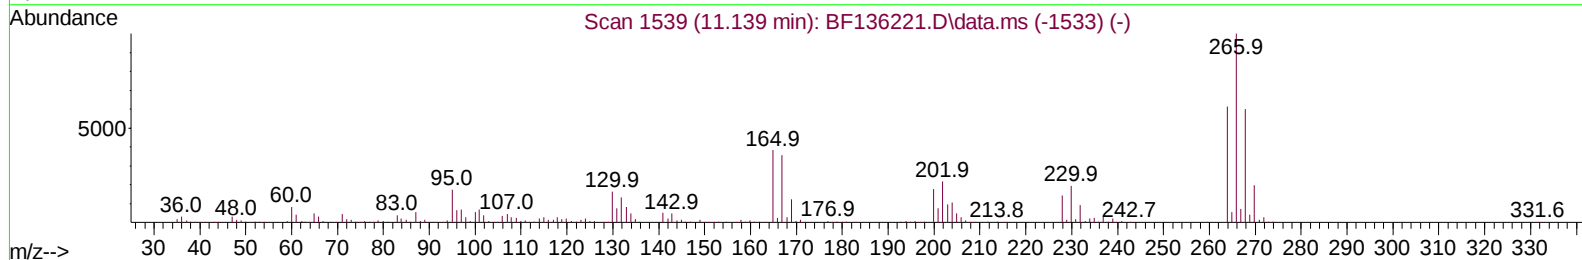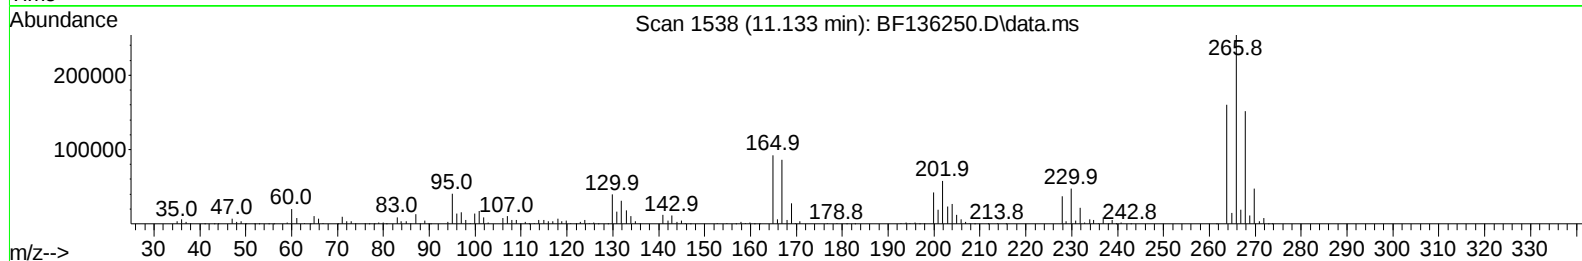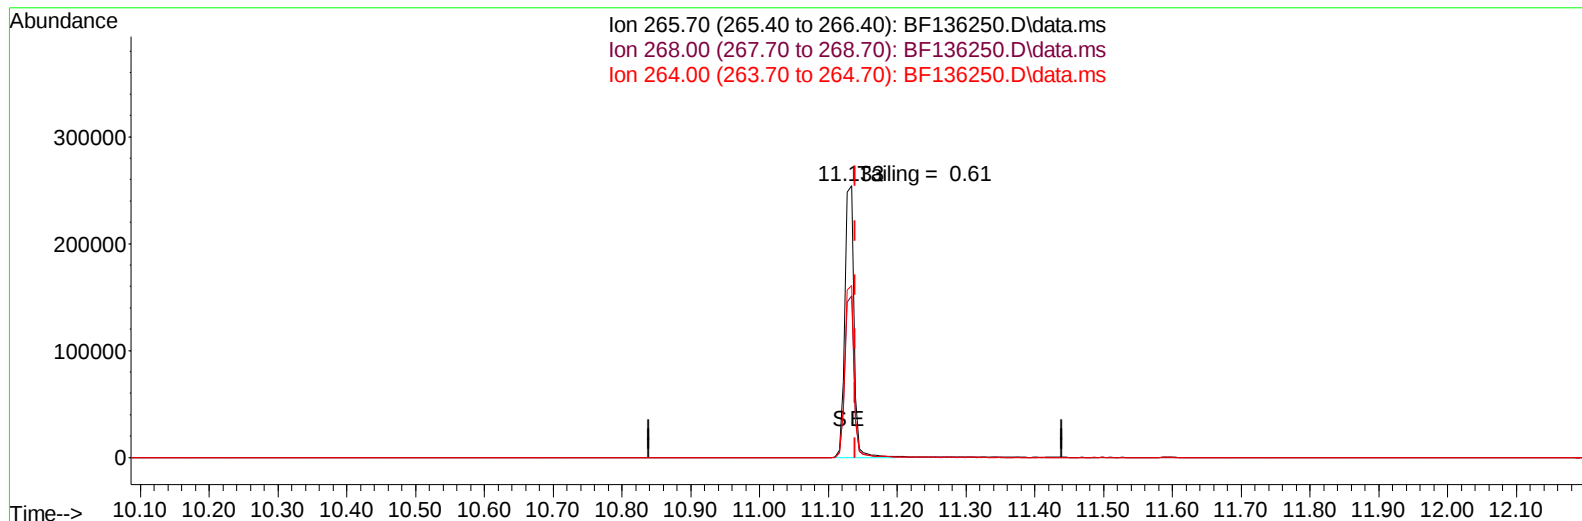

TIC: BF136250.D\data.ms

**(70) Pentachlorophenol (C)**

**11.133min (-0.006) 61048.64 ng**




**response 234372**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 59.90  | 59.66  |
| 264.00 | 61.40  | 63.21  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112823\  
 Data File : BF136250.D  
 Acq On : 28 Nov 2023 15:40  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Nov 29 00:33:41 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112723.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Nov 28 03:04:20 2023  
 Response via : Initial Calibration

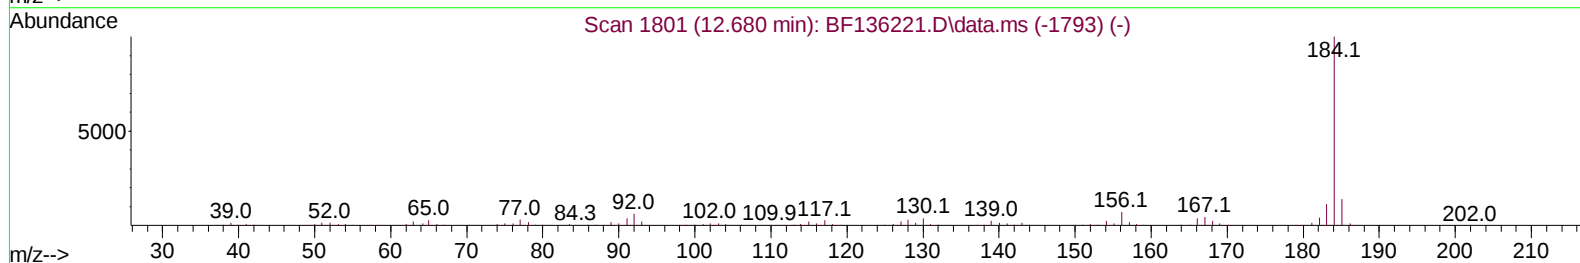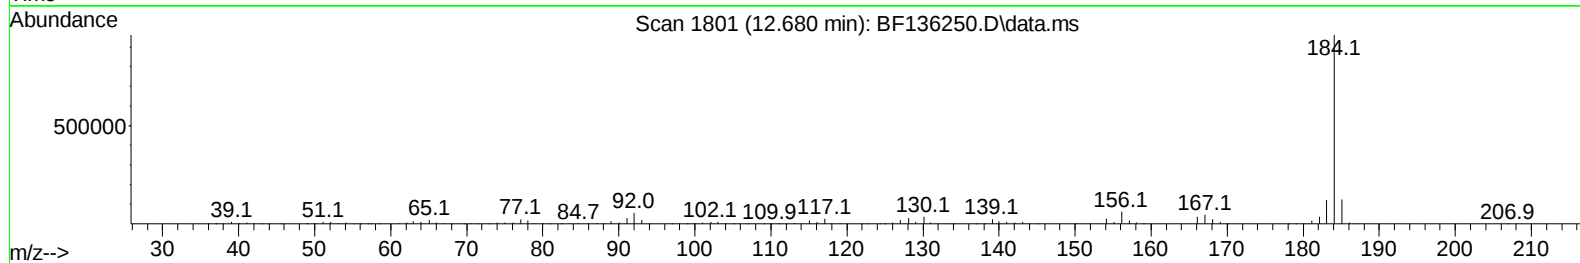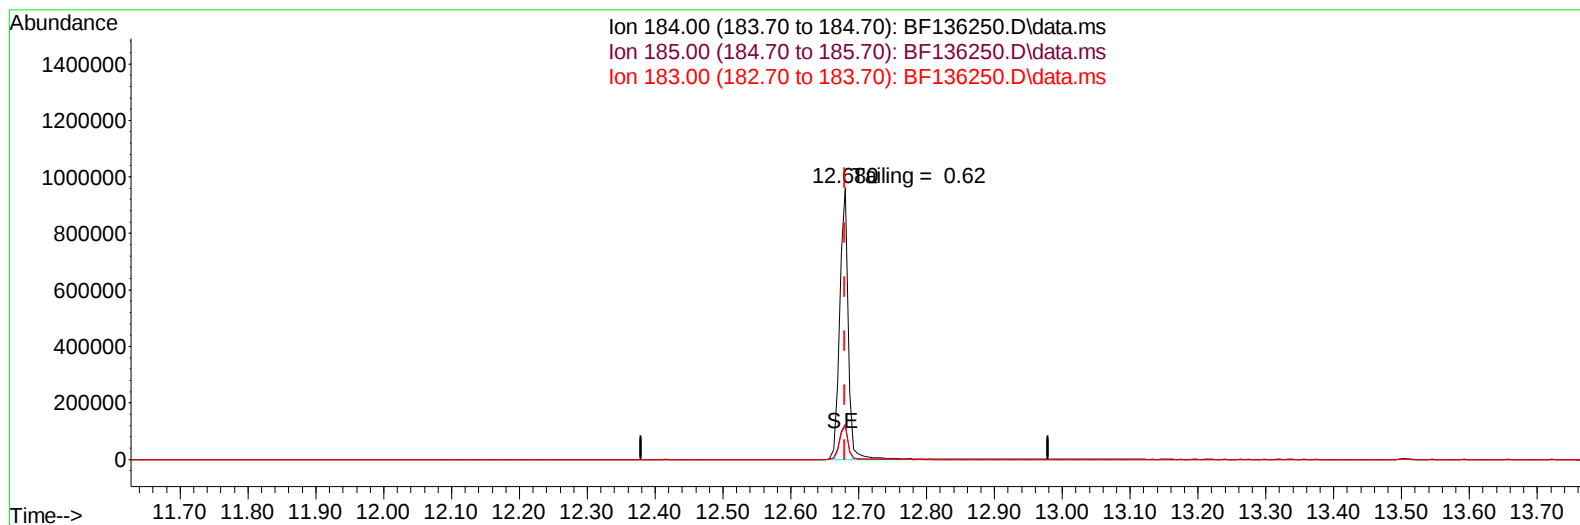

TIC: BF136250.D\data.ms

**(77) Benzidine**

**12.680min (+ 0.000) 98078.77 ng**

**response 831918**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 12.82  |
| 183.00 | 11.20  | 12.50  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/28/2023    | BNA_F            | <u>BF136250.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 526267           | 13.504             |
| DDD           | 9829             | 13.204             |
| DDE           | 327              | 12.416             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 10156         | 536423           | 1.89               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP