
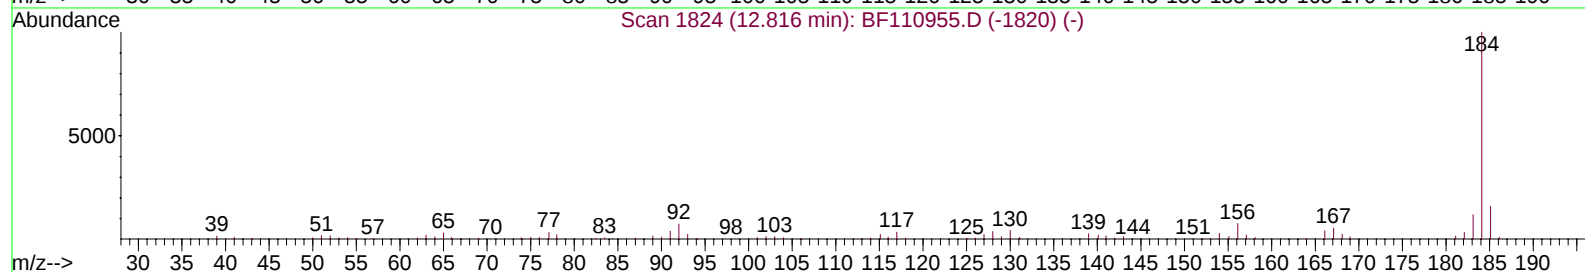
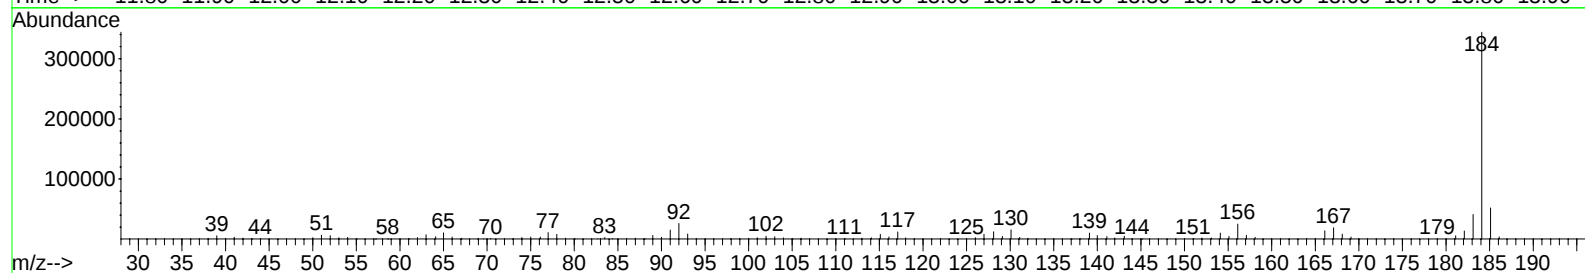


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112918\
 Data File : BF111086.D
 Acq On : 29 Nov 2018 12:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 13:31:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 29 10:35:31 2018
 Response via : Initial Calibration

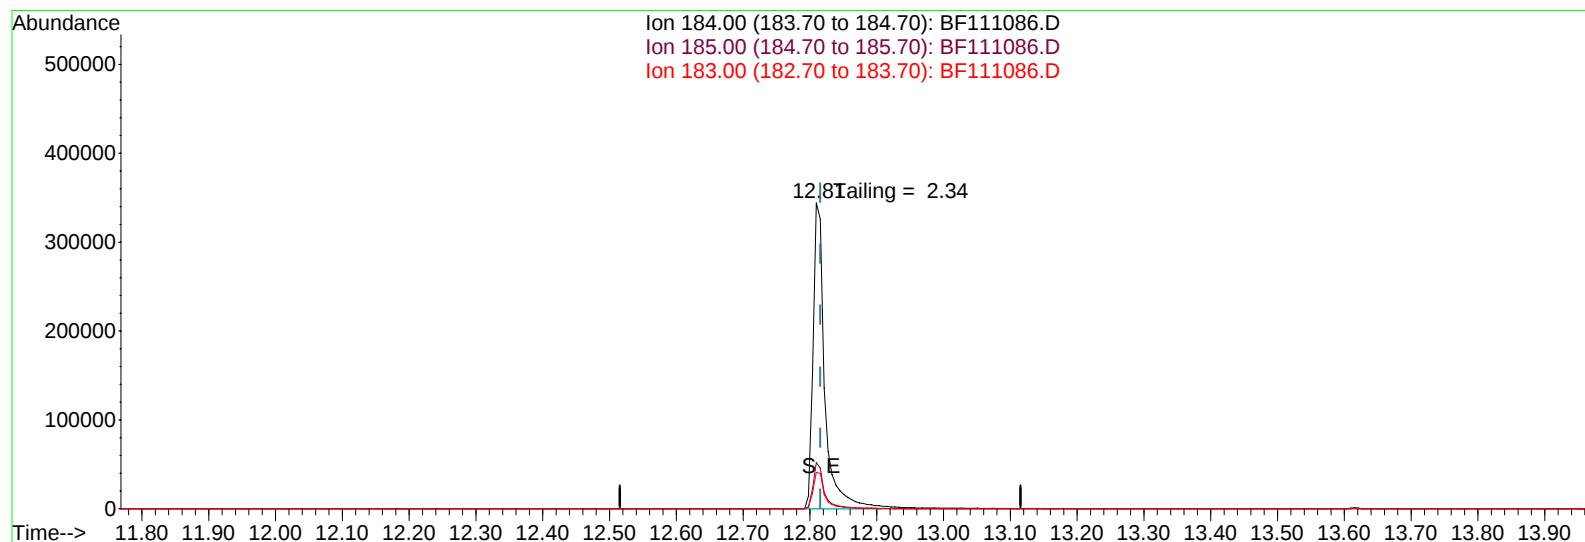

TIC: BF111086.D

(77) Benzidine




12.810min (-0.006) 0.00ng

response 428075

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.07
183.00	11.80	11.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112918\
Data File : BF111086.D
Acq On : 29 Nov 2018 12:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 13:31:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 29 10:35:31 2018
Response via : Initial Calibration

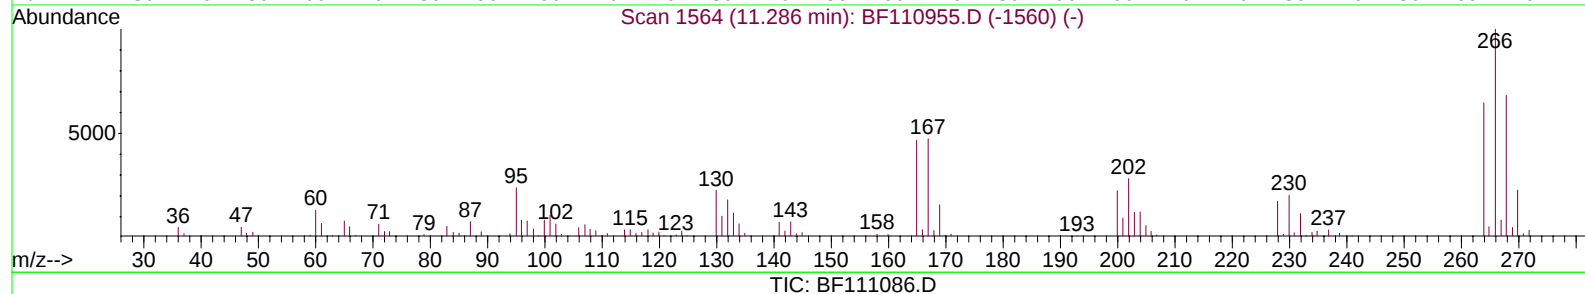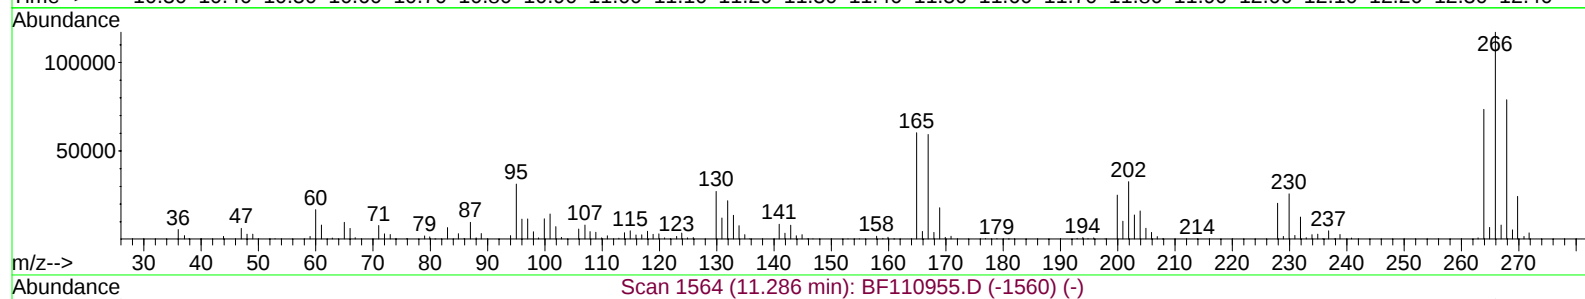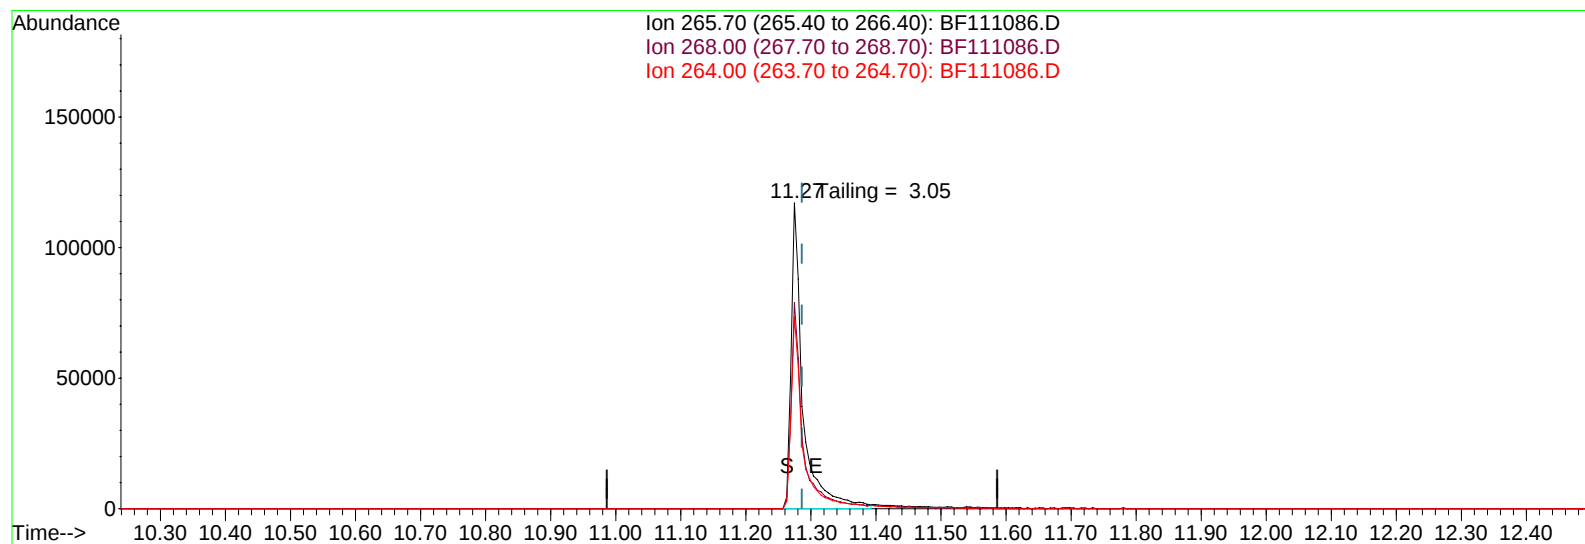

(70) Pentachlorophenol (C)

11.274min (-0.012) 115715.81ng

response 154340

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	67.43
264.00	63.20	62.76
0.00	0.00	0.00