

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112918\
 Data File : BF111096.D
 Acq On : 29 Nov 2018 17:52
 Operator : JU/SJ
 Sample : J5767-19 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-112818-B

Manual Integrations
 APPROVED

mohammad
 11/30/2018 3:49:41 PM

Quant Time: Nov 30 03:00:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 29 10:35:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.93	152	67907	20.00	ng	0.00
21) Naphthalene-d8	8.22	136	284559	20.00	ng	0.00
39) Acenaphthene-d10	9.97	164	126906	20.00	ng	-0.01
64) Phenanthrene-d10	11.47	188	190976	20.00	ng	0.00
76) Chrysene-d12	14.13	240	154874	20.00	ng	0.00
87) Perylene-d12	15.66	264	120544	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	194600	47.52	ng	0.00
7) Phenol-d6	6.56	99	263071	49.30	ng	-0.01
23) Nitrobenzene-d5	7.50	82	162886	32.76	ng	-0.01
42) 2,4,6-Tribromophenol	10.77	330	49575	39.33	ng	-0.01
45) 2-Fluorobiphenyl	9.29	172	272698	31.13	ng	0.00
79) Terphenyl-d14	13.04	244	185210	23.28	ng	-0.01
Target Compounds						
10) Phenol	6.57	94	21047	3.502	ng	82
50) Dimethylphthalate	9.69	163	23764	2.553	ng	99
71) Phenanthrene	11.49	178	44793	4.429	ng	97
75) Fluoranthene	12.69	202	99423	9.564	ng	97
78) Pyrene	12.92	202	96422	8.524	ng	98
81) Benzo(a)anthracene	14.12	228	62937	6.883	ng	97
83) Chrysene	14.15	228	52918	5.879	ng	99
86) Indeno(1,2,3-cd)pyrene	17.26	276	26133	4.045	ng	97
88) Benzo(b)fluoranthene	15.20	252	69156m	9.766	ng	
89) Benzo(k)fluoranthene	15.23	252	26471m	3.632	ng	
90) Benzo(a)pyrene	15.60	252	47879	7.264	ng	# 97
92) Benzo(a,h,i)perylene	17.74	276	23780	4.535	ng	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112918\
Data File : BF111096.D
Acq On : 29 Nov 2018 17:52
Operator : JU/SJ
Sample : J5767-19 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B

Manual Integrations
APPROVED

mohammad
11/30/2018 3:49:41 PM

Quant Time: Nov 30 03:00:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF112618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 29 10:35:31 2018
Response via : Initial Calibration

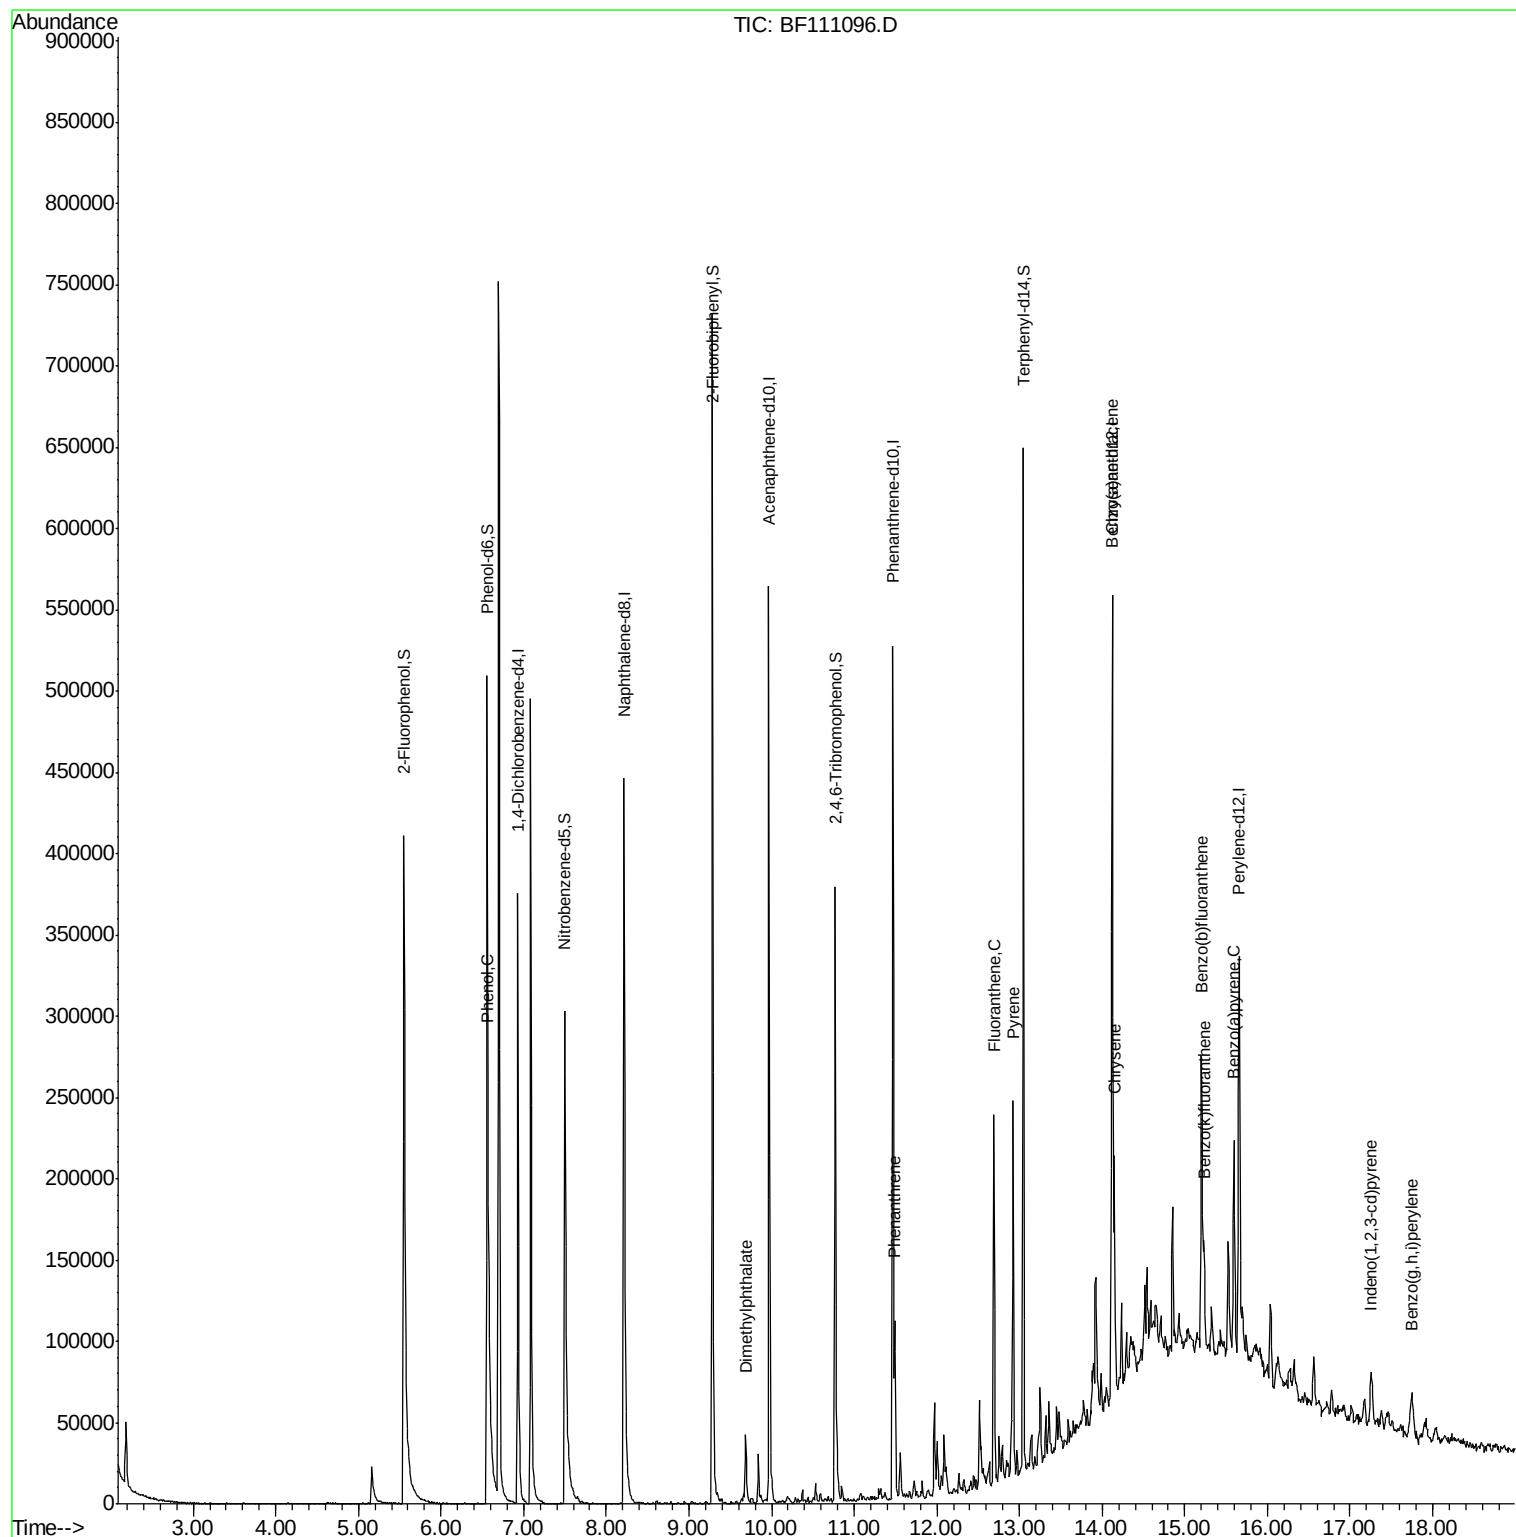

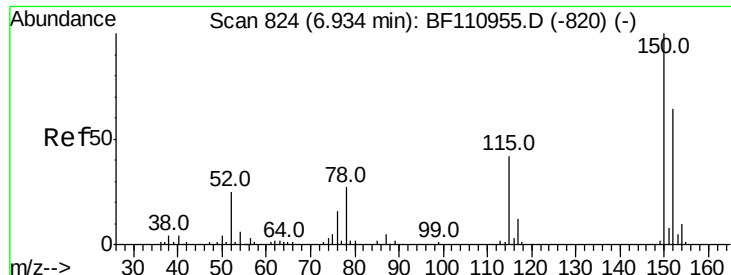

#1





1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.93 min Scan# 823
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	159.7	122.7	184.1
115	67.3	49.1	73.7

Manual Integrations
APPROVED




mohammad
11/30/2018 3:49:41 PM

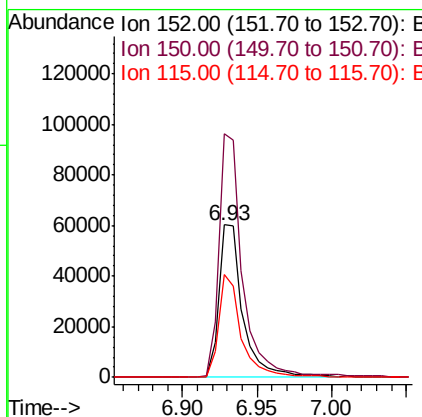


#5

2-Fluorophenol
Concen: 47.522 ng
RT: 5.55 min Scan# 589
Delta R.T. -0.00 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.1	44.1	66.1
63	31.4	23.7	35.5

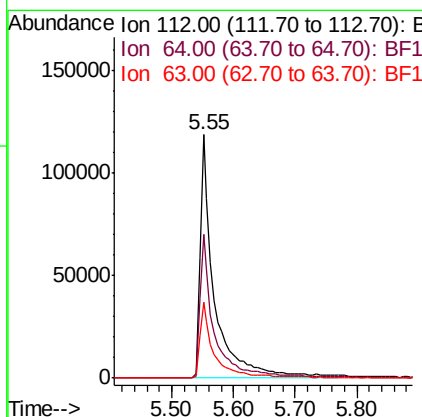

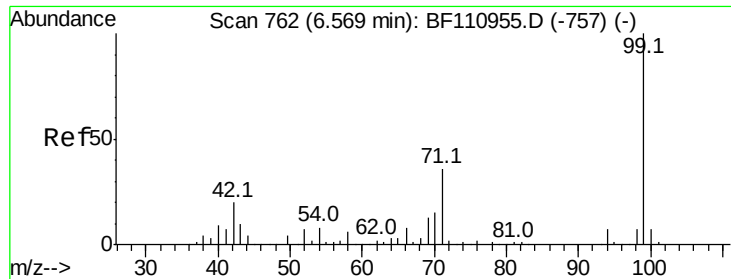

#7

Phenol-d6

Concen: 49.298 ng

RT: 6.56 min Scan# 760

Delta R.T. -0.01 min

Lab File: BF111096.D

Acq: 29 Nov 2018 17:52

Instrument :

BNA_F





ClientSampleId :

CL-02-112818-B

Tot Ion	Ion	Ratio	Resp	Lower	Upper
99	100		263071		
42	19.4	15.8	23.6		
71	35.4	28.0	42.0		

Manual Integrations
APPROVED

mohammad
11/30/2018 3:49:41 PM

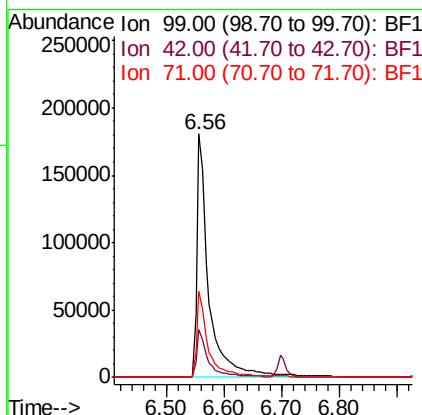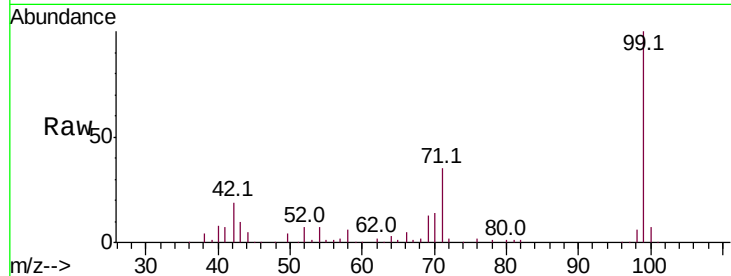

#10

Phenol

Concen: 3.502 ng




RT: 6.57 min Scan# 763


Delta R.T. -0.01 min

Lab File: BF111096.D

Acq: 29 Nov 2018 17:52

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
94	100		21047		
65	30.7	25.3	65.3		
66	61.9	54.5	94.5		

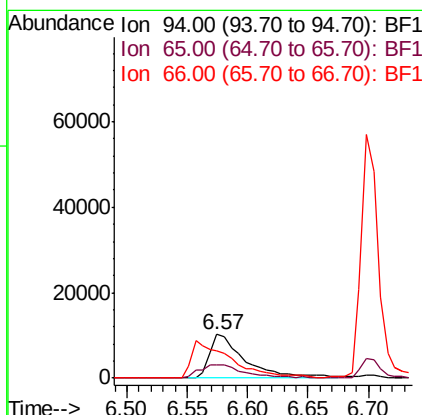

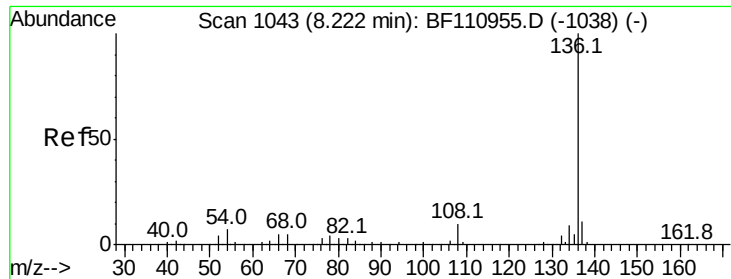





#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.22 min Scan# 1042
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B

Tot Ion	Ratio	Resp	Lower	Upper
136	100	284559		
137	10.4		8.8	13.2
54	7.6		5.4	8.2
68	4.8		4.2	6.2




Manual Integrations
APPROVED


mohammad
11/30/2018 3:49:41 PM

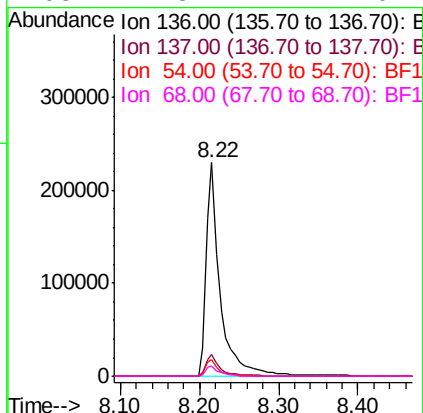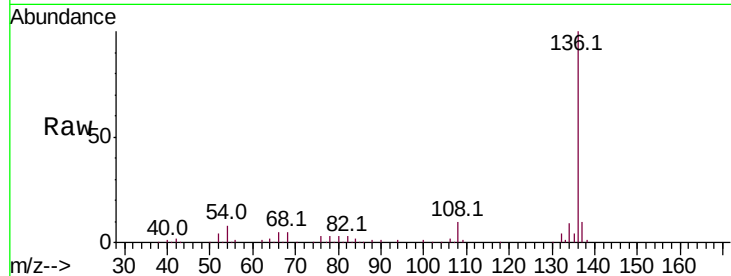

#23
Nitrobenzene-d5
Concen: 32.760 ng
RT: 7.50 min Scan# 920
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion	Ratio	Resp	Lower	Upper
82	100	162886		
128	42.3		34.2	51.2
54	52.5		38.6	58.0

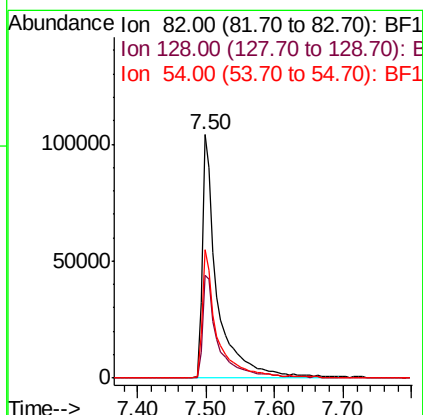

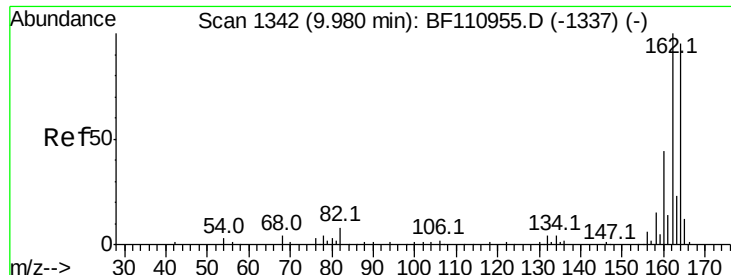


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.97 min Scan# 1340
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B




Tot Ion	Ratio	Resp	Lower	Upper
164	100			
162	103.3	83.0	124.6	
160	46.0	37.0	55.6	

Manual Integrations
APPROVED

mohammad
11/30/2018 3:49:41 PM

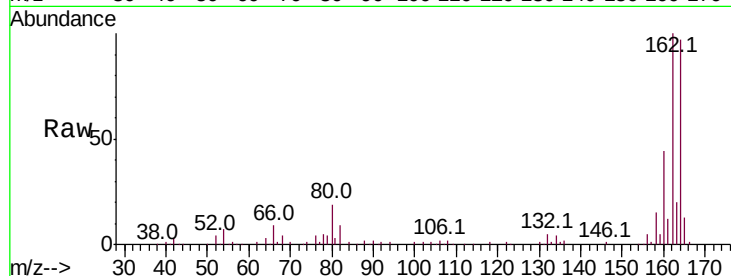




Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

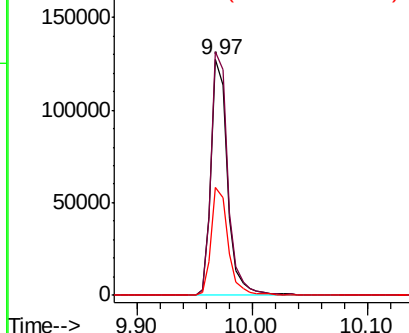


#42
2,4,6-Tribromophenol
Concen: 39.334 ng
RT: 10.77 min Scan# 1476
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion	Ratio	Resp	Lower	Upper
330	100			
332	95.9	77.1	115.7	
141	39.1	27.0	40.4	

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

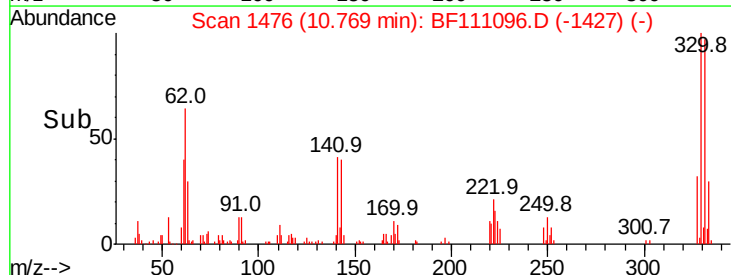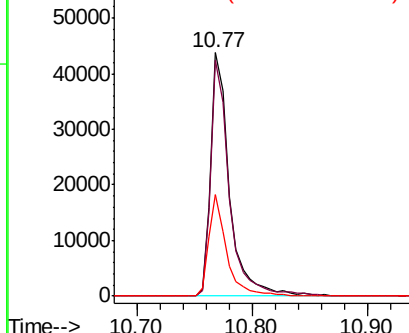

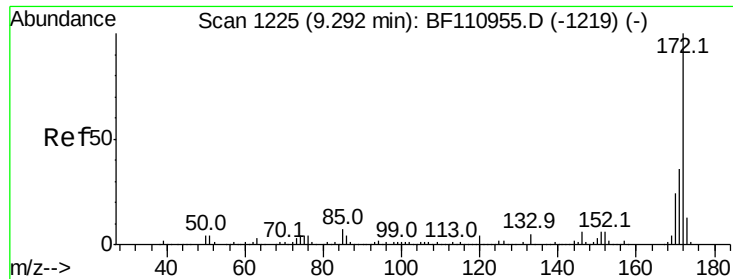





#45
2-Fluorobiphenyl
Concen: 31.132 ng
RT: 9.29 min Scan# 1224
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B

Tot Ion	Ratio	Resp	Lower	Upper
172	100	272698		
171	35.8		28.6	43.0
170	23.7		19.7	29.5




Manual Integrations
APPROVED


mohammad
11/30/2018 3:49:41 PM

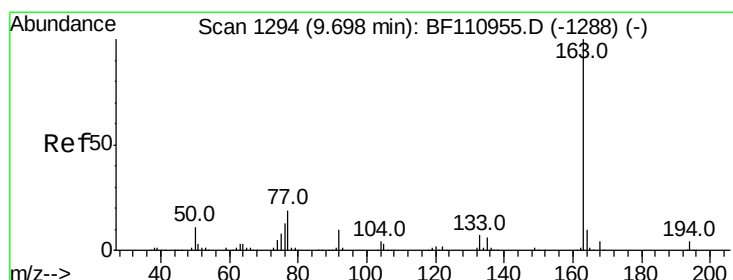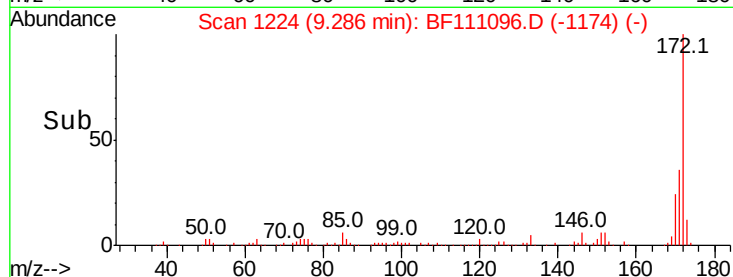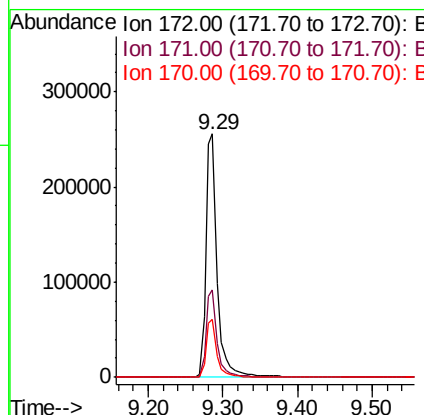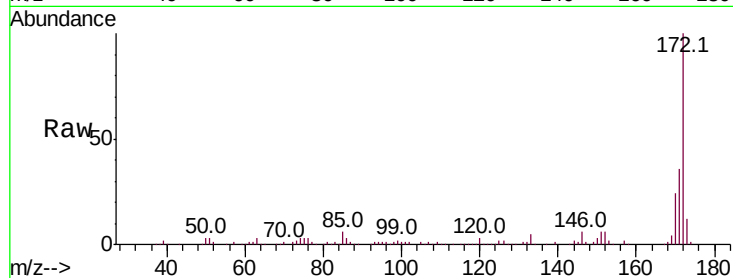

#50
Dimethylphthalate
Concen: 2.553 ng
RT: 9.69 min Scan# 1292
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	23764		
194	3.5		3.2	4.8
164	10.0		8.1	12.1

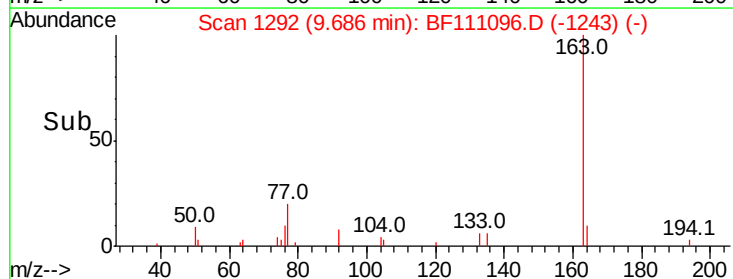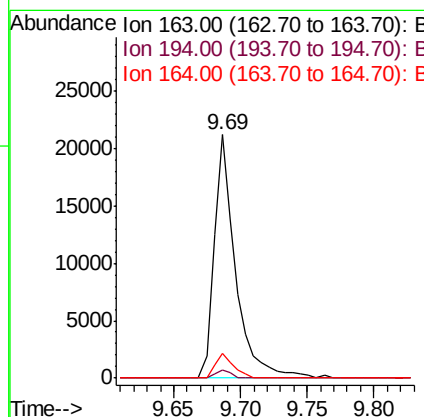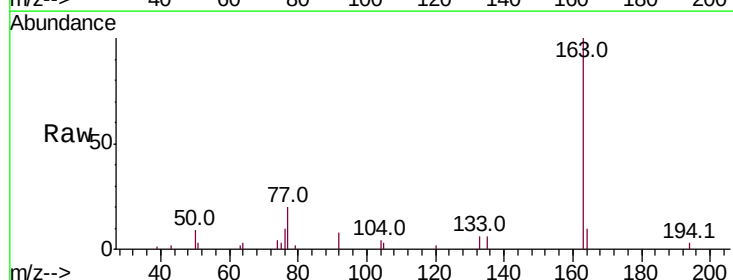

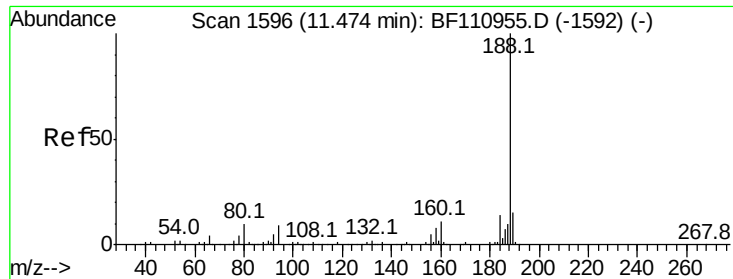


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.47 min Scan# 1595
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B




Tot Ion:	188	Resp:	190976
Ion Ratio	Lower	Upper	
188	100		
94	8.5	7.2	10.8
80	9.1	7.9	11.9

Manual Integrations
APPROVED

mohammad
11/30/2018 3:49:41 PM

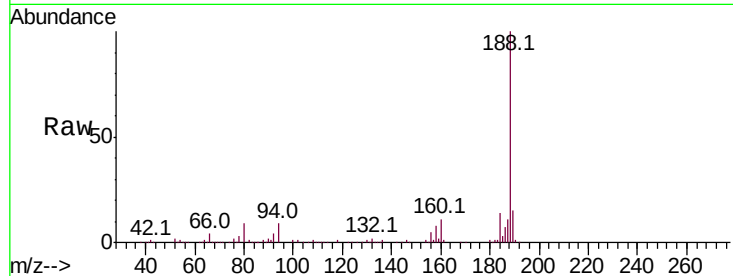


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

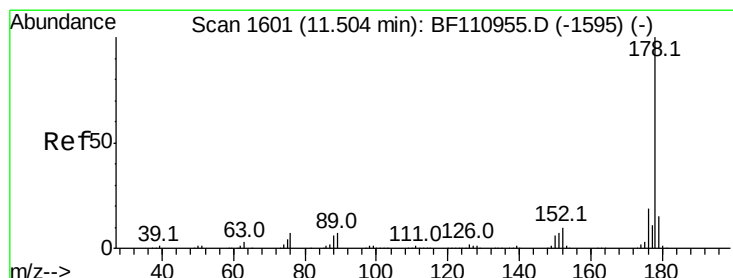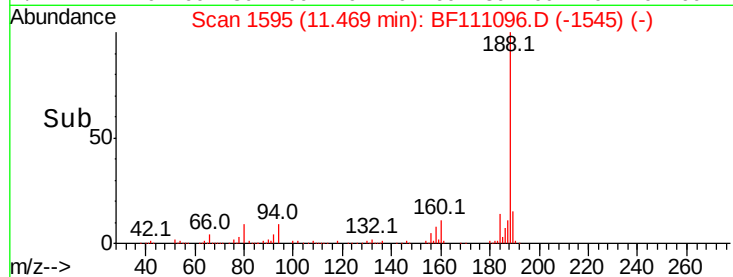
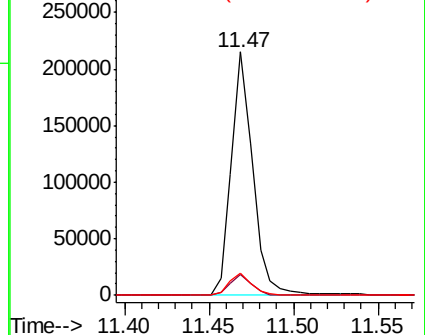



#71
Phenanthrene
Concen: 4.429 ng
RT: 11.49 min Scan# 1599
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion:	178	Resp:	44793
Ion Ratio	Lower	Upper	
178	100		
176	18.3	15.5	23.3
179	14.3	12.5	18.7

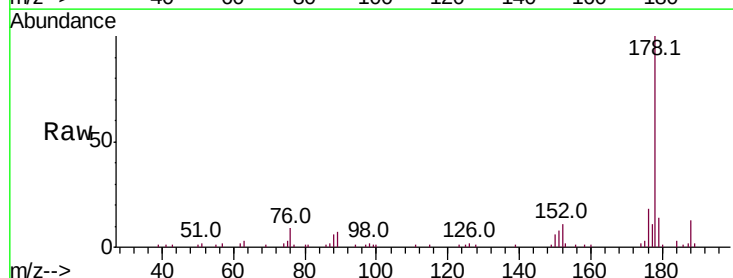

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

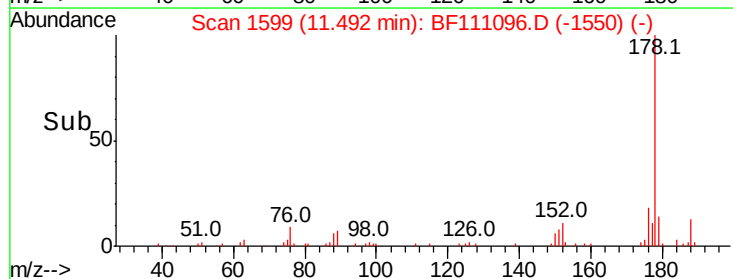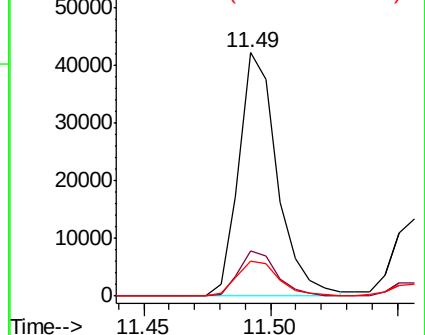

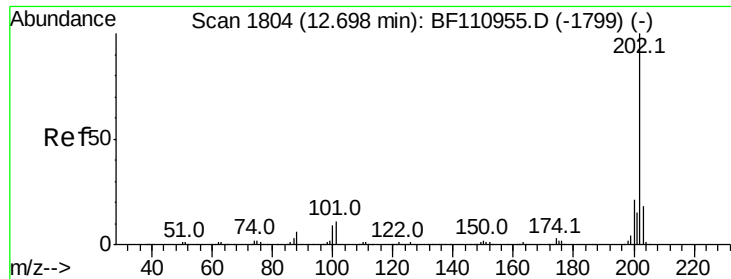


#75
Fluoranthene
Concen: 9.564 ng
RT: 12.69 min Scan# 1803
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B




Tot Ion	Ratio	Resp	Lower	Upper
202	100	99423		
101	9.6		0.0	31.4
203	17.1		0.0	37.7

Manual Integrations
APPROVED

mohammad
11/30/2018 3:49:41 PM

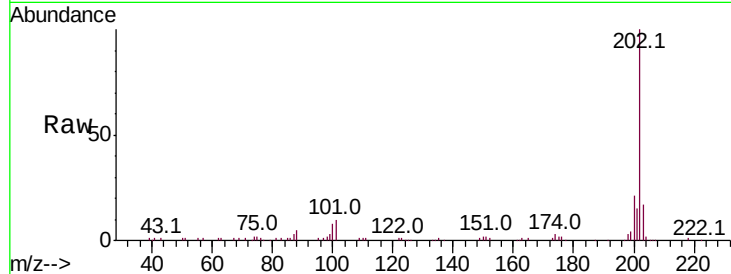




Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

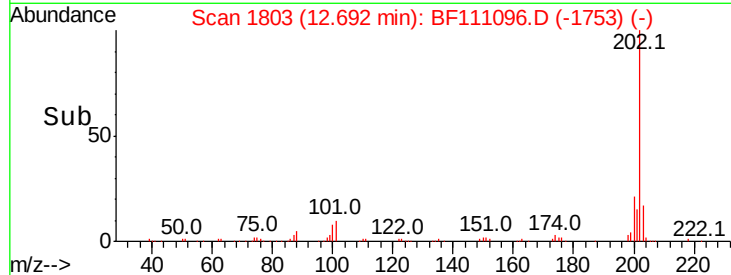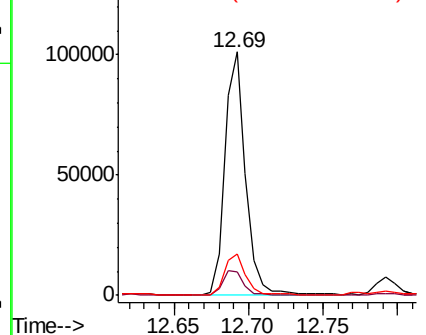


#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2047
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion	Ratio	Resp	Lower	Upper
240	100	154874		
120	9.7		8.3	12.5
236	25.0		21.2	31.8

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

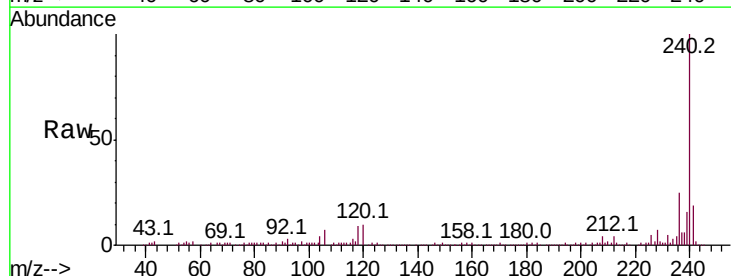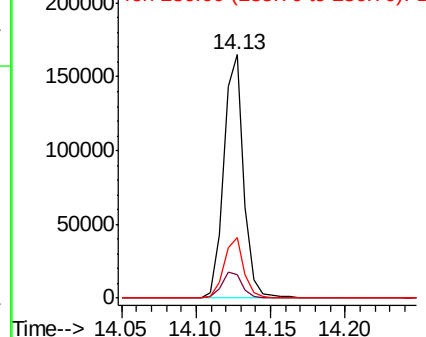

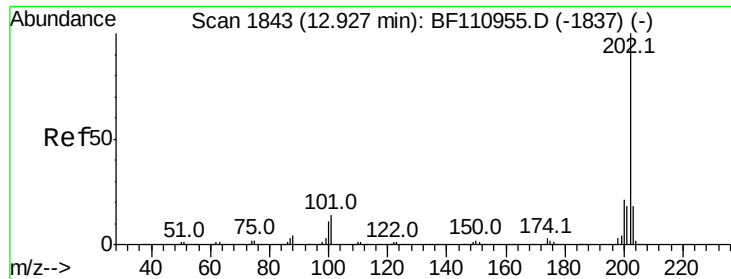





#78
Pvrene
Concen: 8.524 ng
RT: 12.92 min Scan# 1842
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B

Tot Ion	Ratio	Resp	Lower	Upper
202	100			
200	20.2	17.8	26.6	
203	17.8	14.2	21.4	




Manual Integrations
APPROVED


mohammad
11/30/2018 3:49:41 PM

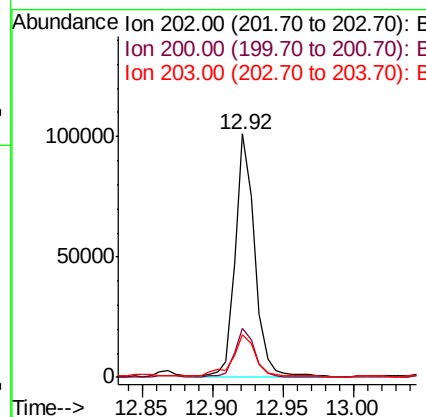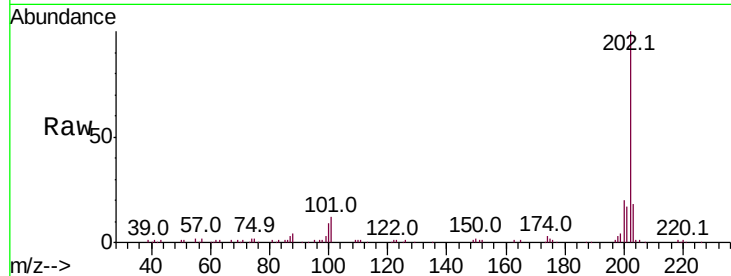

#79
Terphenyl-d14
Concen: 23.279 ng
RT: 13.04 min Scan# 1863
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion	Ratio	Resp	Lower	Upper
244	100			
212	6.8	5.8	8.8	
122	11.9	8.7	13.1	

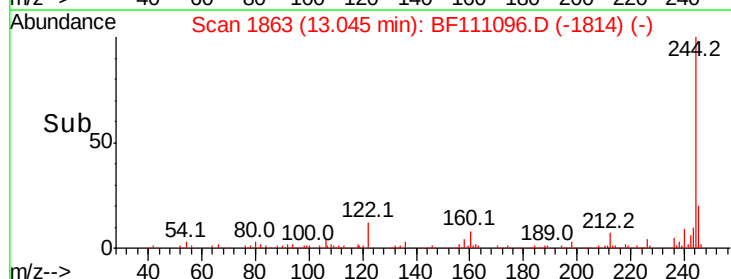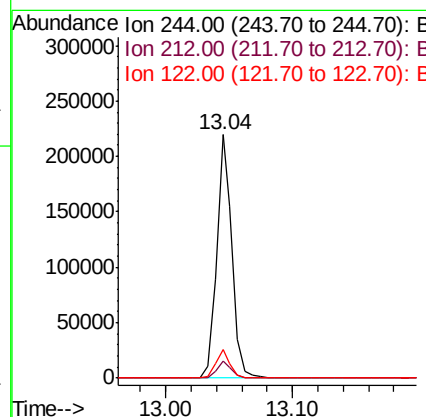







#81
Benzo(a)anthracene
Concen: 6.883 ng
RT: 14.12 min Scan# 2045
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B

Tot Ion	Ratio	Lower	Upper
228	100		
226	27.0	22.1	33.1
229	22.1	15.6	23.4




Manual Integrations
APPROVED


mohammad
11/30/2018 3:49:41 PM

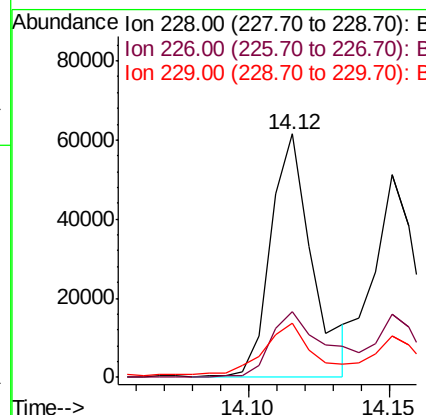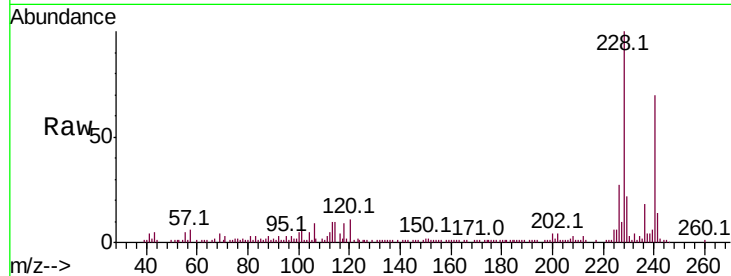

#83
Chrysene
Concen: 5.879 ng
RT: 14.15 min Scan# 2051
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.1	24.7	37.1
229	20.6	15.9	23.9

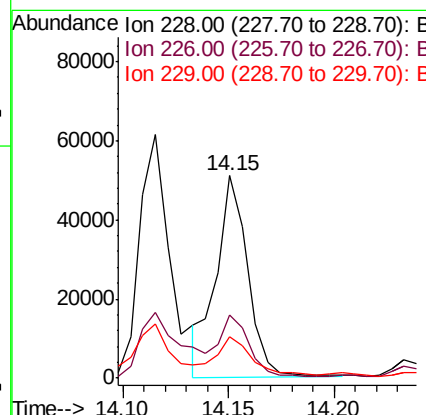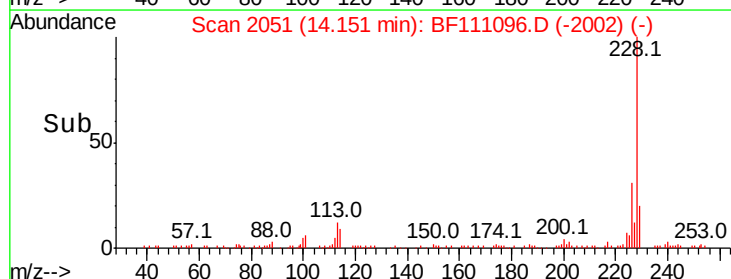

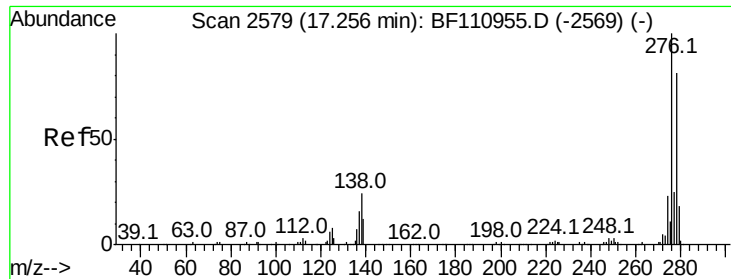


#86
Indeno(1,2,3-cd)pyrene
Concen: 4.045 ng
RT: 17.26 min Scan# 2579
Delta R.T. 0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B

Tot Ion	Ratio	Lower	Upper
276	100		
138	24.8	18.5	27.7
277	26.7	20.0	30.0

Manual Integrations
APPROVED

mohammad
11/30/2018 3:49:41 PM



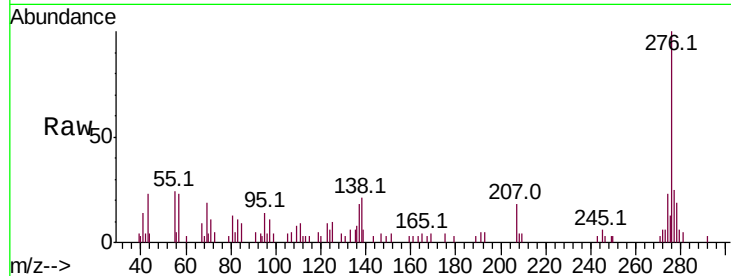


Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

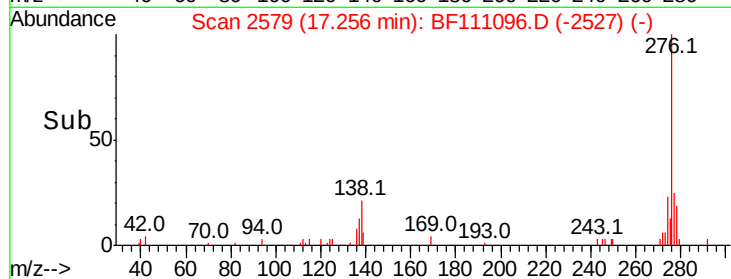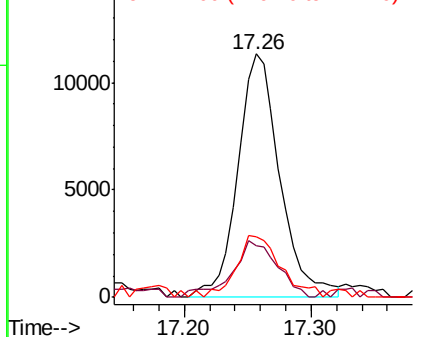

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.66 min Scan# 2307
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52




Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.4	18.7	28.1
265	21.7	16.7	25.1


Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

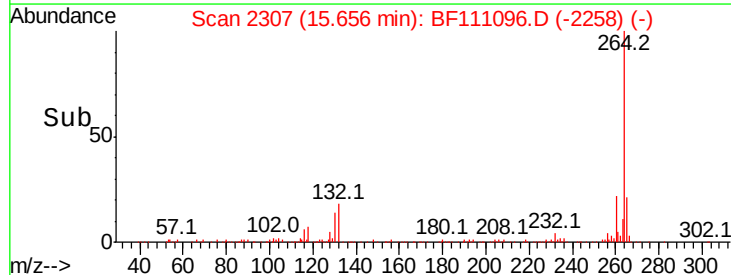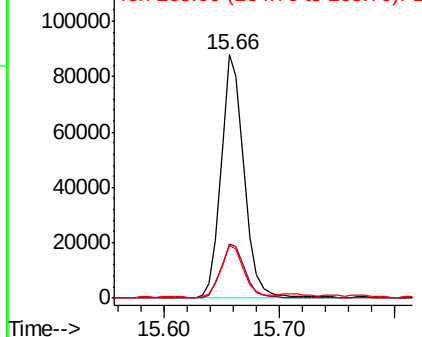







#88
Benzo(b)fluoranthene
Concen: 9.766 ng m
RT: 15.20 min Scan# 2230
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.2	25.8
125	13.5	8.2	12.4




Manual Integrations
APPROVED


mohammad
11/30/2018 3:49:41 PM

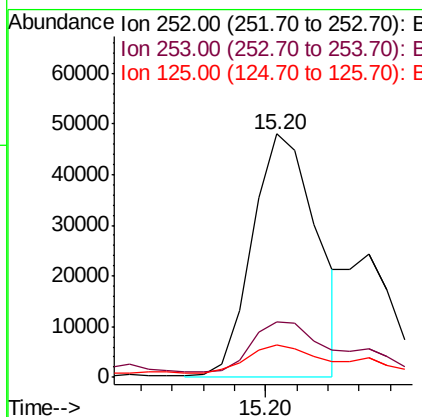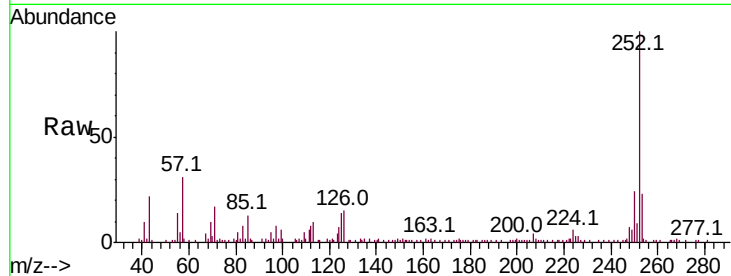

#89
Benzo(k)fluoranthene
Concen: 3.632 ng m
RT: 15.23 min Scan# 2235
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	17.2	25.8
125	15.7	7.4	11.0

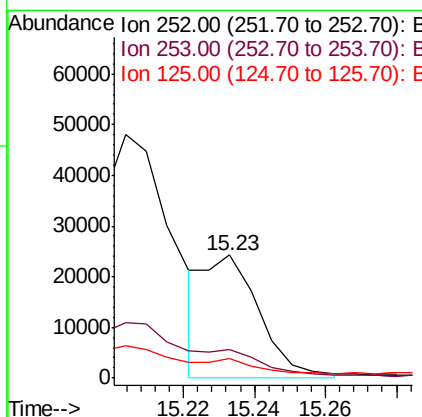

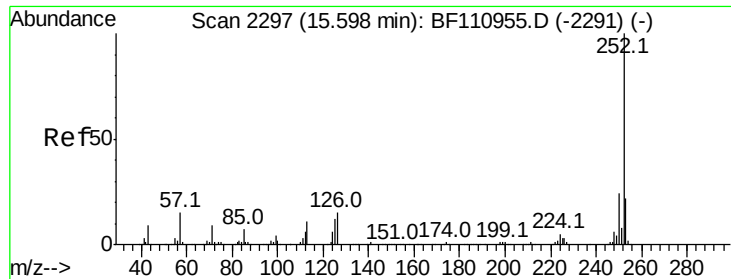


#90
Benzo(a)pyrene
Concen: 7.264 ng
RT: 15.60 min Scan# 2297
Delta R.T. -0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Instrument :
BNA_F
ClientSampleId :
CL-02-112818-B

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.2	27.4
125	14.2	9.0	13.6

Manual Integrations
APPROVED

mohammad
11/30/2018 3:49:41 PM



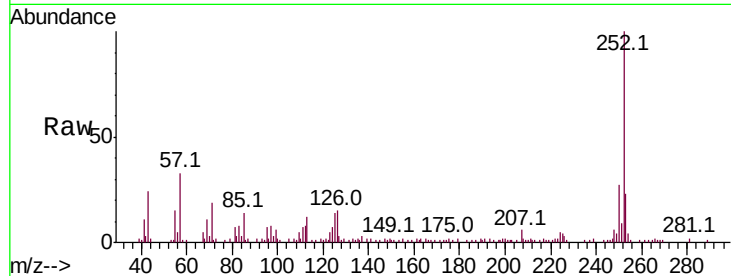


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

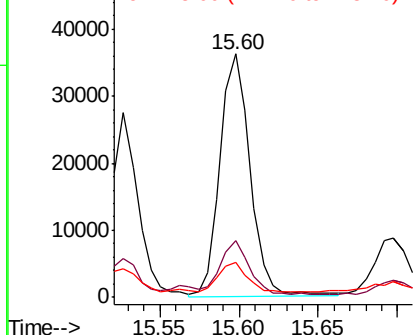

#92
Benzo(g,h,i)perylene
Concen: 4.535 ng
RT: 17.74 min Scan# 2662
Delta R.T. 0.01 min
Lab File: BF111096.D
Acq: 29 Nov 2018 17:52

Tgt Ion	Ratio	Lower	Upper
276	100		
277	27.3	18.8	28.2
138	23.0	16.0	24.0

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

