
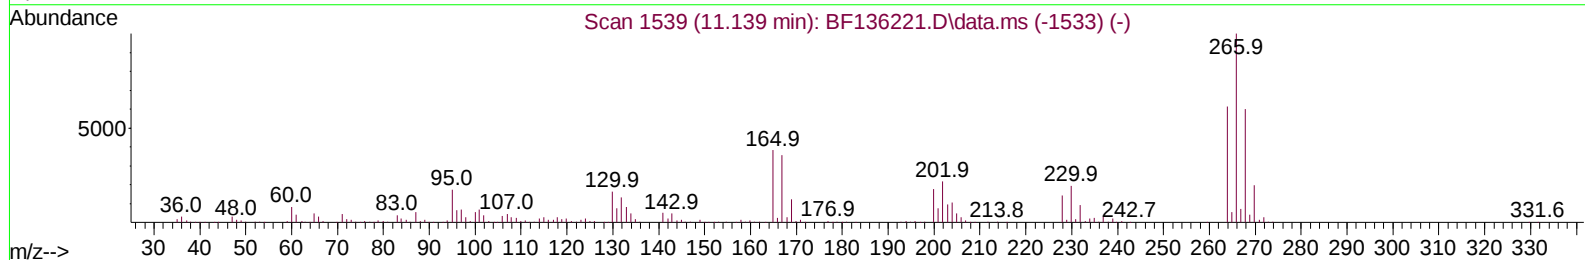
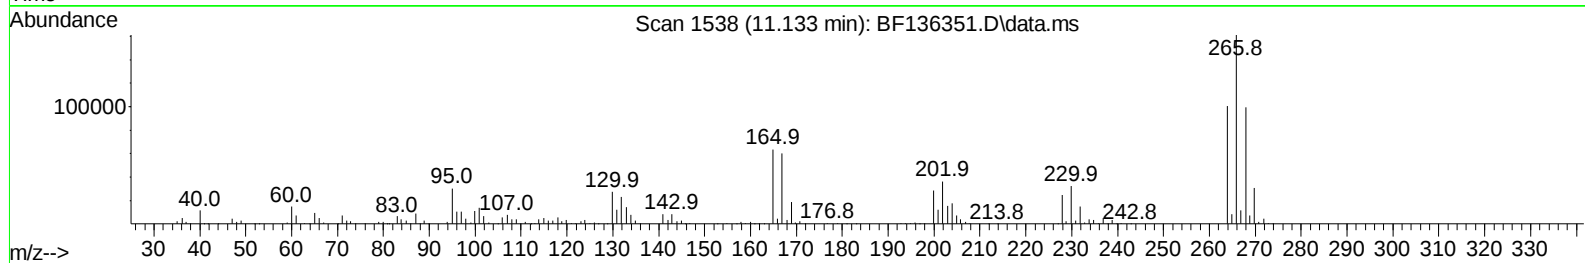


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136351.D
Acq On : 01 Dec 2023 22:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 01:10:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

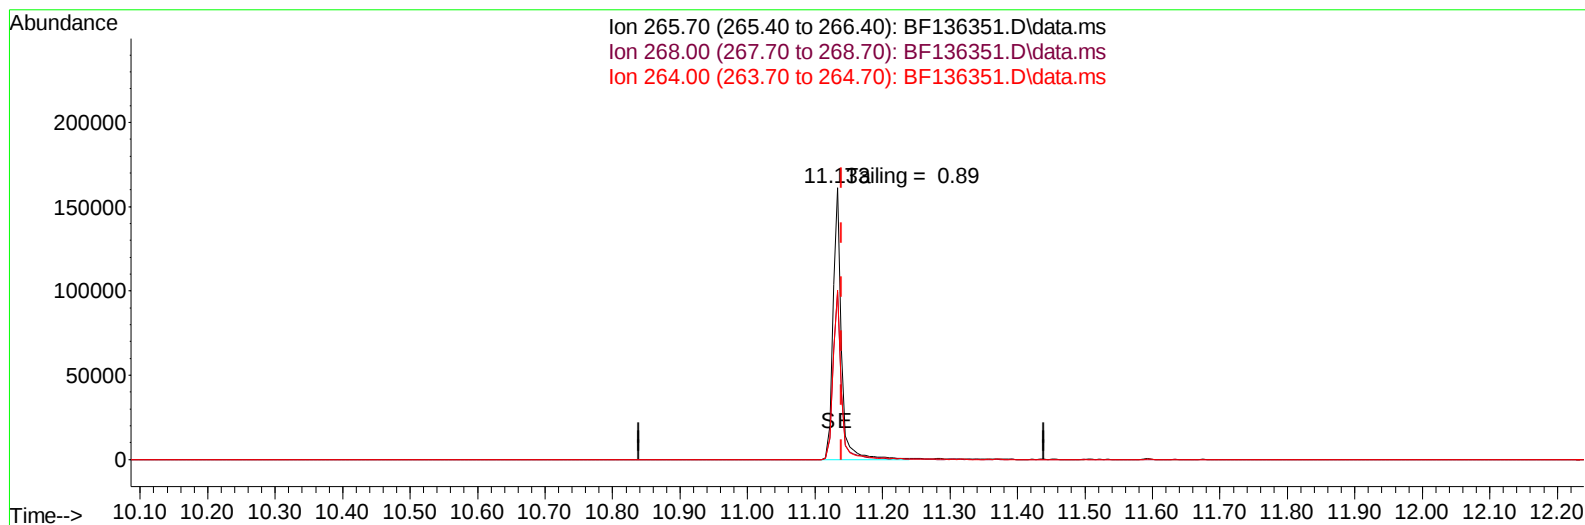

TIC: BF136351.D\data.ms

(70) Pentachlorophenol (C)




11.133min (-0.006) 32594.53 ng

response 140309

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	61.69
264.00	61.40	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136351.D
Acq On : 01 Dec 2023 22:56
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 01:10:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

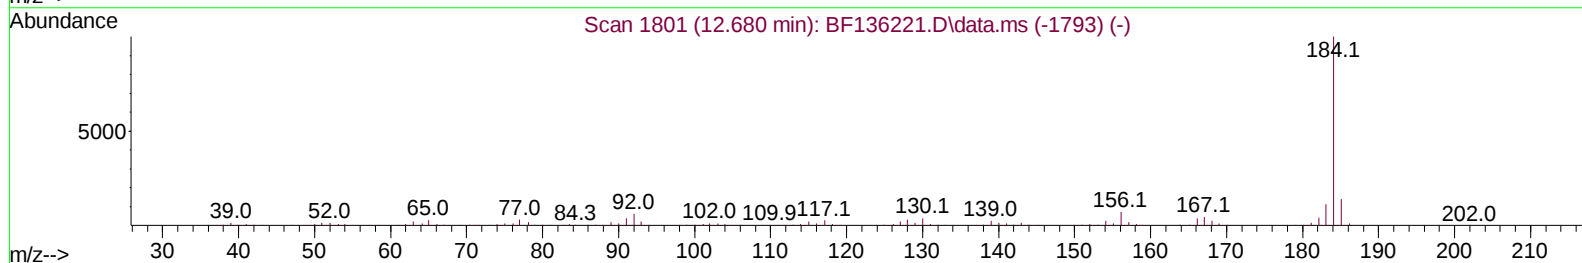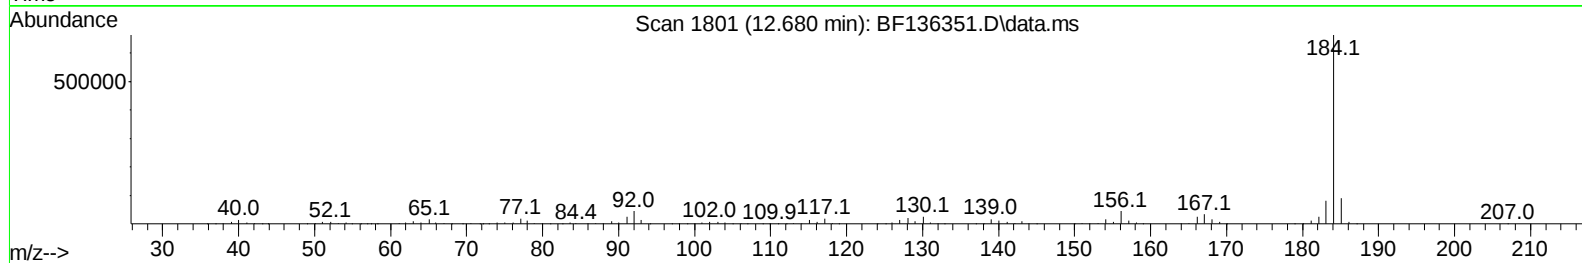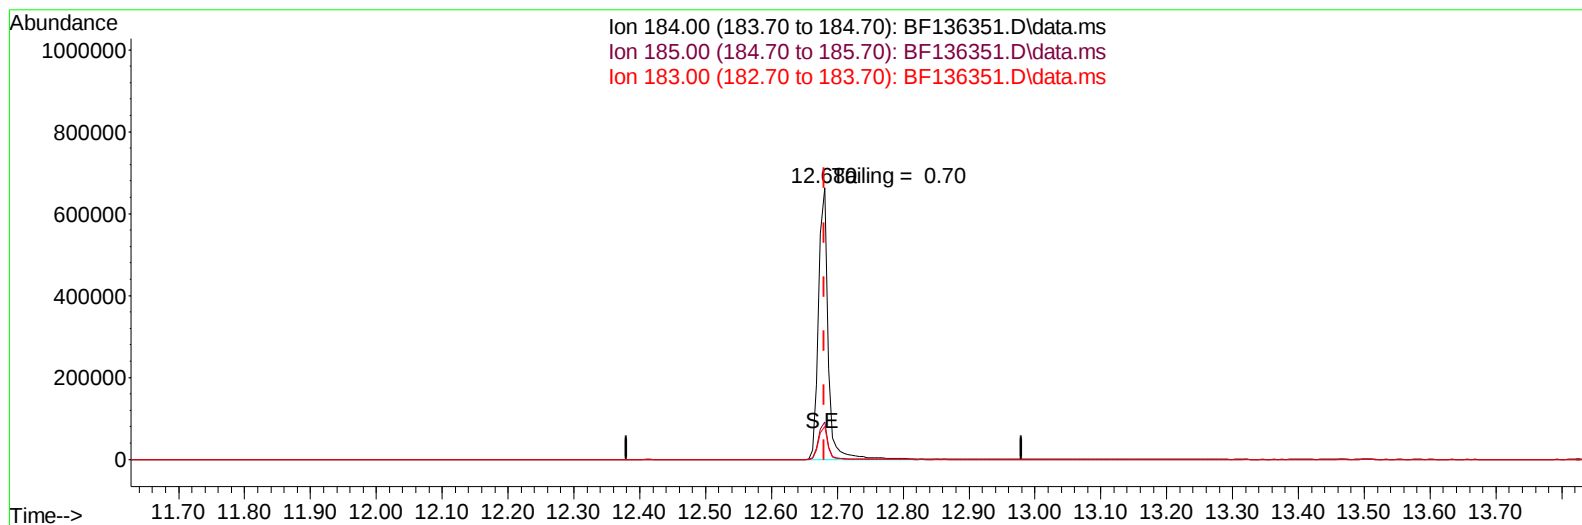

TIC: BF136351.D\data.ms

(77) Benzidine**12.680min (+ 0.000) 161064.62 ng****response 651315**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.74
183.00	11.20	12.12
0.00	0.00	0.00