

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
 Data File : BF136333.D
 Acq On : 01 Dec 2023 12:40
 Operator : CG\JU
 Sample : PB157138BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157138BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136333.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	10	14	21	rVB	47768	69310	1.13%	0.205%
2	3.946	310	316	320	rBV	50747	65838	1.07%	0.195%
3	5.087	506	510	518	rVB	41477	62764	1.02%	0.186%
4	5.457	567	573	576	rBV	4393743	4600531	74.99%	13.614%
5	6.451	735	742	744	rBV	3626743	4576116	74.59%	13.542%
6	6.804	799	802	806	rVB	1107466	916850	14.95%	2.713%
7	7.369	892	898	901	rBV	2724451	2967440	48.37%	8.782%
8	8.081	1014	1019	1023	rBV	1379376	1264988	20.62%	3.744%
9	9.163	1197	1203	1206	rBV	6051419	6134644	100.00%	18.154%
10	9.839	1313	1318	1321	rBV	1822246	1475447	24.05%	4.366%
11	10.633	1448	1453	1457	rBV	3273705	3401205	55.44%	10.065%
12	11.333	1568	1572	1575	rBV	1803471	1476016	24.06%	4.368%
13	12.933	1839	1844	1847	rBV	5573177	5292425	86.27%	15.662%
14	13.986	2019	2023	2032	rBV	784146	778337	12.69%	2.303%
15	15.468	2270	2275	2283	rBV	516650	709639	11.57%	2.100%




Sum of corrected areas: 33791550

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136333.D
Acq On : 01 Dec 2023 12:40
Operator : CG\JU
Sample : PB157138BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157138BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

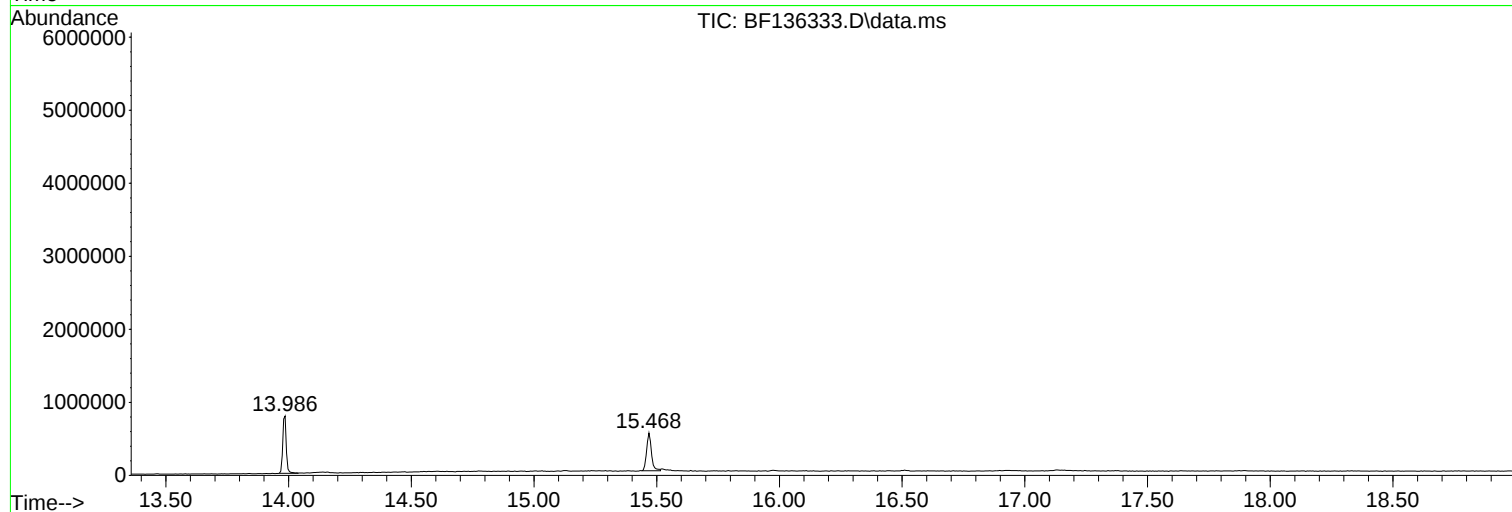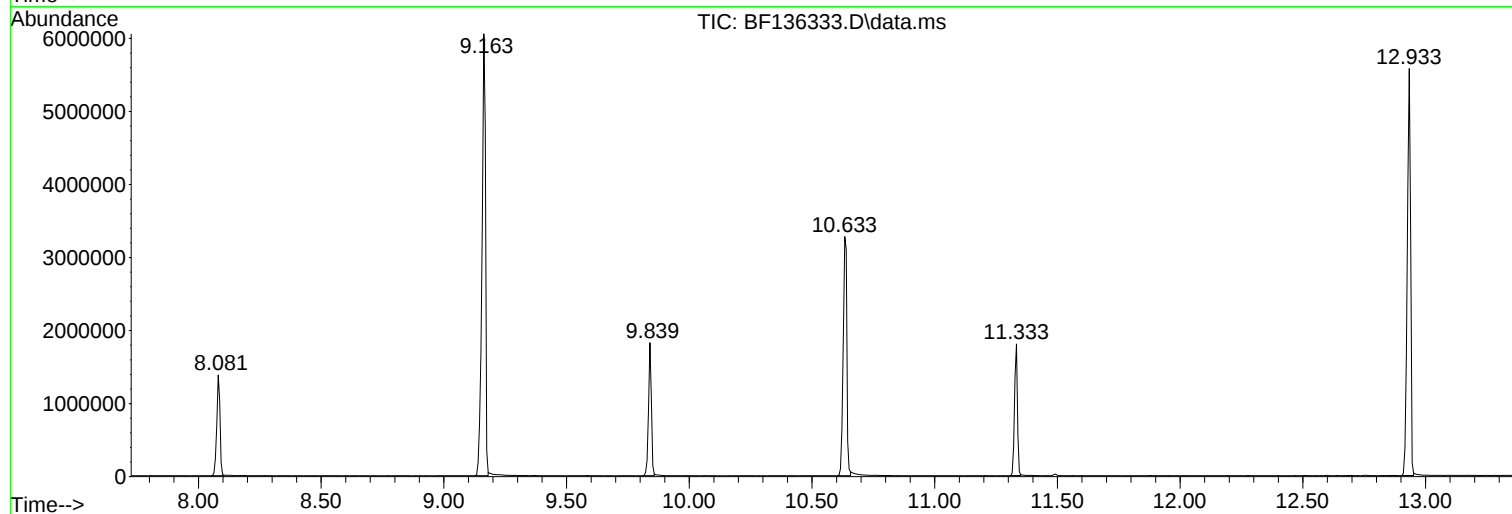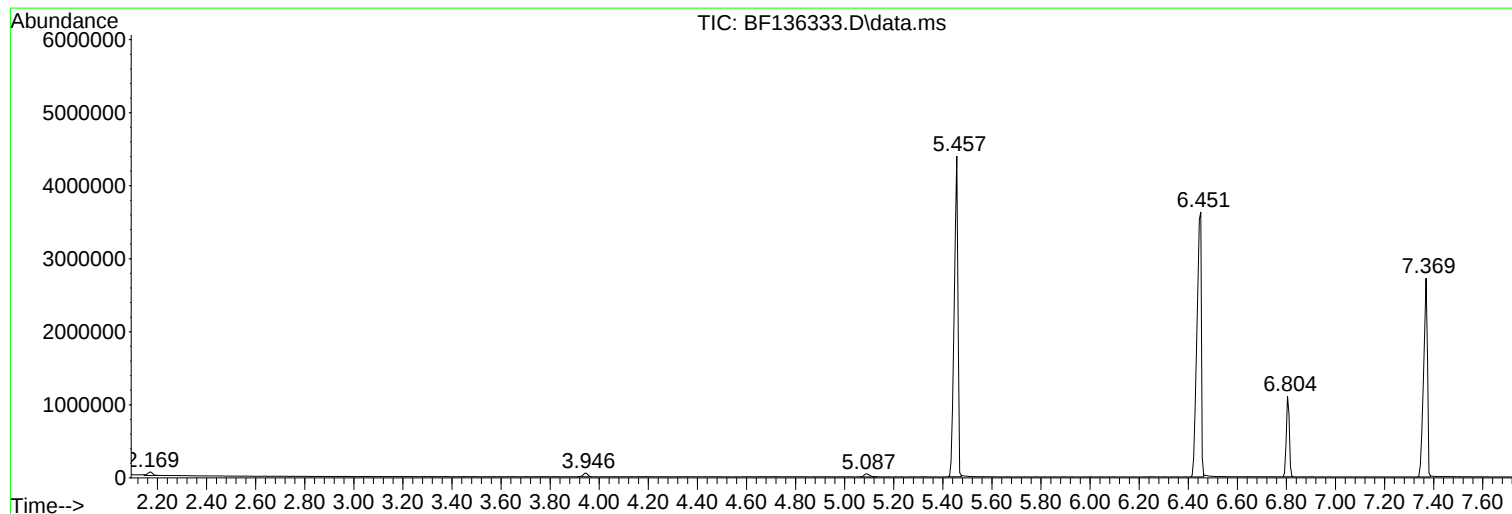

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136333.D
Acq On : 01 Dec 2023 12:40
Operator : CG\JU
Sample : PB157138BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157138BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136333.D
Acq On : 01 Dec 2023 12:40
Operator : CG\JU
Sample : PB157138BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157138BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------