

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
 Data File : BF136335.D
 Acq On : 01 Dec 2023 13:44
 Operator : CG\JU
 Sample : PB157087BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157087BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.940	311	315	323	rVB	51507	67495	1.13%	0.203%
2	5.087	505	510	518	rVB	40212	62648	1.05%	0.189%
3	5.457	567	573	576	rBV	4369688	4517566	75.38%	13.609%
4	6.445	735	741	744	rBV	3541355	4544103	75.82%	13.689%
5	6.804	798	802	806	rBV	1136389	913944	15.25%	2.753%
6	7.369	892	898	901	rBV	2712756	2920514	48.73%	8.798%
7	8.081	1014	1019	1023	rBV	1429295	1247262	20.81%	3.757%
8	9.163	1197	1203	1206	rBV	5960413	5993053	100.00%	18.054%
9	9.839	1312	1318	1321	rBV	1759179	1439618	24.02%	4.337%
10	10.633	1448	1453	1456	rBV	3486838	3277953	54.70%	9.875%
11	11.333	1568	1572	1575	rBV	1627987	1449791	24.19%	4.367%
12	12.933	1839	1844	1847	rBV	5709295	5232946	87.32%	15.764%
13	13.980	2018	2022	2032	rBV	809651	791465	13.21%	2.384%
14	15.468	2269	2275	2282	rBV	509241	736822	12.29%	2.220%




Sum of corrected areas: 33195180

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136335.D
Acq On : 01 Dec 2023 13:44
Operator : CG\JU
Sample : PB157087BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157087BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

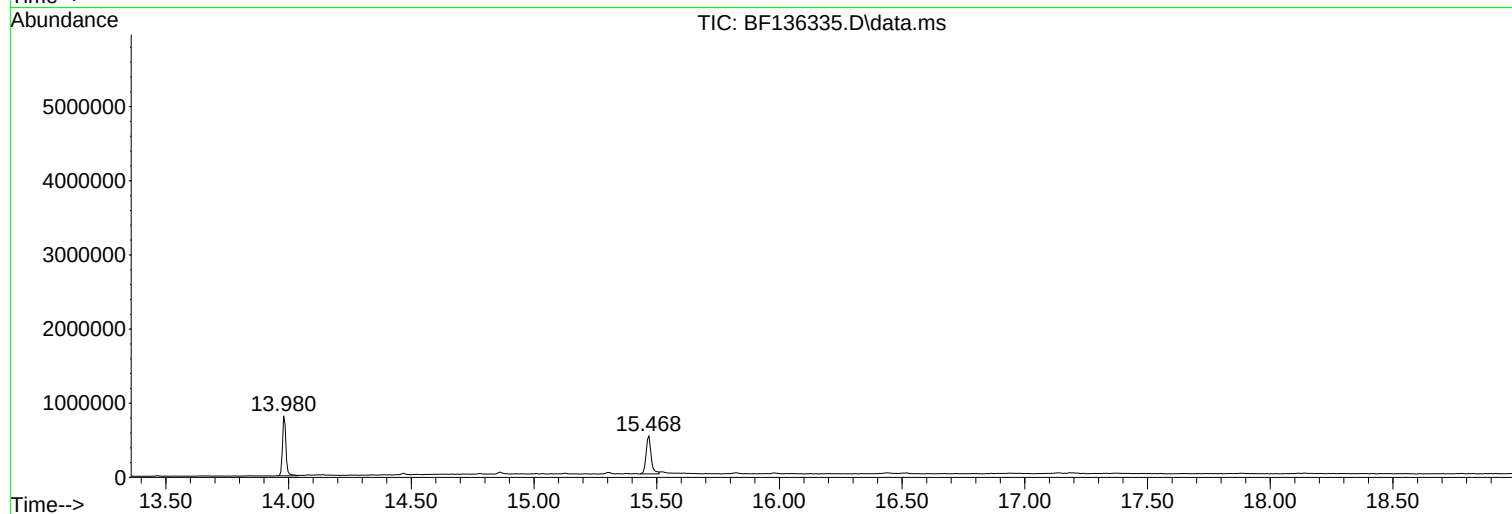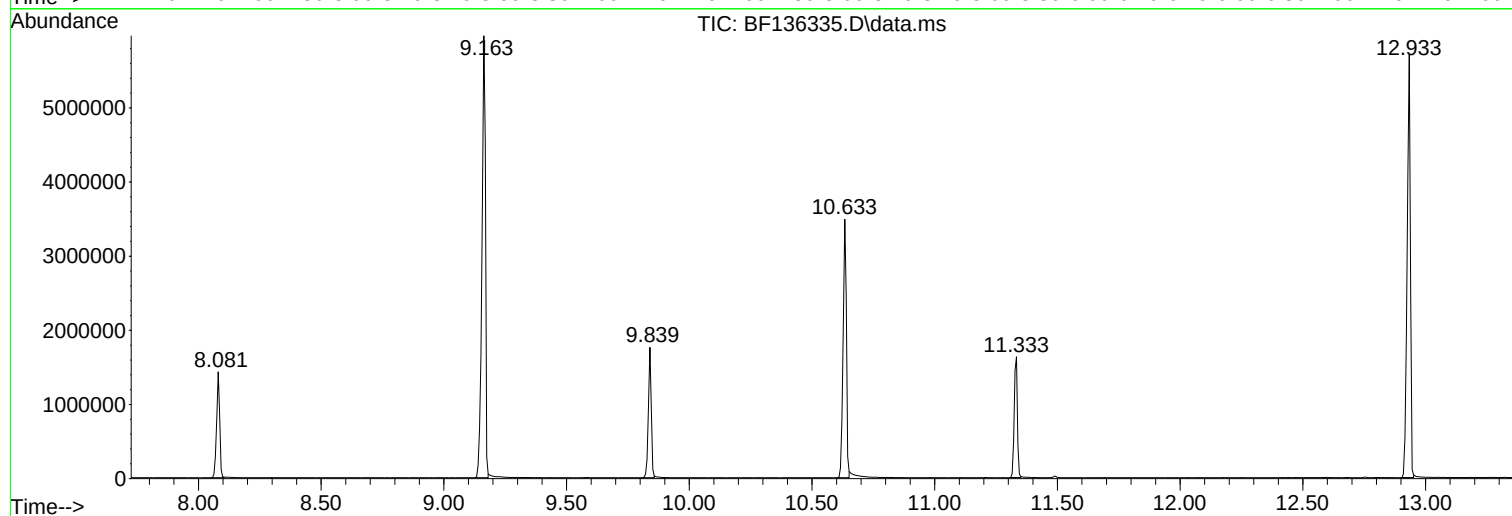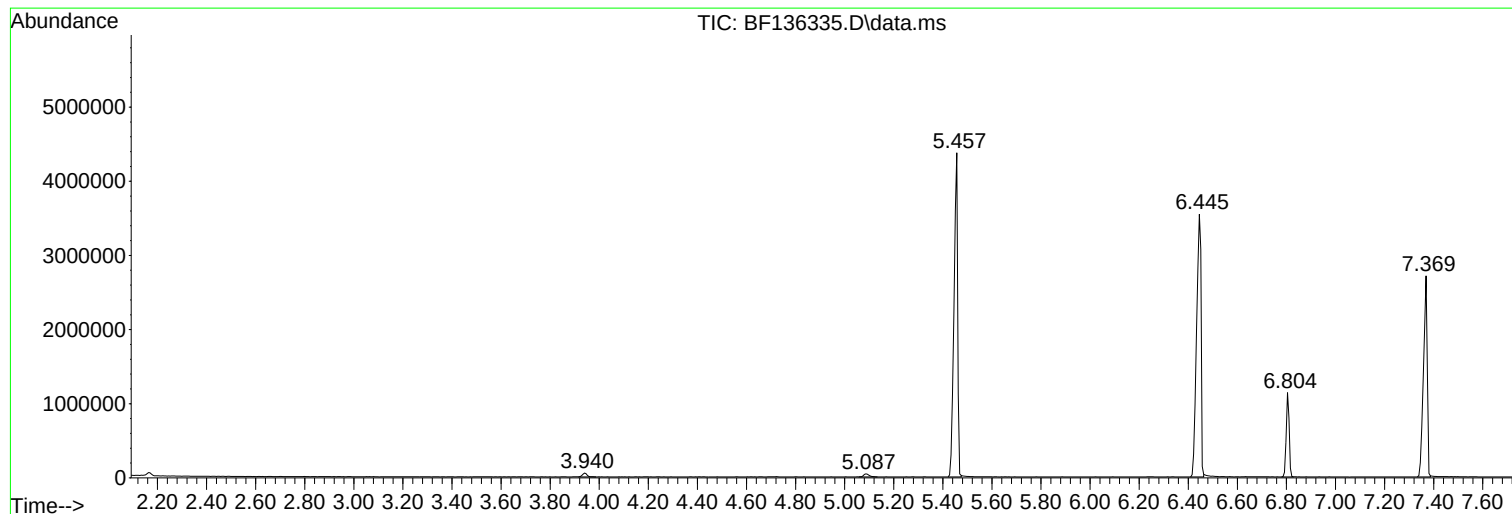

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136335.D
Acq On : 01 Dec 2023 13:44
Operator : CG\JU
Sample : PB157087BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157087BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136335.D
Acq On : 01 Dec 2023 13:44
Operator : CG\JU
Sample : PB157087BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157087BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------