

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
 Data File : BF136343.D
 Acq On : 01 Dec 2023 18:02
 Operator : CG\JU
 Sample : 05525-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136343.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.116	3	5	10	rVB	1724293	1652540	29.57%	7.228%
2	5.440	566	570	573	rBV	1411414	1199159	21.45%	5.245%
3	6.434	735	739	748	rBV	892223	738112	13.21%	3.228%
4	6.804	798	802	806	rBV	1024223	803072	14.37%	3.513%
5	7.369	892	898	901	rBV	2720721	2870439	51.36%	12.555%
6	8.081	1015	1019	1022	rBV	1384781	1106440	19.80%	4.839%
7	9.163	1197	1203	1206	rBV	6061351	5589259	100.00%	24.447%
8	9.839	1314	1318	1321	rBV	1522309	1199807	21.47%	5.248%
9	10.257	1386	1389	1397	rVB	153926	139316	2.49%	0.609%
10	10.628	1448	1452	1463	rBV	1819007	1790569	32.04%	7.832%
11	11.327	1567	1571	1575	rBV	1165808	974095	17.43%	4.261%
12	11.863	1658	1662	1666	rBV	90905	93984	1.68%	0.411%
13	12.927	1839	1843	1846	rBV	3831070	3410911	61.03%	14.919%
14	13.980	2018	2022	2031	rVB	657235	606797	10.86%	2.654%
15	15.462	2269	2274	2281	rBV	542183	688670	12.32%	3.012%




Sum of corrected areas: 22863170

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136343.D
Acq On : 01 Dec 2023 18:02
Operator : CG\JU
Sample : 05525-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

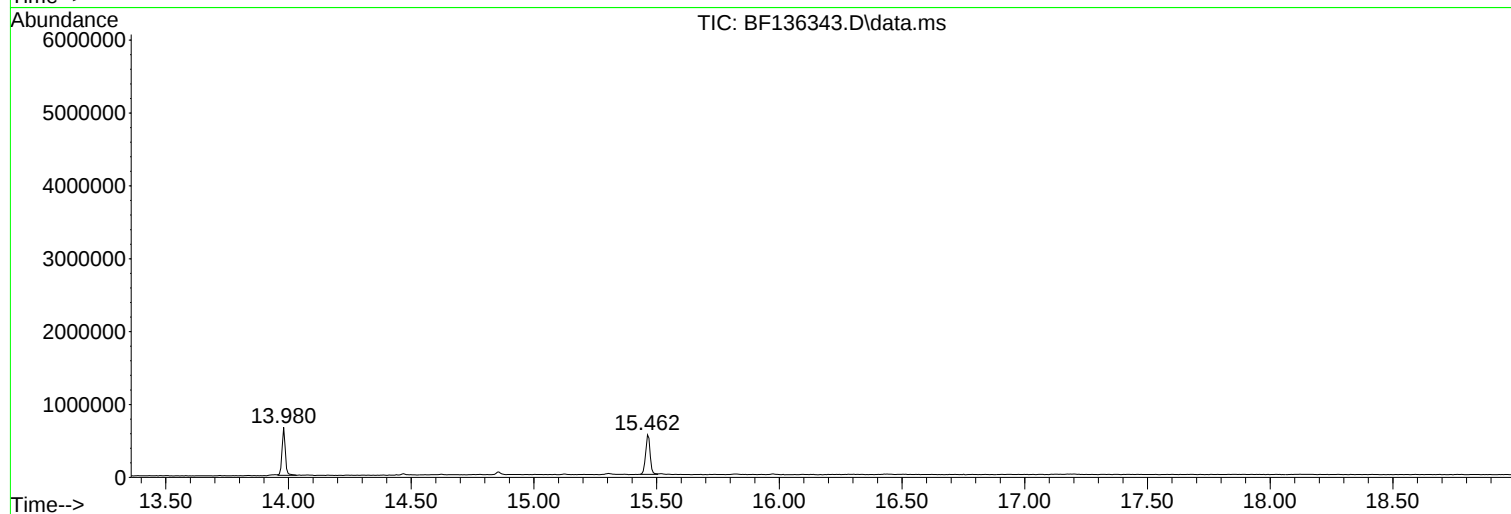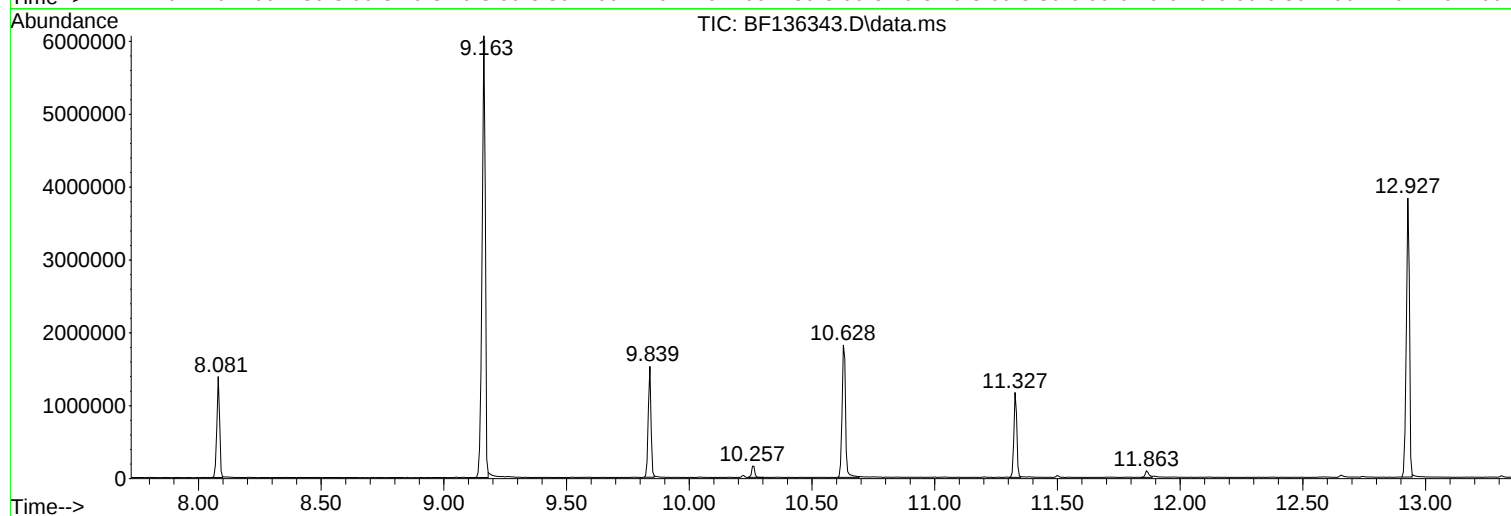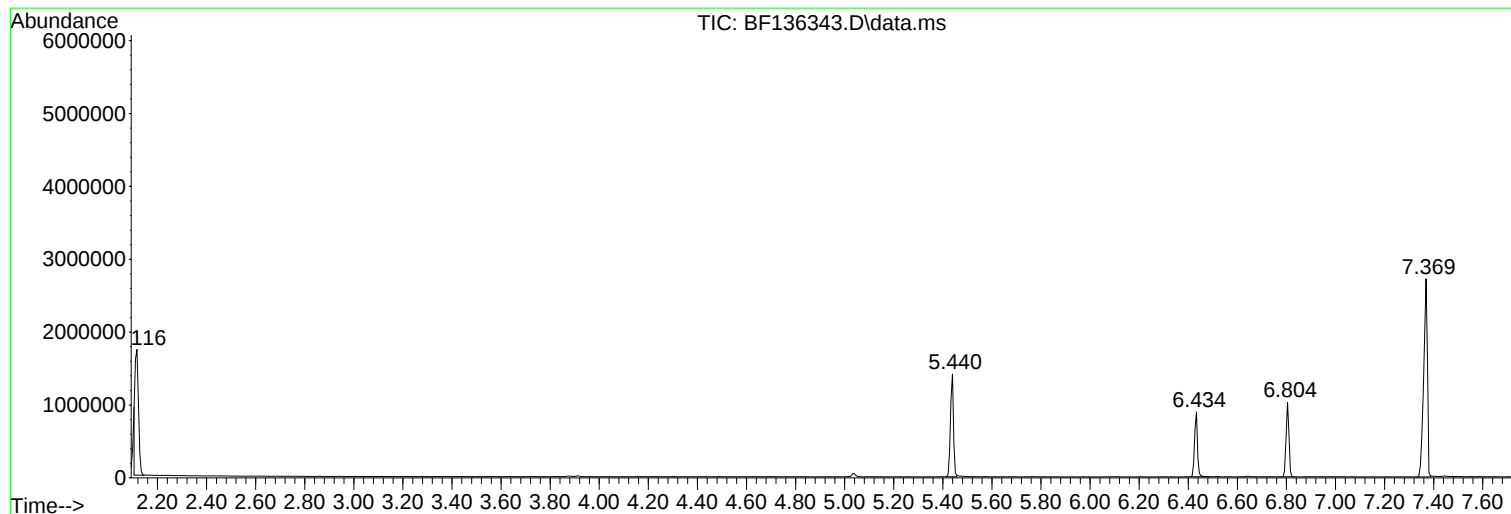

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136343.D
Acq On : 01 Dec 2023 18:02
Operator : CG\JU
Sample : 05525-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP10










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.116	41.16 ng	1652540	1,4-Dichlorobenzene-d4	6.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	33
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	12
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

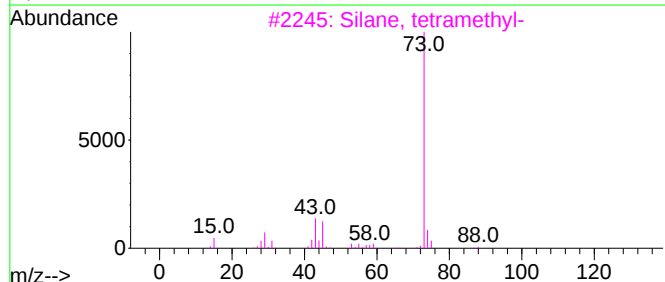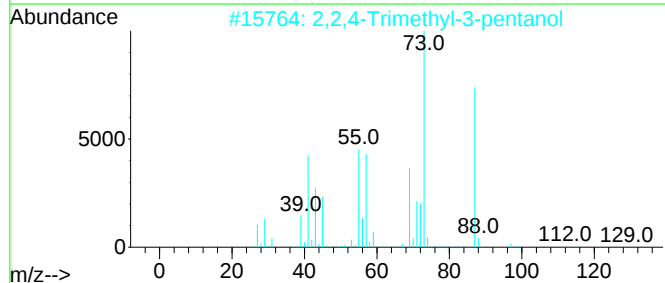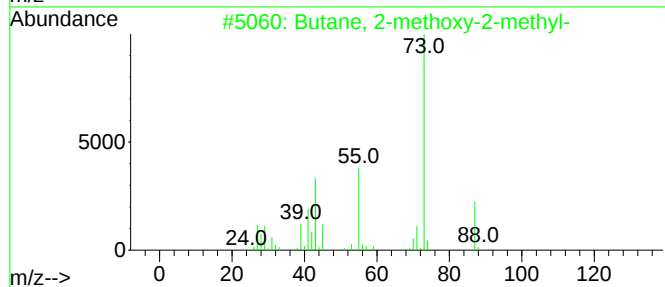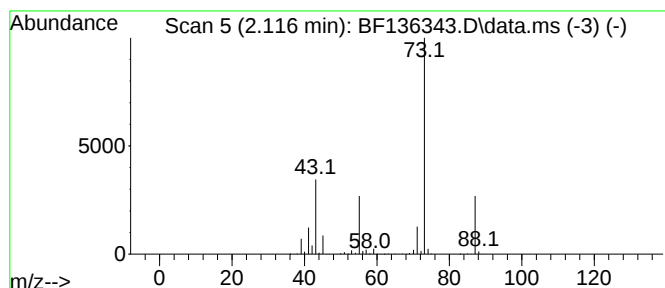

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136343.D
Acq On : 01 Dec 2023 18:02
Operator : CG\JU
Sample : 05525-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.116	41.2	ng	1652540	1	6.804	803072	20.0