

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
 Data File : BF136344.D
 Acq On : 01 Dec 2023 18:35
 Operator : CG\JU
 Sample : 05525-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP13

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	6	11	rVB	1760189	2024558	35.70%	8.538%
2	5.440	566	570	573	rBV	1469173	1239456	21.86%	5.227%
3	6.434	735	739	748	rBV	914613	771205	13.60%	3.252%
4	6.804	798	802	805	rBV	1021073	797616	14.07%	3.364%
5	7.369	892	898	901	rBV	2685156	2883364	50.84%	12.160%
6	8.081	1014	1019	1023	rBV	1340669	1104721	19.48%	4.659%
7	9.163	1197	1203	1206	rBV	6137667	5670890	100.00%	23.916%
8	9.839	1314	1318	1321	rBV	1559784	1213175	21.39%	5.116%
9	10.627	1448	1452	1462	rBV	1941980	1897297	33.46%	8.002%
10	11.327	1567	1571	1575	rBV	1171948	1030973	18.18%	4.348%
11	11.863	1659	1662	1666	rBV	90172	86518	1.53%	0.365%
12	12.927	1838	1843	1847	rBV	3676624	3677598	64.85%	15.510%
13	13.980	2018	2022	2035	rVB	655410	628546	11.08%	2.651%
14	15.462	2269	2274	2283	rBV	497881	685406	12.09%	2.891%




Sum of corrected areas: 23711323

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136344.D
Acq On : 01 Dec 2023 18:35
Operator : CG\JU
Sample : 05525-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

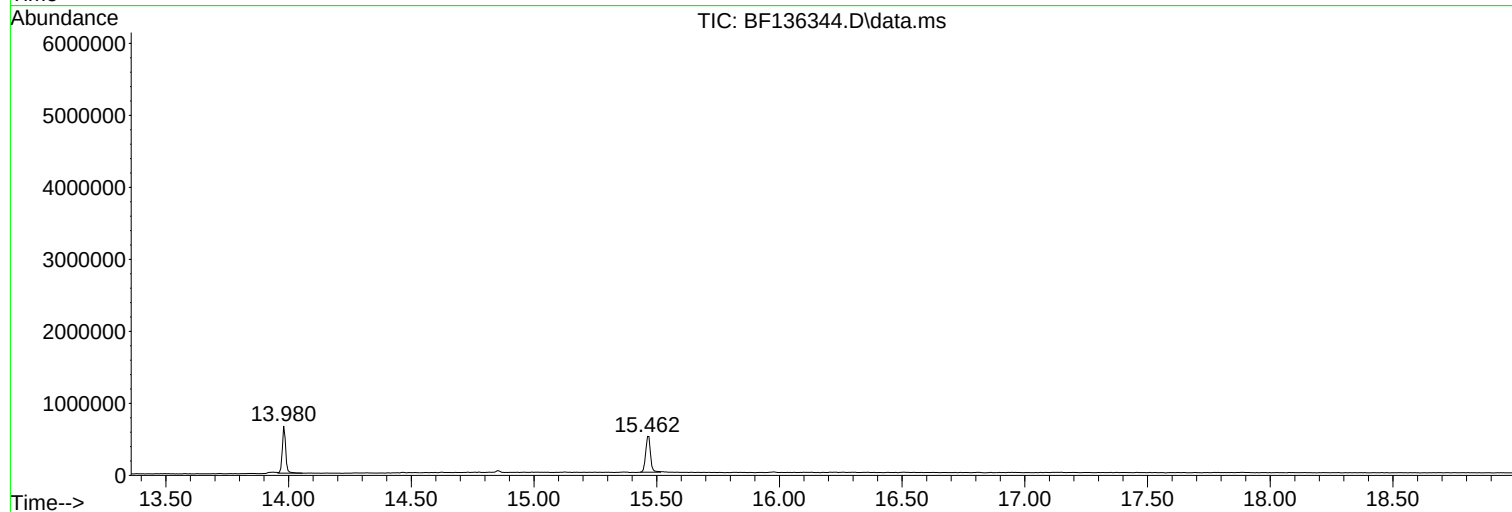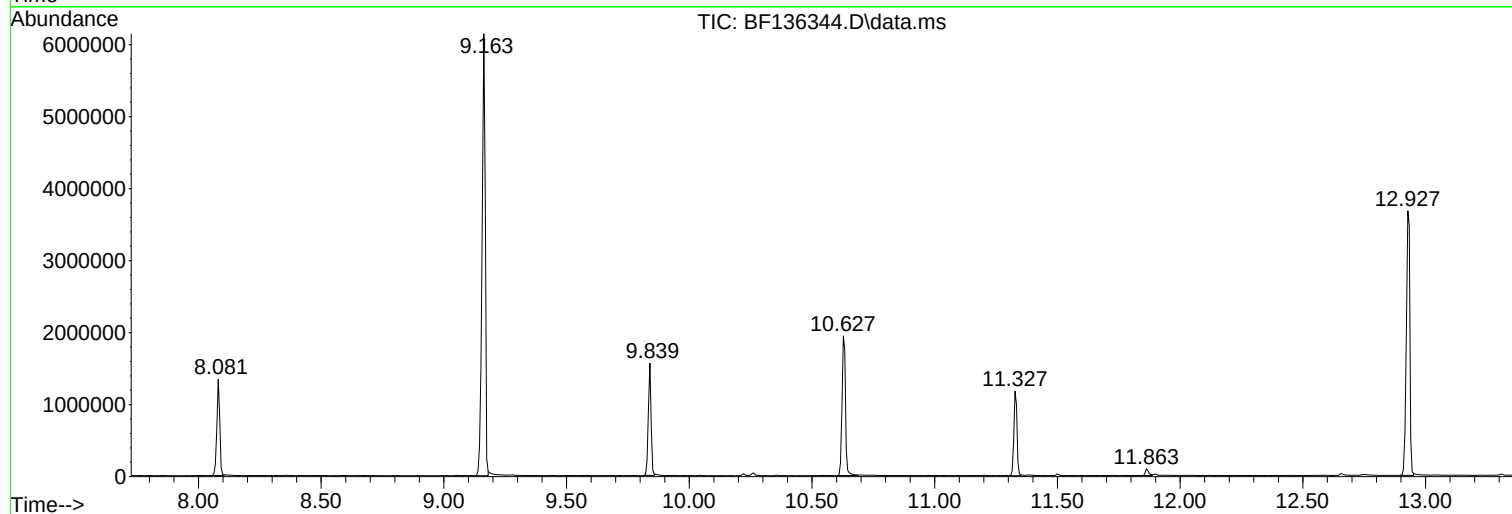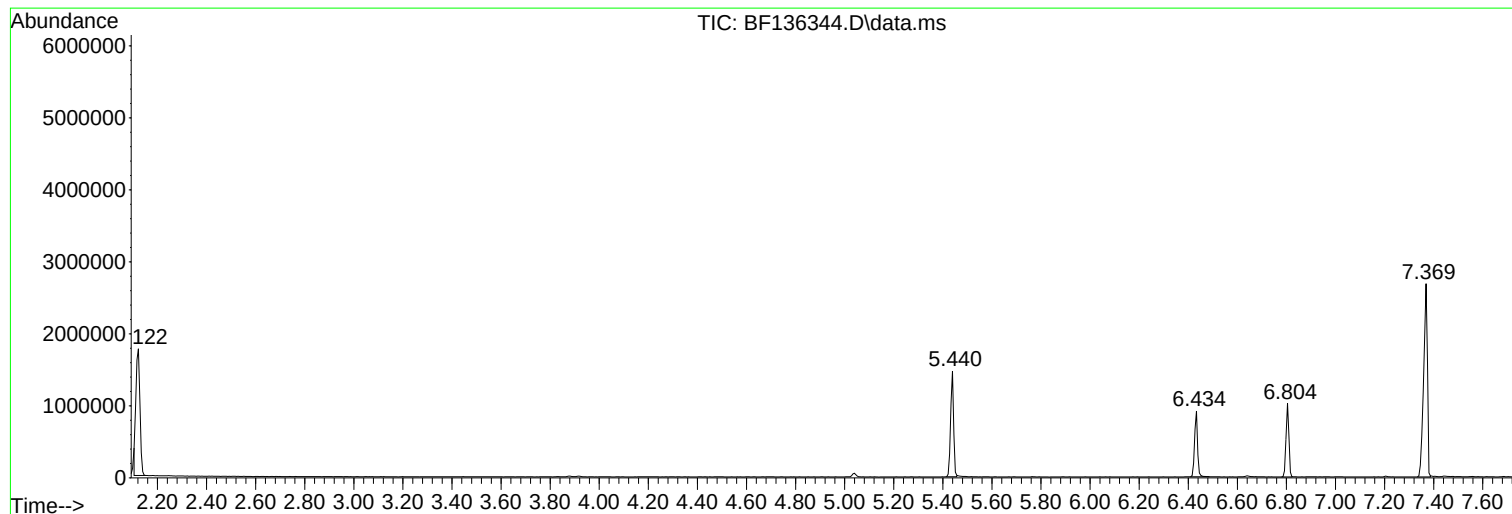

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136344.D
Acq On : 01 Dec 2023 18:35
Operator : CG\JU
Sample : 05525-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP13










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.122	50.77 ng	2024560	1,4-Dichlorobenzene-d4	6.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	37
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	23
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17

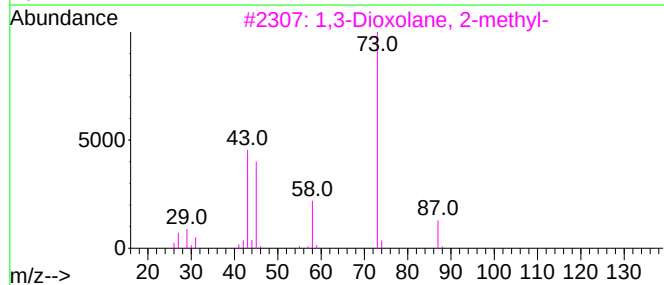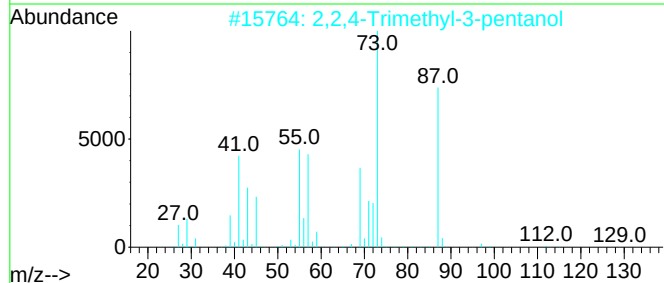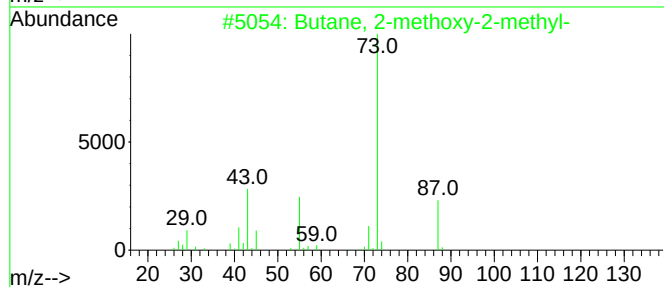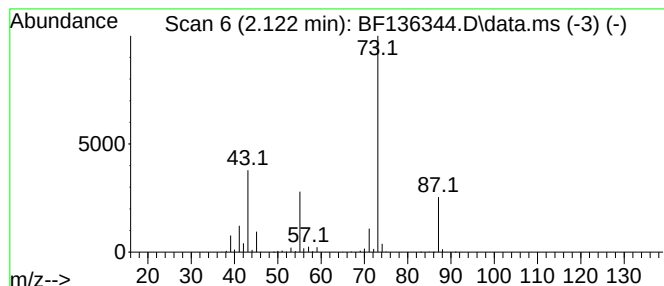

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136344.D
Acq On : 01 Dec 2023 18:35
Operator : CG\JU
Sample : 05525-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.122	50.8	ng	2024560	1	6.804	797616	20.0