

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
 Data File : BF136347.D
 Acq On : 01 Dec 2023 20:09
 Operator : CG\JU
 Sample : 05525-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.110	3	4	14	rVB	1540178	1358289	25.66%	6.370%
2	5.440	566	570	573	rBV	1190595	1075347	20.31%	5.043%
3	6.434	735	739	746	rBV	760124	658522	12.44%	3.088%
4	6.804	798	802	805	rBV	938964	732391	13.83%	3.435%
5	7.369	892	898	901	rBV	2644179	2636370	49.80%	12.364%
6	8.081	1014	1019	1022	rBV	1216014	999468	18.88%	4.687%
7	9.163	1197	1203	1206	rBV	6085374	5294107	100.00%	24.829%
8	9.839	1314	1318	1321	rBV	1354695	1097440	20.73%	5.147%
9	10.257	1385	1389	1394	rVB	168629	151989	2.87%	0.713%
10	10.627	1448	1452	1466	rBV	1855622	1746965	33.00%	8.193%
11	11.327	1567	1571	1575	rBV	1142409	919446	17.37%	4.312%
12	11.863	1659	1662	1666	rBV	69464	64589	1.22%	0.303%
13	12.927	1838	1843	1846	rBV	3712339	3412289	64.45%	16.003%
14	13.980	2018	2022	2033	rVB	586567	549038	10.37%	2.575%
15	15.462	2269	2274	2282	rBV	473552	626343	11.83%	2.937%




Sum of corrected areas: 21322593

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136347.D
Acq On : 01 Dec 2023 20:09
Operator : CG\JU
Sample : 05525-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

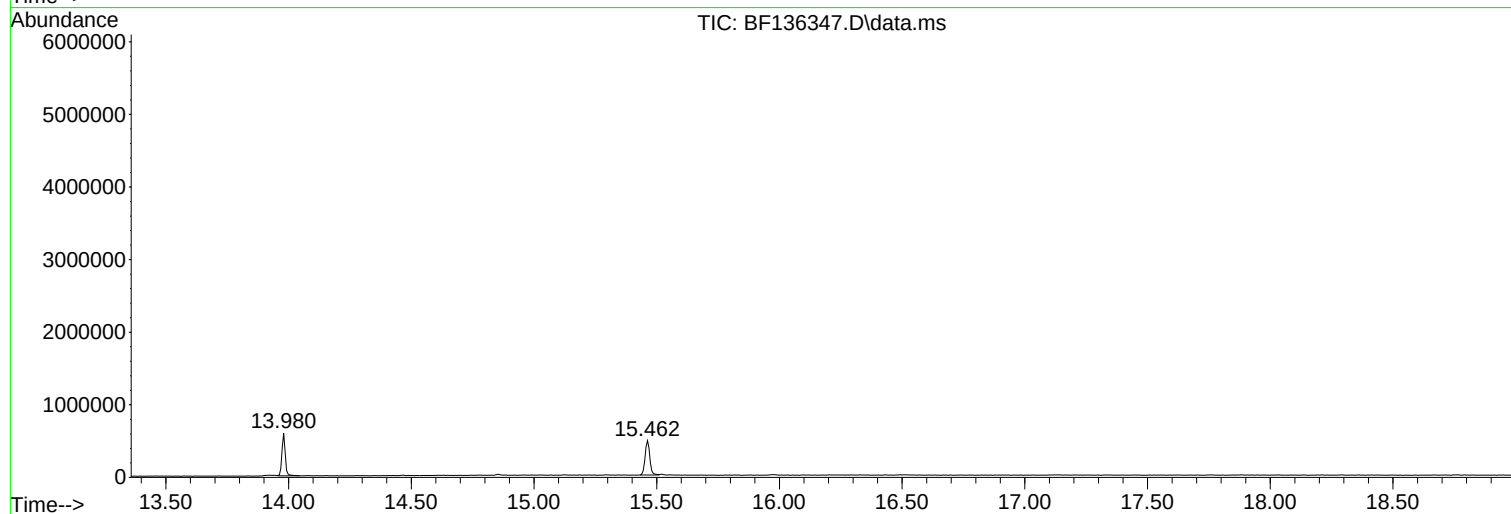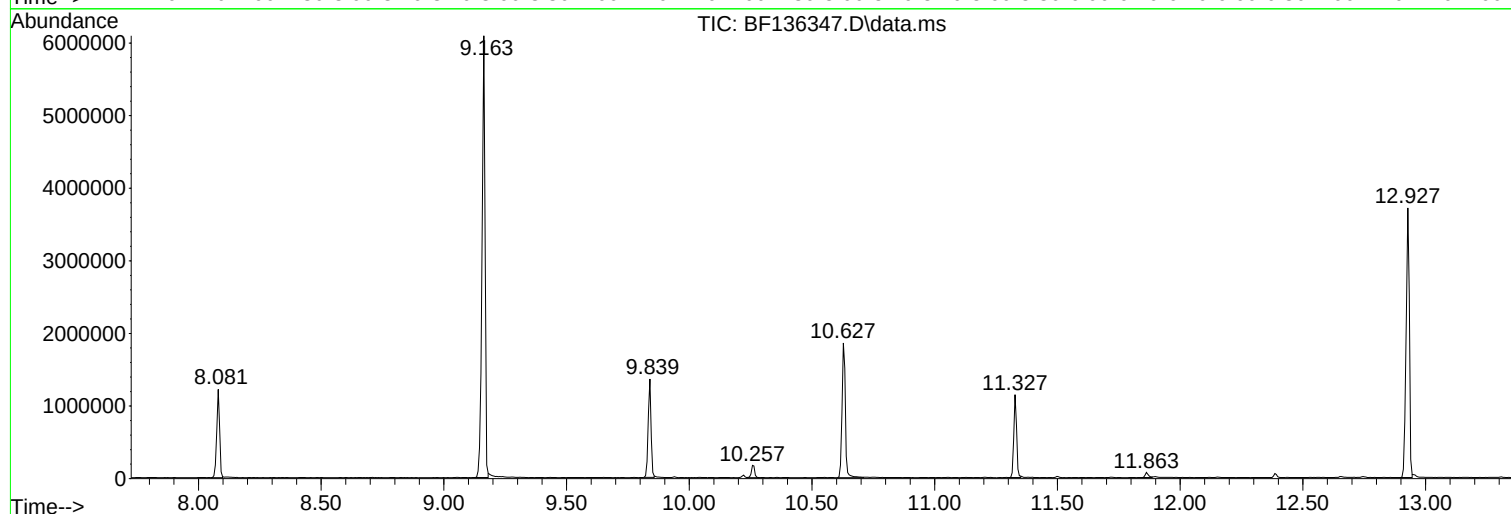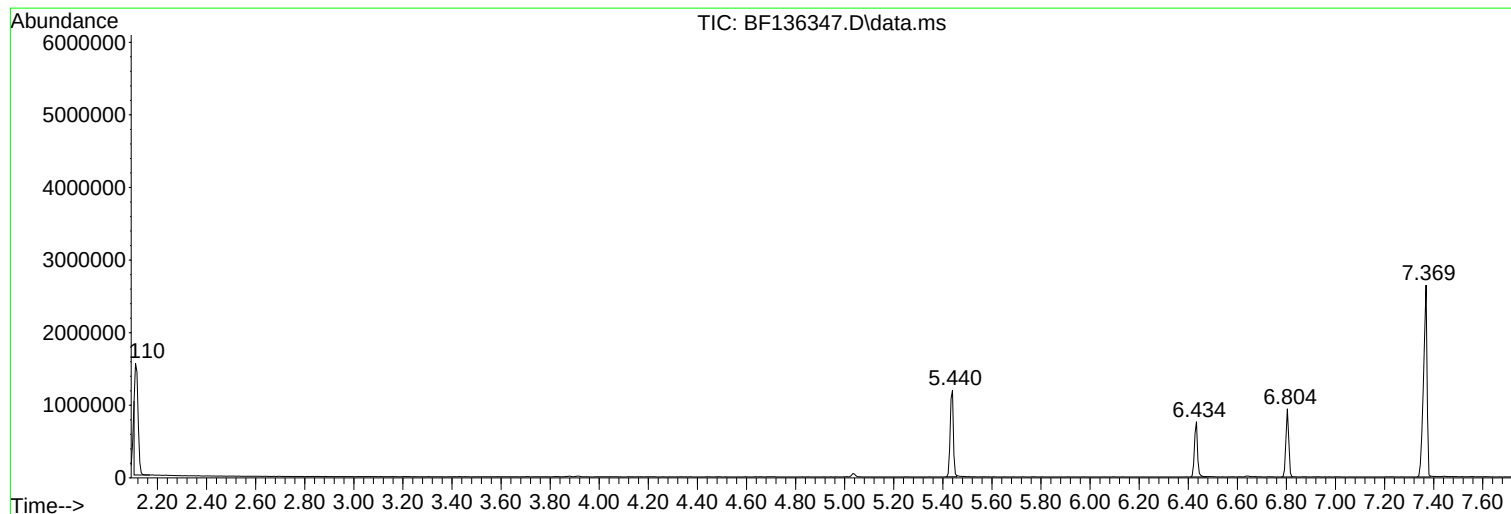

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136347.D
Acq On : 01 Dec 2023 20:09
Operator : CG\JU
Sample : 05525-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP14










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.110	37.09 ng	1358290	1,4-Dichlorobenzene-d4	6.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			1-(2-Methoxyethoxy)-2-methyl-2-p...	162	C8H18O3	1000364-24-4	17
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	16
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

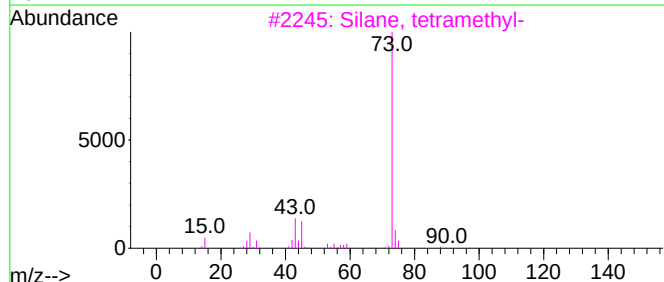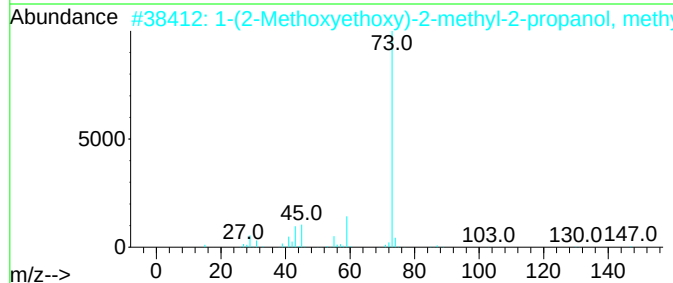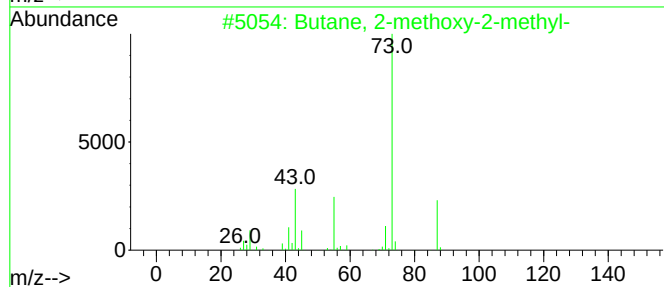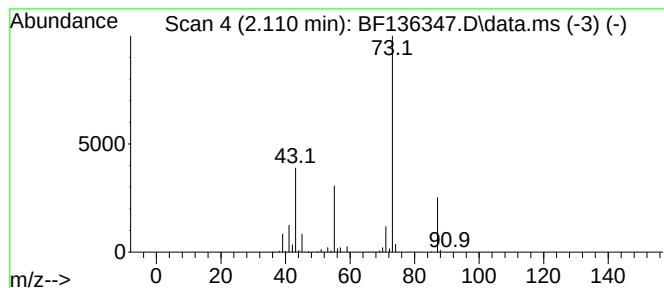

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136347.D
Acq On : 01 Dec 2023 20:09
Operator : CG\JU
Sample : 05525-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.110	37.1	ng	1358290	1	6.804	732391	20.0