

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
 Data File : BF136353.D
 Acq On : 02 Dec 2023 00:38
 Operator : CG\JU
 Sample : PB157389BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB157389BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	11	15	19	rVB	45480	55743	1.08%	0.201%
2	5.081	505	509	515	rBV	44167	65468	1.27%	0.236%
3	5.457	567	573	576	rBV	3840656	4186399	81.27%	15.088%
4	6.446	734	741	744	rBV	3499794	4025060	78.14%	14.506%
5	6.804	798	802	805	rBV	1114436	847873	16.46%	3.056%
6	7.369	892	898	901	rBV	2525632	2594867	50.38%	9.352%
7	8.081	1014	1019	1022	rBV	1353726	1160619	22.53%	4.183%
8	9.163	1197	1203	1206	rBV	5827637	5150993	100.00%	18.564%
9	9.839	1312	1318	1321	rBV	1573803	1253339	24.33%	4.517%
10	10.633	1448	1453	1456	rBV	2667321	2435575	47.28%	8.778%
11	11.328	1567	1571	1575	rBV	1286355	1043985	20.27%	3.762%
12	12.927	1839	1843	1846	rBV	3813500	3401950	66.04%	12.260%
13	13.980	2018	2022	2033	rBV	740641	686280	13.32%	2.473%
14	14.863	2168	2172	2177	rBV2	42608	56133	1.09%	0.202%
15	15.463	2267	2274	2281	rBV	521964	718812	13.95%	2.591%
16	15.521	2281	2284	2294	rVB	40850	64301	1.25%	0.232%




Sum of corrected areas: 27747397

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136353.D
Acq On : 02 Dec 2023 00:38
Operator : CG\JU
Sample : PB157389BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

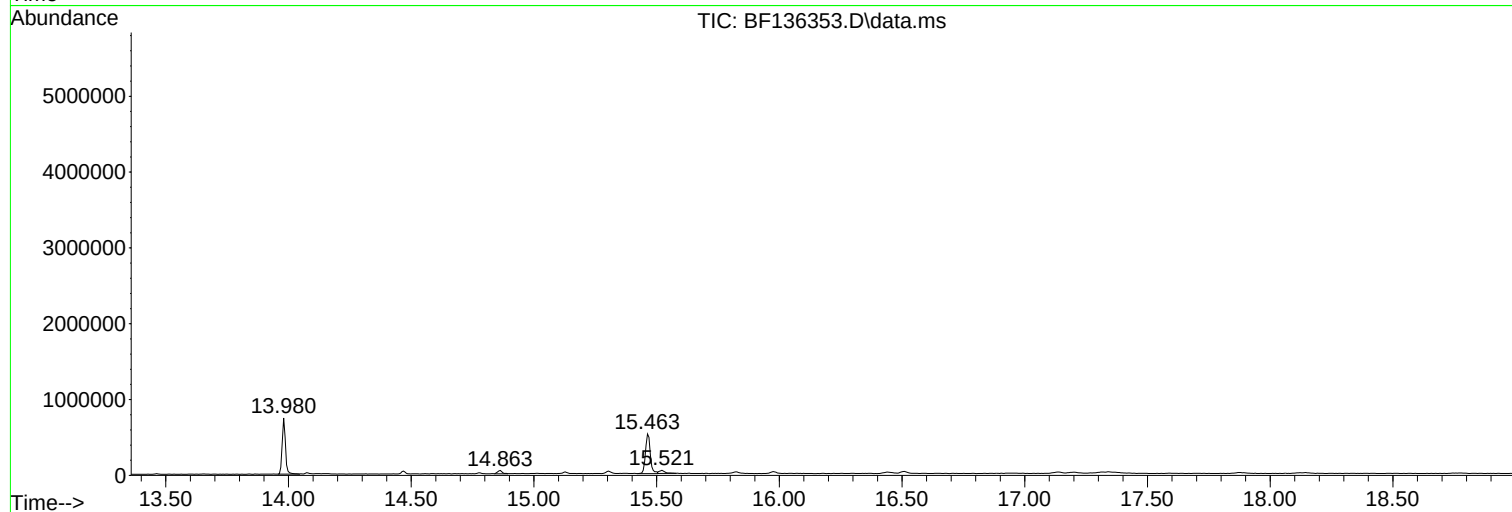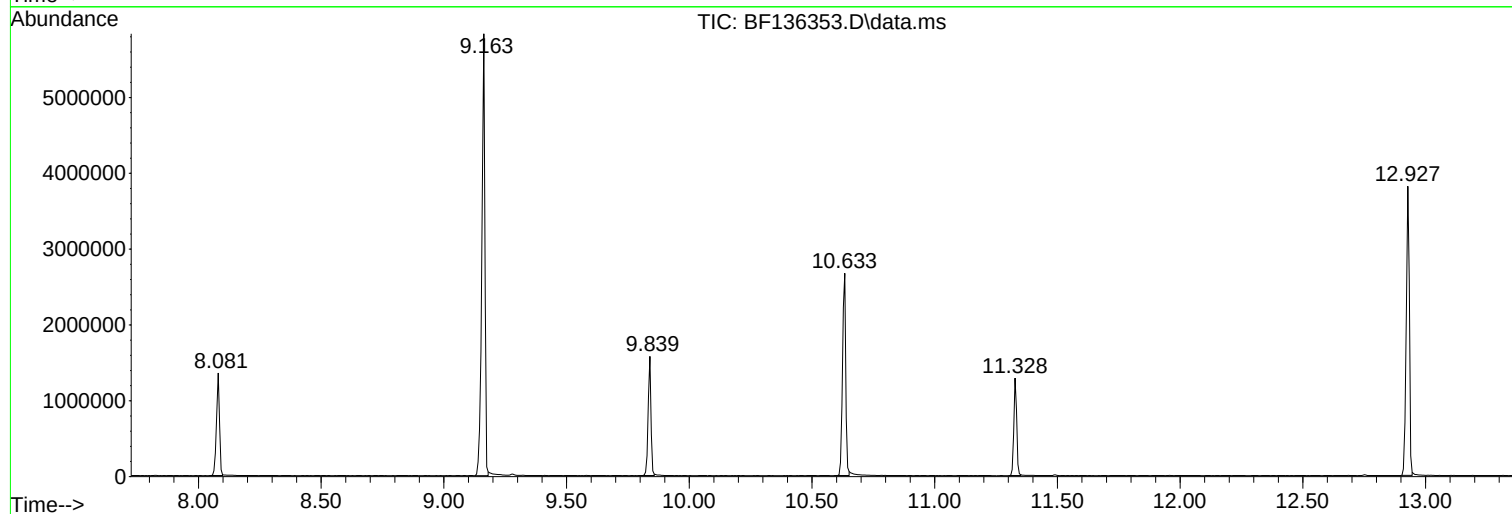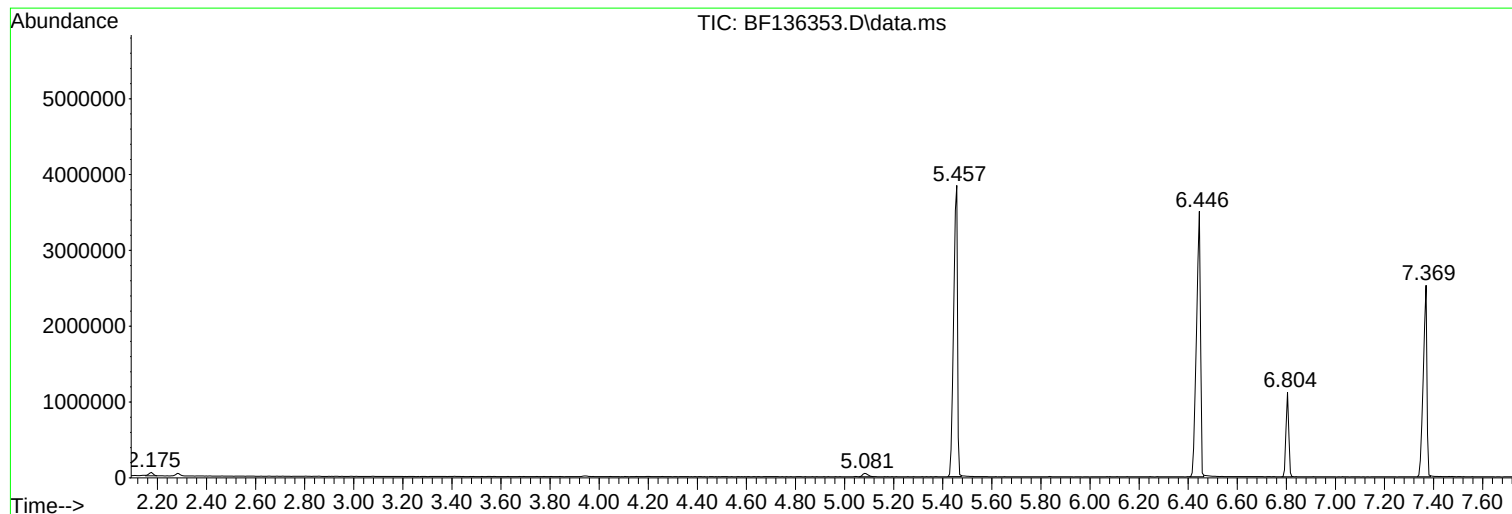

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136353.D
Acq On : 02 Dec 2023 00:38
Operator : CG\JU
Sample : PB157389BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136353.D
Acq On : 02 Dec 2023 00:38
Operator : CG\JU
Sample : PB157389BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB157389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------