

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
 Data File : BF136373.D
 Acq On : 02 Dec 2023 11:29
 Operator : CG\JU
 Sample : 05434-09
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF136373.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.893	304	307	312	rVB2	8513	10401	1.63%	0.175%
2	5.028	497	500	504	rBV2	11610	12164	1.90%	0.204%
3	5.434	565	569	575	rBV	629383	532580	83.32%	8.945%
4	6.434	735	739	751	rBV	555122	447416	69.99%	7.514%
5	6.804	799	802	806	rBV	651379	530556	83.00%	8.911%
6	7.363	893	897	905	rBV	306121	261194	40.86%	4.387%
7	8.081	1016	1019	1023	rBV	679925	541471	84.71%	9.094%
8	9.157	1199	1202	1209	rBV	534385	424939	66.48%	7.137%
9	9.839	1314	1318	1321	rBV	702406	539736	84.44%	9.065%
10	10.627	1449	1452	1457	rBV	307750	260058	40.68%	4.368%
11	10.822	1482	1485	1488	rBV2	4952	7417	1.16%	0.125%
12	11.327	1568	1571	1575	rBV	656930	615204	96.24%	10.332%
13	11.398	1581	1583	1587	rVB2	4851	6820	1.07%	0.115%
14	11.863	1659	1662	1666	rBV3	24219	26190	4.10%	0.440%
15	12.468	1762	1765	1769	rBV6	6260	7758	1.21%	0.130%
16	12.545	1775	1778	1781	rBV	39551	39379	6.16%	0.661%
17	12.774	1814	1817	1820	rVB	33762	32082	5.02%	0.539%
18	12.833	1824	1827	1832	rBV4	8549	13117	2.05%	0.220%
19	12.927	1839	1843	1846	rBV	635633	581273	90.94%	9.762%
20	13.110	1867	1874	1877	rBV6	10411	20734	3.24%	0.348%
21	13.210	1889	1891	1895	rBV4	7222	10907	1.71%	0.183%
22	13.404	1921	1924	1926	rBV3	9462	9915	1.55%	0.167%
23	13.510	1940	1942	1945	rBV4	8325	8100	1.27%	0.136%
24	13.986	2018	2023	2026	rBV	631604	639213	100.00%	10.736%
25	15.468	2271	2275	2283	rVB	306823	375540	58.75%	6.307%




Sum of corrected areas: 5954164

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136373.D
Acq On : 02 Dec 2023 11:29
Operator : CG\JU
Sample : 05434-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

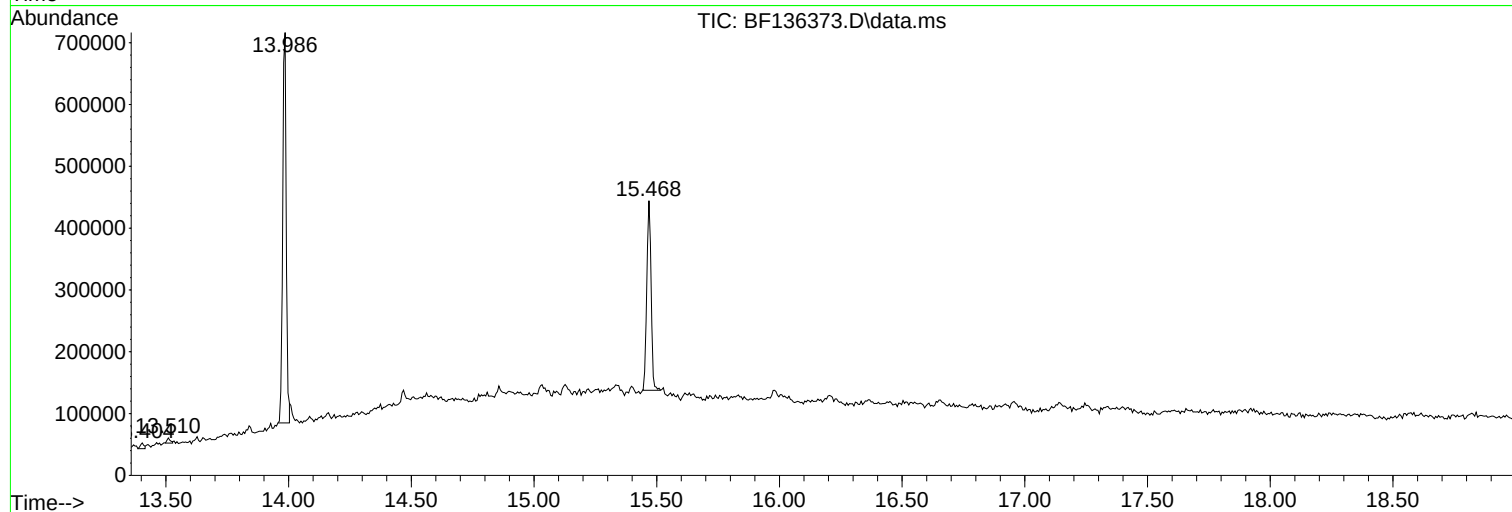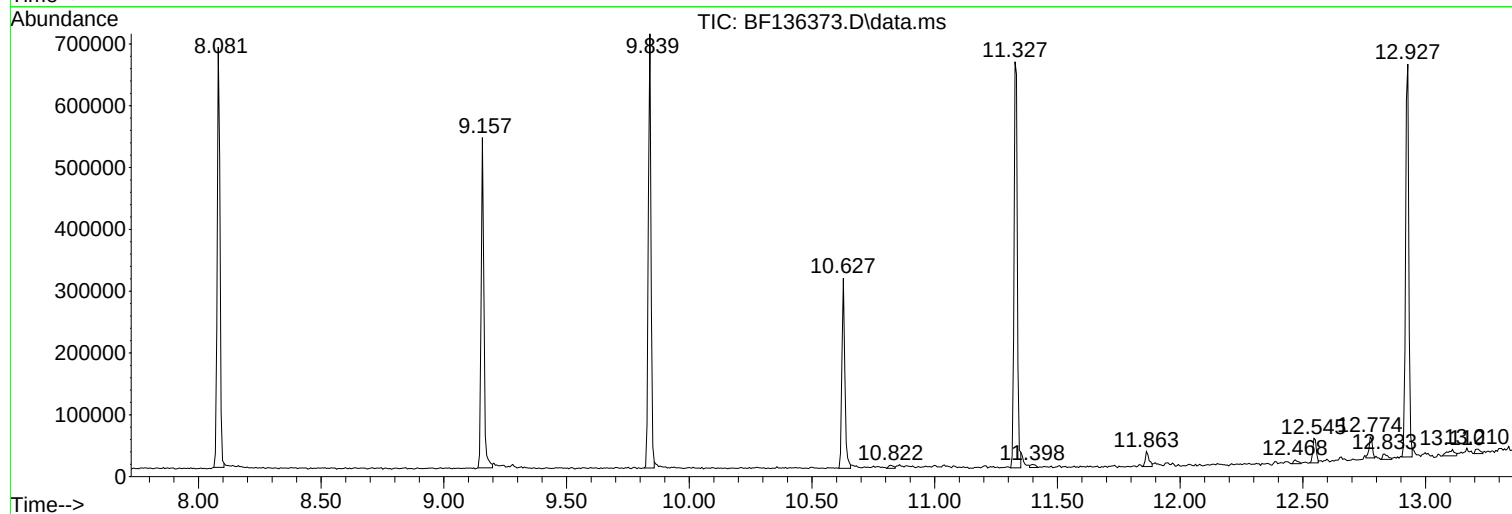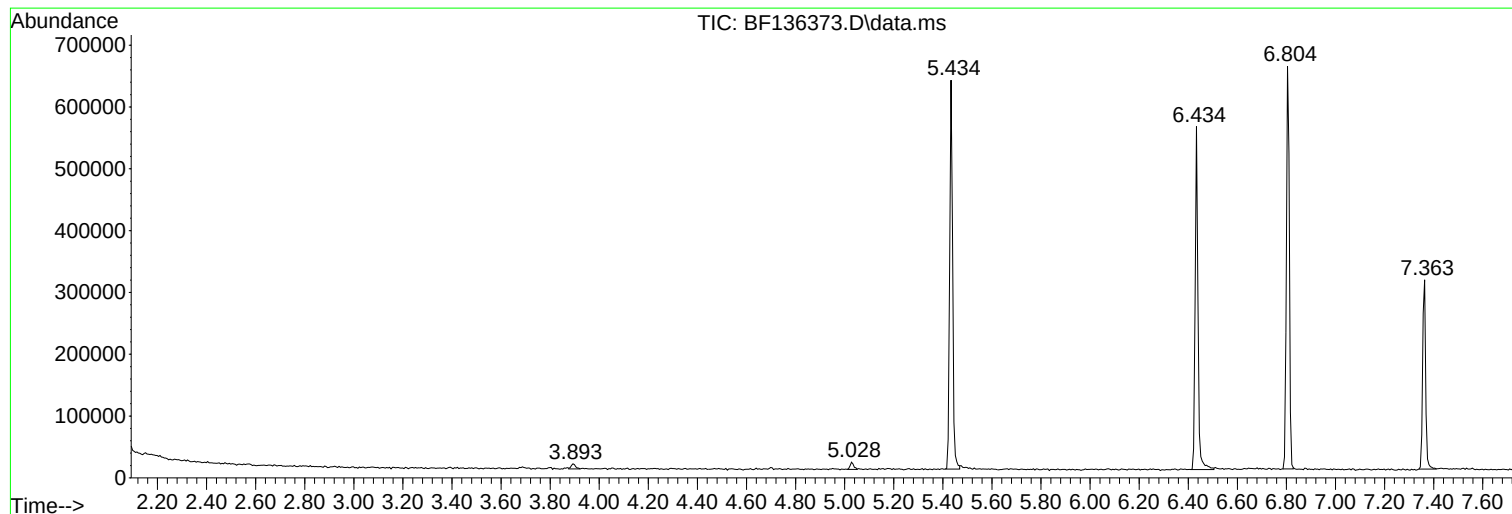

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136373.D
Acq On : 02 Dec 2023 11:29
Operator : CG\JU
Sample : 05434-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136373.D
Acq On : 02 Dec 2023 11:29
Operator : CG\JU
Sample : 05434-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------