


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136328.D
Acq On : 01 Dec 2023 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 28 03:04:20 2023



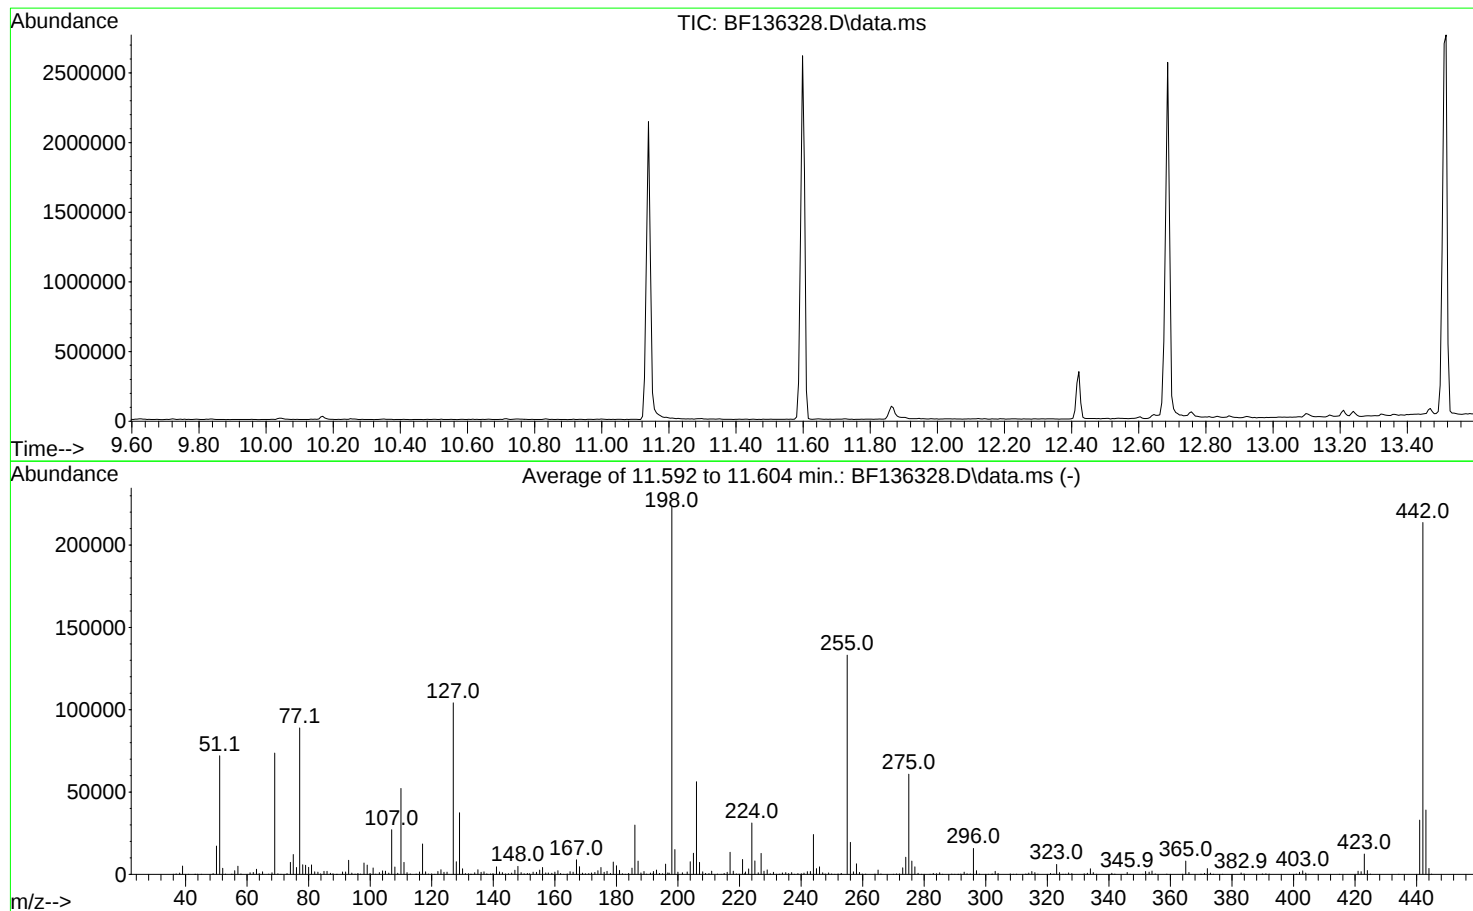


AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	72069	PASS
68	69	0.00	2	1.3	980	PASS
69	198	0.00	100	33.0	73691	PASS
70	69	0.00	2	0.5	359	PASS
127	198	10	80	46.6	104152	PASS
197	198	0.00	2	0.4	846	PASS
198	198	100	100	100.0	223445	PASS
199	198	5	9	6.8	15104	PASS
275	198	10	60	27.2	60875	PASS
365	198	1	100	3.6	8024	PASS
441	198	0.01	100	14.7	32941	PASS
442	442	50	100	100.0	213725	PASS
443	442	15	24	18.3	39106	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
lon 265.70 (265.40 to 266.40): BF136328.D\data.ms
lon 268.00 (267.70 to 268.70): BF136328.D\data.ms
lon 264.00 (263.70 to 264.70): BF136328.D\data.ms
```

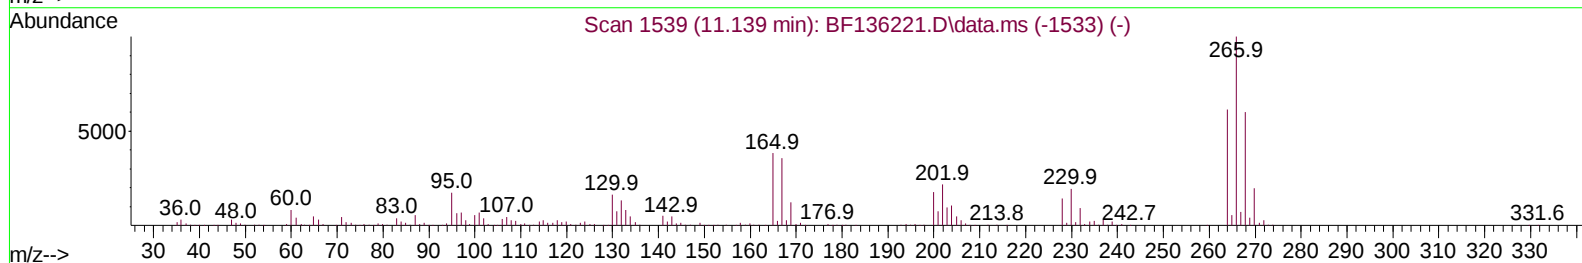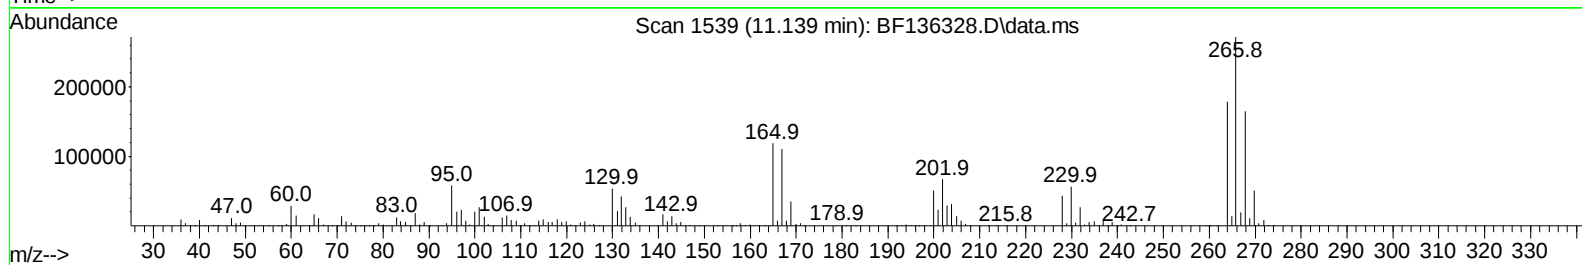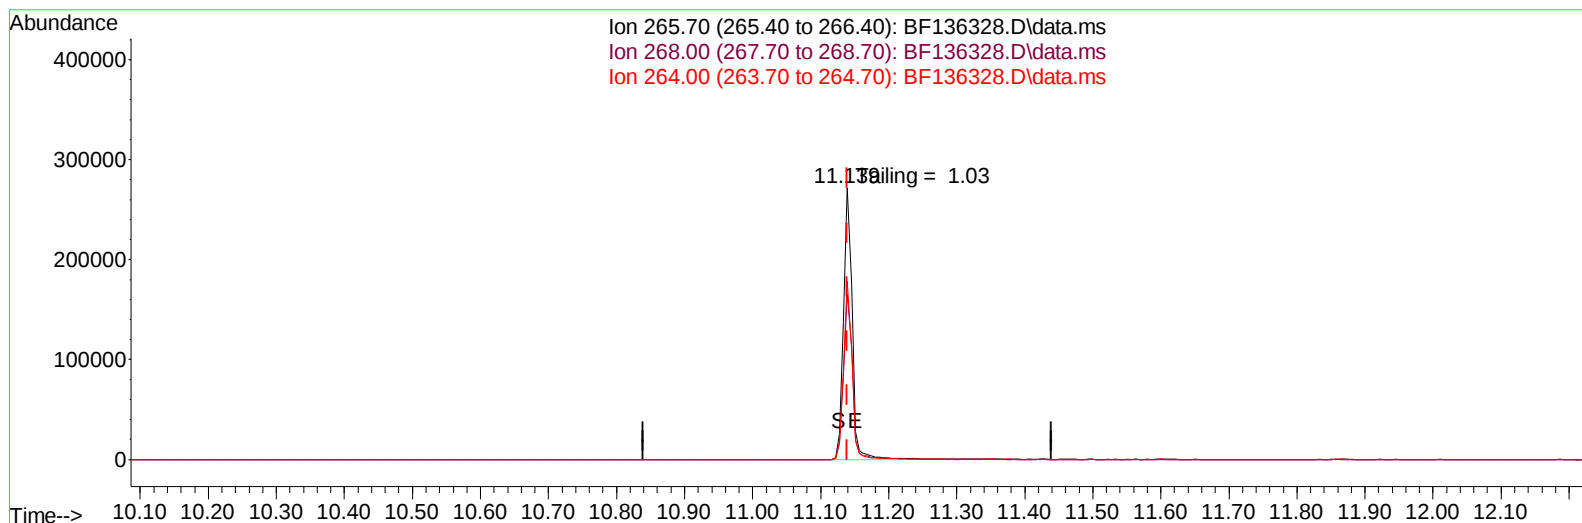

TIC: BF136328.D\data.ms




response **237803**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	60.87
264.00	61.40	65.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136328.D
Acq On : 01 Dec 2023 10:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 02 01:09:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

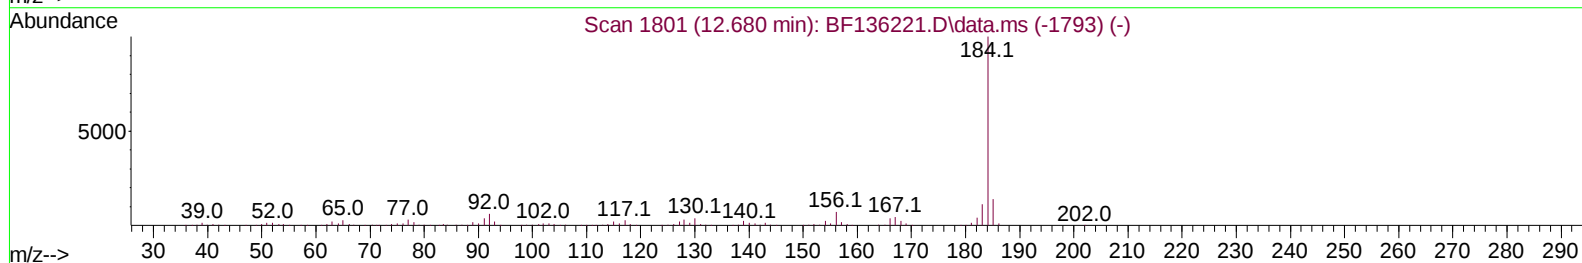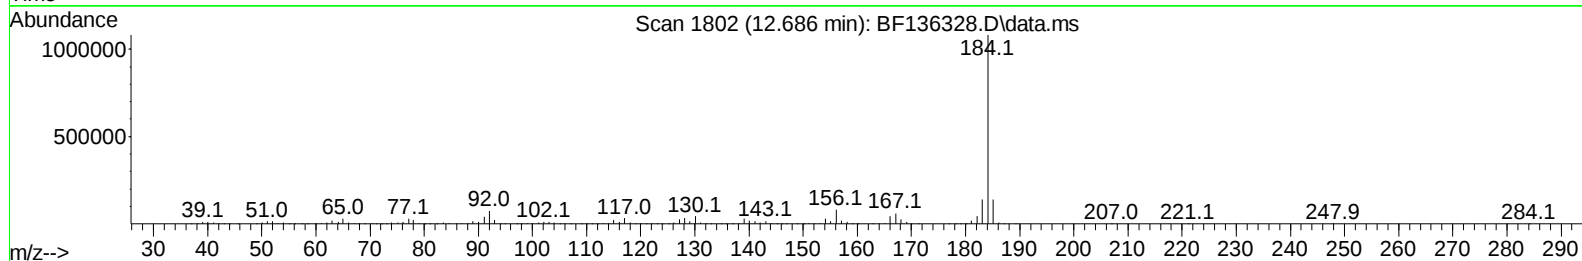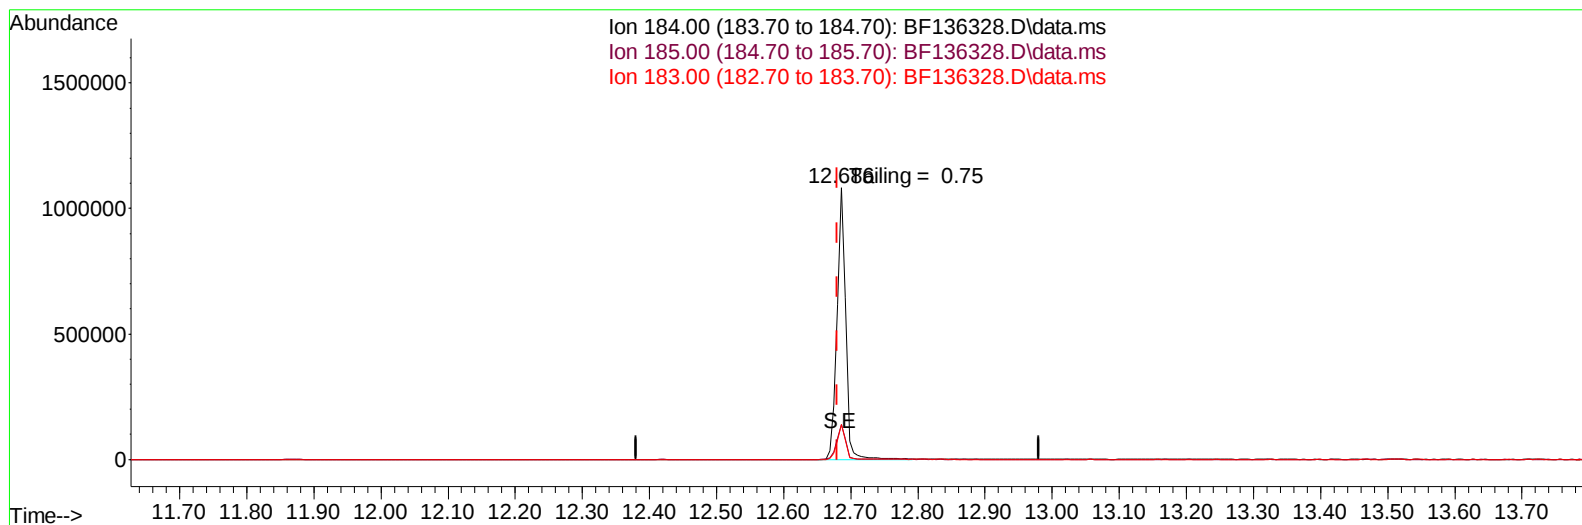

TIC: BF136328.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 45393.79 ng

response 980500

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	12.83
183.00	11.20	12.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2023	BNA_F	<u>BF136328.D</u>
Compound Name	Response	Retention Time
DDT	549222	13.516
DDD	13141	13.21
DDE	1108	12.869
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14249	563471	2.53

Instrument :
BNA_F
ClientSampleId :
DFTPP