


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
 Data File : BF136351.D
 Acq On : 01 Dec 2023 22:56
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 28 03:04:20 2023

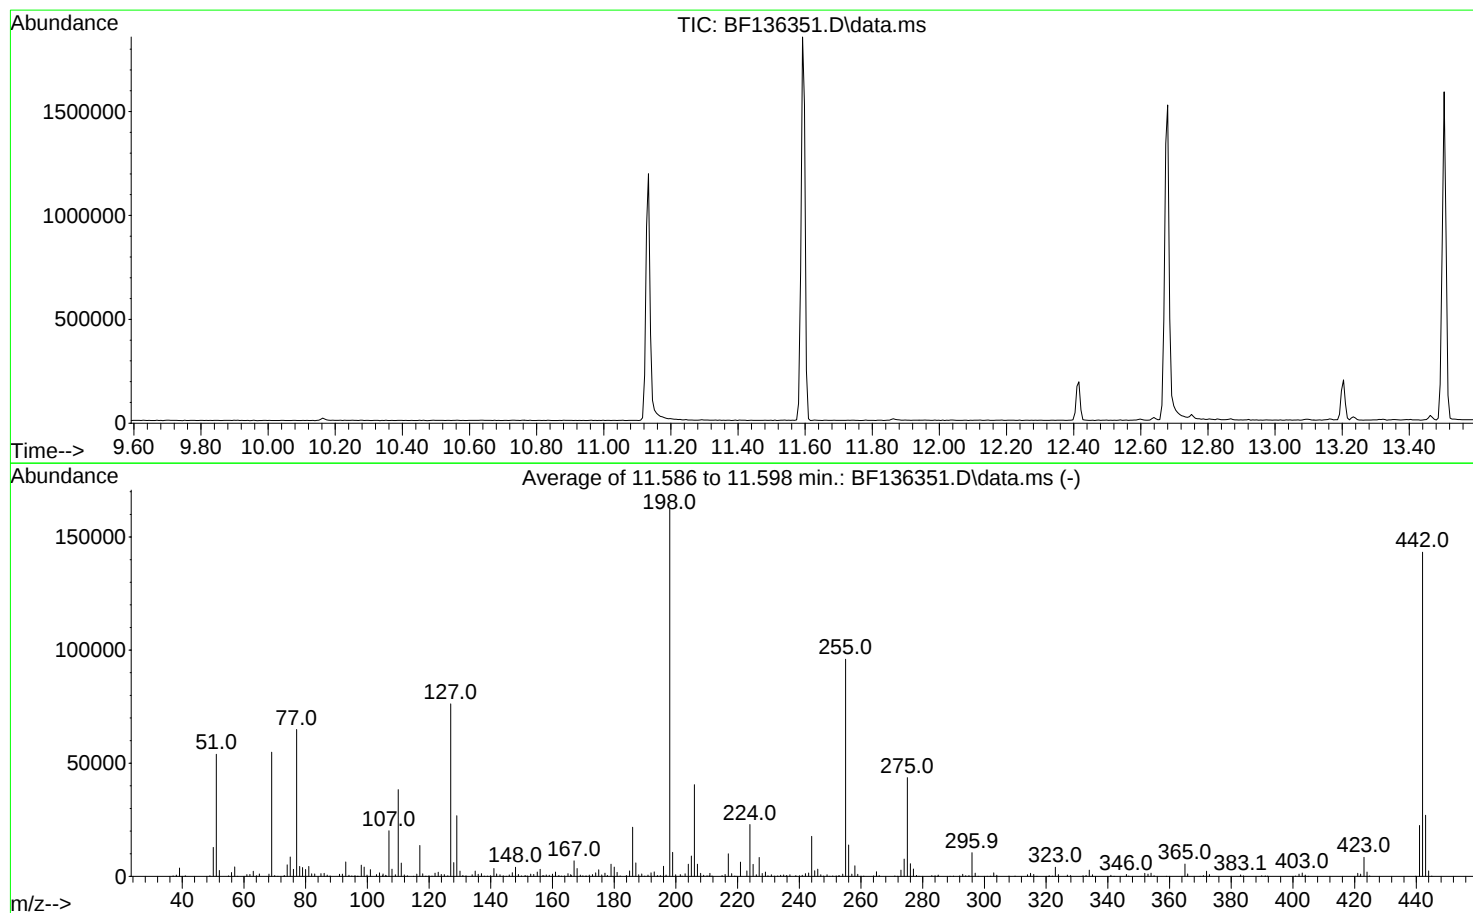




AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	53936	PASS
68	69	0.00	2	1.9	1019	PASS
69	198	0.00	100	33.7	54856	PASS
70	69	0.00	2	0.6	329	PASS
127	198	10	80	46.9	76219	PASS
197	198	0.00	2	0.4	590	PASS
198	198	100	100	100.0	162600	PASS
199	198	5	9	6.5	10611	PASS
275	198	10	60	26.8	43635	PASS
365	198	1	100	3.3	5420	PASS
441	198	0.01	100	13.8	22474	PASS
442	442	50	100	100.0	143261	PASS
443	442	15	24	18.9	27029	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136351.D
Acq On : 01 Dec 2023 22:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 02 01:10:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

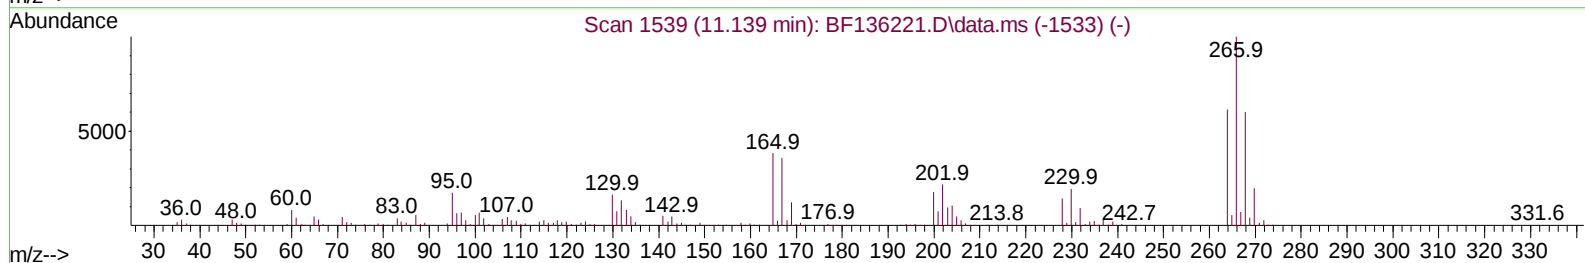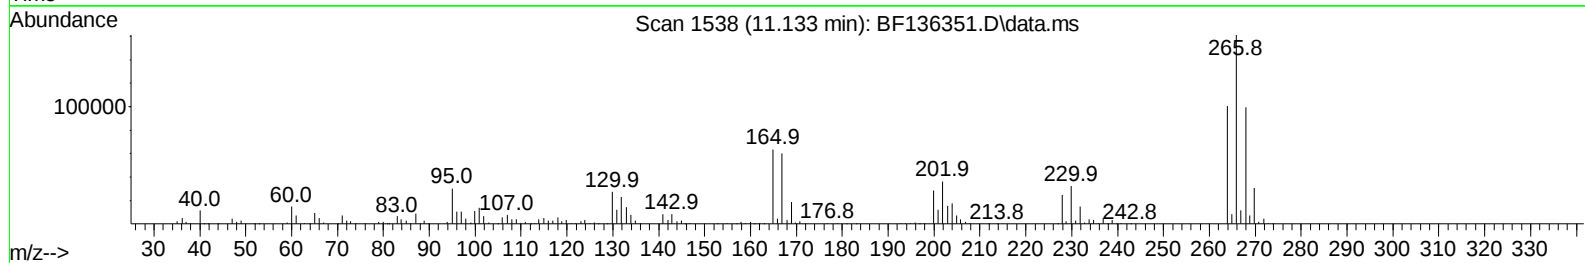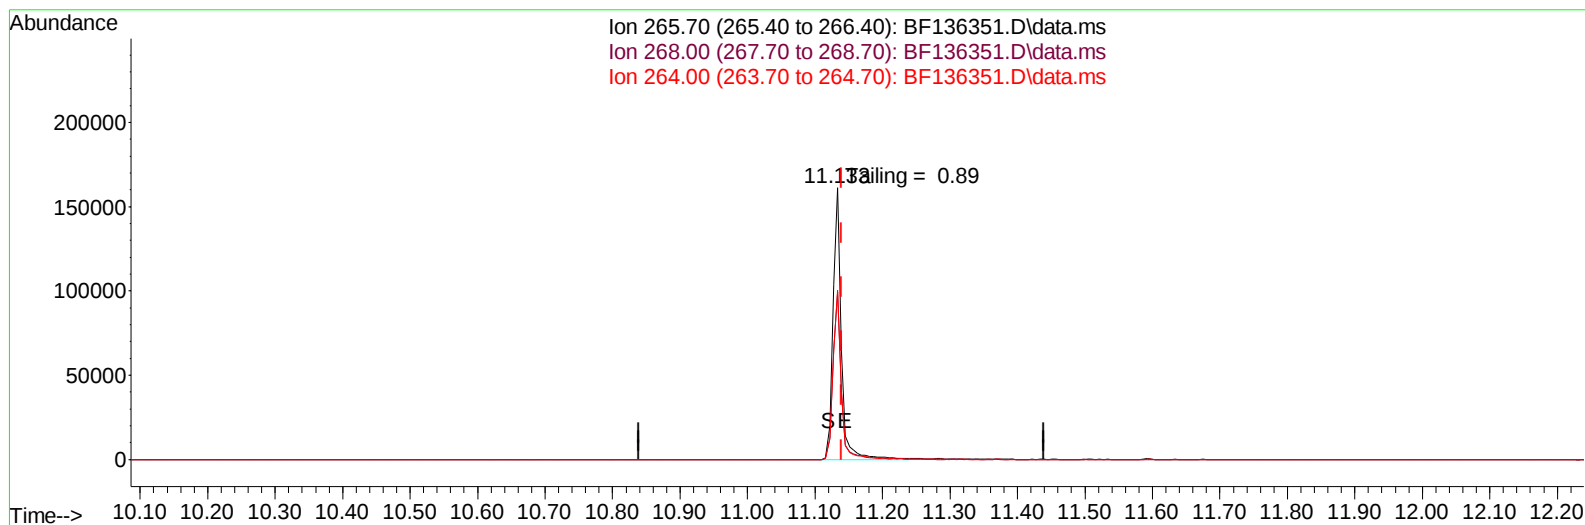

TIC: BF136351.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.006) 32594.53 ng




response 140309

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	61.69
264.00	61.40	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120123\
Data File : BF136351.D
Acq On : 01 Dec 2023 22:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 02 01:10:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 28 03:04:20 2023
Response via : Initial Calibration

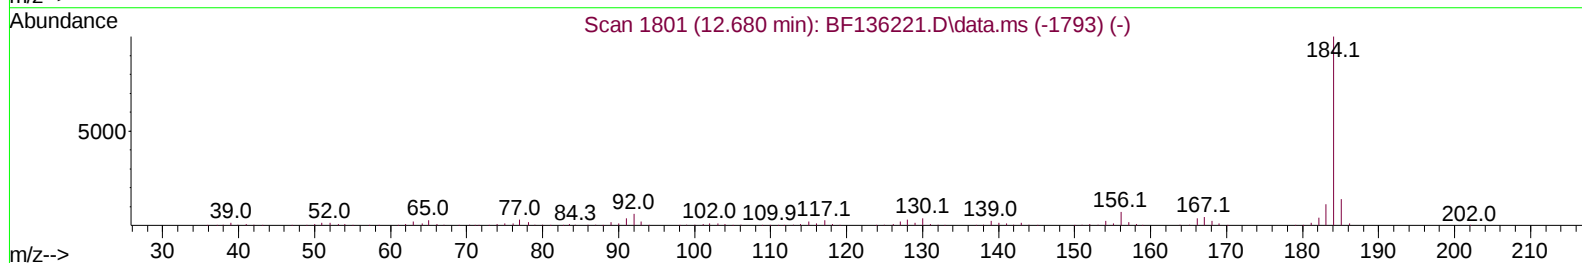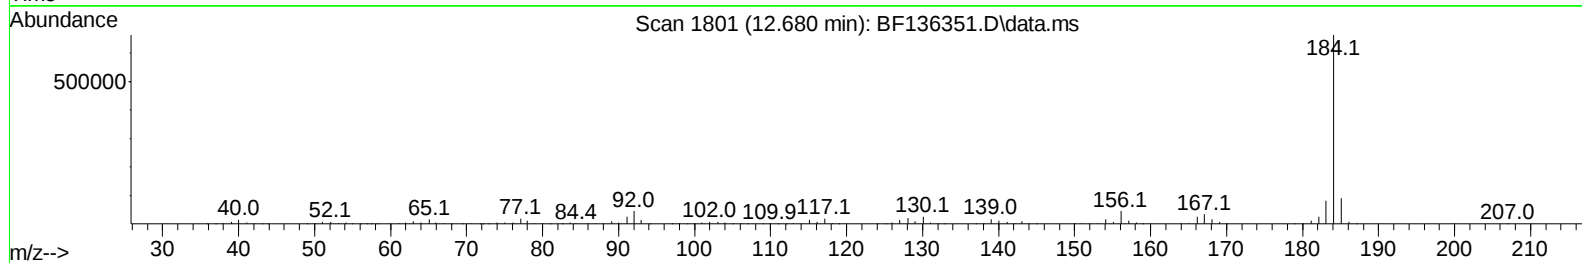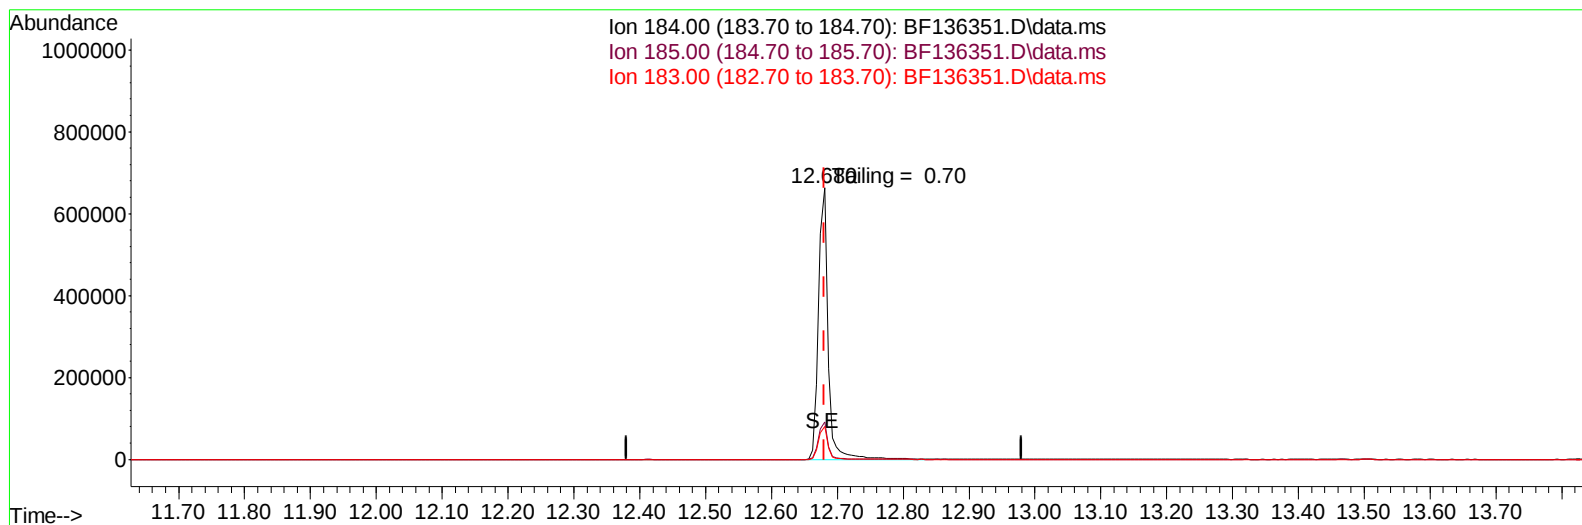

TIC: BF136351.D\data.ms

(77) Benzidine

12.680min (+ 0.000) 161064.62 ng

response 651315

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.74
183.00	11.20	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2023	BNA_F	<u>BF136351.D</u>
Compound Name	Response	Retention Time
DDT	268348	13.504
DDD	36890	13.204
DDE	968	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37858	306206	12.36

Instrument :
BNA_F
ClientSampleId :
DFTPP